

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054015.D
 Acq On : 23 Jun 2022 16:20
 Operator : CG/JU
 Sample : PB145673BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK673

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.490	14	17	24	rVB	4393	6646	0.79%	0.091%
2	3.908	85	88	107	rBV	56981	107395	12.83%	1.469%
3	4.248	143	146	151	rVB3	1619	2466	0.29%	0.034%
4	4.342	160	162	166	rBV4	1271	1299	0.16%	0.018%
5	4.389	168	170	173	rVV2	896	1114	0.13%	0.015%
6	4.448	177	180	181	rVV2	804	846	0.10%	0.012%
7	4.489	183	187	191	rVB4	997	1388	0.17%	0.019%
8	5.206	306	309	311	rVB3	658	843	0.10%	0.012%
9	5.247	311	316	320	rBV3	947	1425	0.17%	0.019%
10	7.227	647	653	664	rVB	77063	139687	16.68%	1.911%
11	7.392	674	681	689	rBV	54832	97421	11.63%	1.332%
12	7.603	710	717	727	rBV	72381	134088	16.01%	1.834%
13	8.073	790	797	804	rBB	56564	98093	11.71%	1.342%
14	8.772	910	916	924	rBV	106276	184788	22.07%	2.527%
15	9.231	987	994	1005	rBV	76519	139161	16.62%	1.903%
16	9.959	1111	1118	1127	rVB	63907	115312	13.77%	1.577%
17	10.500	1203	1210	1223	rVB	106642	199729	23.85%	2.732%
18	10.882	1267	1275	1285	rVB	86128	159872	19.09%	2.187%
19	11.011	1290	1297	1306	rBV	105704	201615	24.08%	2.758%
20	11.076	1306	1308	1312	rVB2	829	898	0.11%	0.012%
21	12.456	1540	1543	1544	rBV	936	871	0.10%	0.012%
22	12.468	1544	1545	1550	rVB	1514	1422	0.17%	0.019%
23	14.101	1816	1823	1829	rBV	229559	350455	41.85%	4.793%
24	14.395	1866	1873	1880	rBV	236571	397274	47.44%	5.434%
25	14.701	1917	1925	1932	rBV	171793	273622	32.68%	3.742%
26	14.883	1951	1956	1974	rBV	82788	147908	17.66%	2.023%
27	15.688	2086	2093	2102	rVB	342603	549067	65.57%	7.510%
28	15.799	2107	2112	2121	rBV	87713	139363	16.64%	1.906%
29	15.935	2130	2135	2140	rVB3	3251	5027	0.60%	0.069%
30	16.469	2224	2226	2230	rVB2	845	1101	0.13%	0.015%
31	16.710	2264	2267	2270	rVB	784	1018	0.12%	0.014%
32	17.116	2333	2336	2341	rVB2	768	1074	0.13%	0.015%
33	17.186	2345	2348	2352	rVB2	588	1036	0.12%	0.014%
34	17.239	2352	2357	2360	rBV4	815	1640	0.20%	0.022%
35	17.445	2385	2392	2401	rVB	243211	374470	44.72%	5.122%
36	17.544	2401	2409	2416	rBV	388020	633566	75.66%	8.665%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054015.D
 Acq On : 23 Jun 2022 16:20
 Operator : CG/JU
 Sample : PB145673BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK673

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	18.743	2610	2613	2617	rVB2	891	1235	0.15%	0.017%
38	18.925	2641	2644	2645	rBV2	886	990	0.12%	0.014%
39	19.096	2670	2673	2677	rBV2	1203	1807	0.22%	0.025%
40	19.295	2704	2707	2710	rVB4	639	872	0.10%	0.012%
41	19.389	2720	2723	2728	rVB3	5528	7807	0.93%	0.107%
42	19.466	2731	2736	2743	rVB	5016	7465	0.89%	0.102%
43	19.666	2765	2770	2774	rVB4	682	1386	0.17%	0.019%
44	19.824	2791	2797	2804	rBV	566473	837344	100.00%	11.453%
45	19.971	2820	2822	2824	rBV3	951	986	0.12%	0.013%
46	20.100	2842	2844	2846	rVB2	1093	847	0.10%	0.012%
47	20.206	2858	2862	2863	rBV3	1260	1924	0.23%	0.026%
48	20.341	2882	2885	2886	rBV	743	991	0.12%	0.014%
49	20.476	2904	2908	2909	rBV3	883	924	0.11%	0.013%
50	20.706	2944	2947	2948	rBV3	1707	1846	0.22%	0.025%
51	20.852	2970	2972	2976	rBV4	2134	2701	0.32%	0.037%
52	21.317	3045	3051	3056	rBV3	8926	18749	2.24%	0.256%
53	21.375	3056	3061	3066	rVV	14942	24145	2.88%	0.330%
54	21.434	3066	3071	3081	rVV	80568	124530	14.87%	1.703%
55	21.716	3112	3119	3127	rBV	277827	468223	55.92%	6.404%
56	21.863	3143	3144	3146	rBV2	1655	1461	0.17%	0.020%
57	21.916	3149	3153	3157	rVB6	3271	5332	0.64%	0.073%
58	21.951	3157	3159	3161	rBV2	1848	1418	0.17%	0.019%
59	23.244	3374	3379	3384	rVB8	4071	9208	1.10%	0.126%
60	24.055	3512	3517	3522	rVB6	5912	13194	1.58%	0.180%
61	24.754	3624	3636	3651	rBV3	267512	828118	98.90%	11.326%
62	24.983	3663	3675	3689	rVB	141459	461622	55.13%	6.314%
63	25.241	3717	3719	3720	rBV	1546	1094	0.13%	0.015%
64	25.611	3780	3782	3786	rBV5	2162	2016	0.24%	0.028%
65	25.782	3809	3811	3812	rBV2	2876	1902	0.23%	0.026%
66	26.928	4005	4006	4008	rVB2	2211	1049	0.13%	0.014%
67	28.461	4265	4267	4270	rBV2	1658	1262	0.15%	0.017%
68	28.872	4335	4337	4339	rVB2	1774	1125	0.13%	0.015%
69	28.978	4353	4355	4356	rBV	1604	998	0.12%	0.014%
70	30.717	4647	4651	4652	rBV3	2038	2594	0.31%	0.035%
71	31.575	4795	4797	4800	rVB4	2416	1280	0.15%	0.018%




Sum of corrected areas: 7311445

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054015.D
Acq On : 23 Jun 2022 16:20
Operator : CG/JU
Sample : PB145673BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK673

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

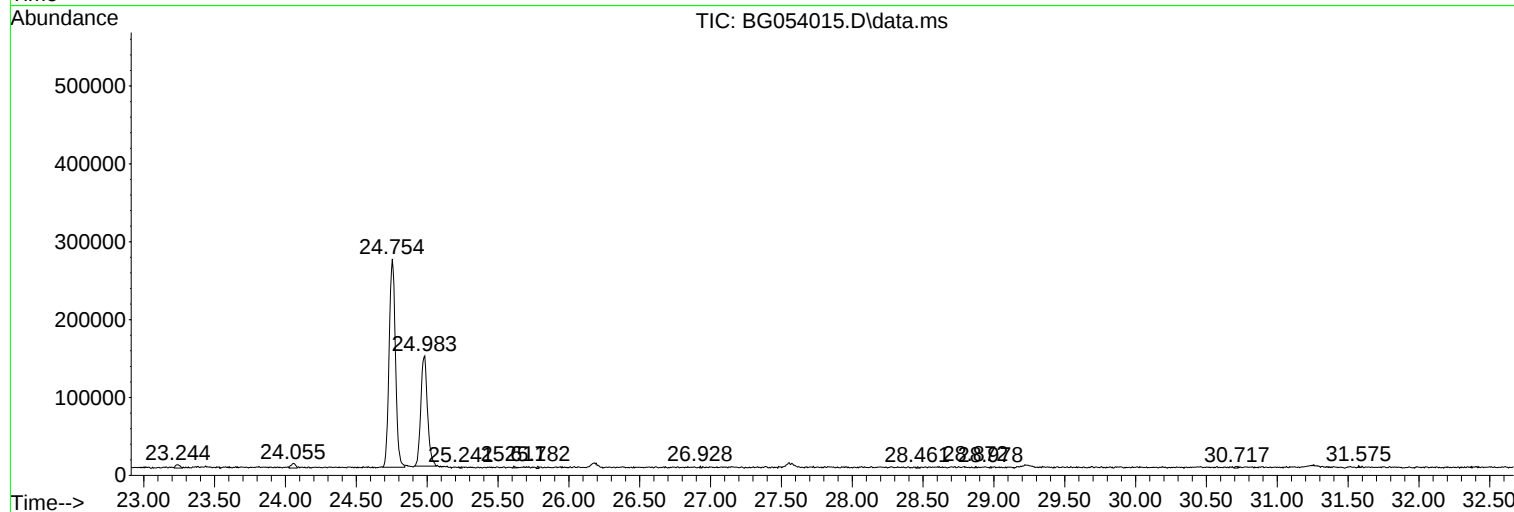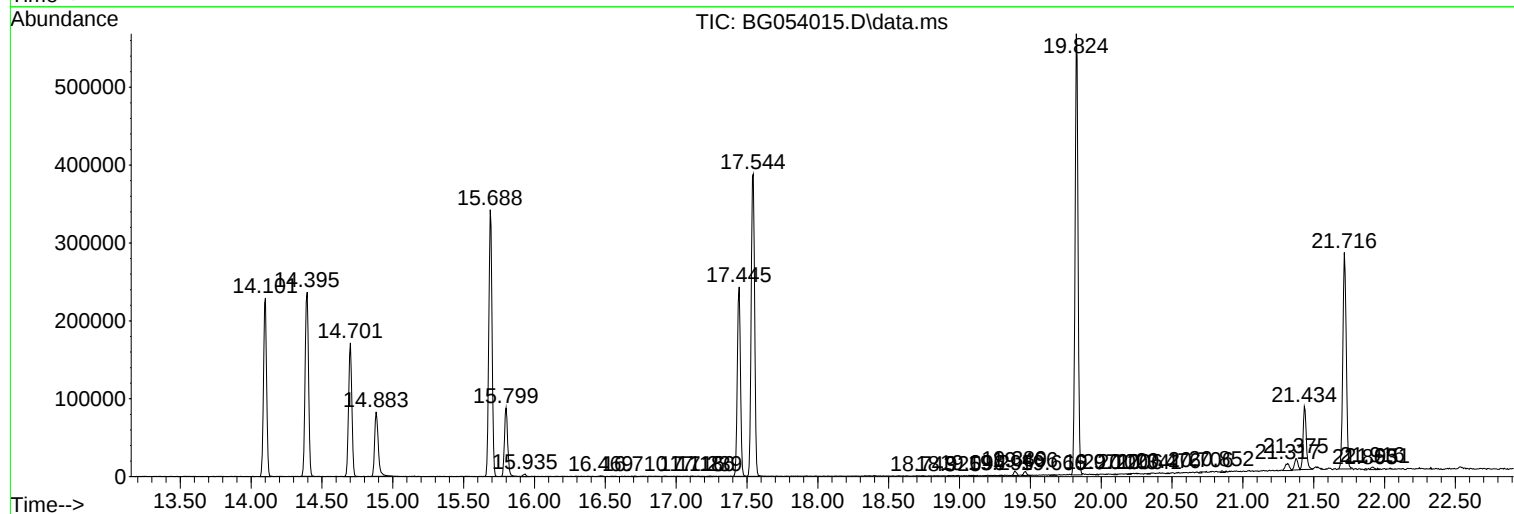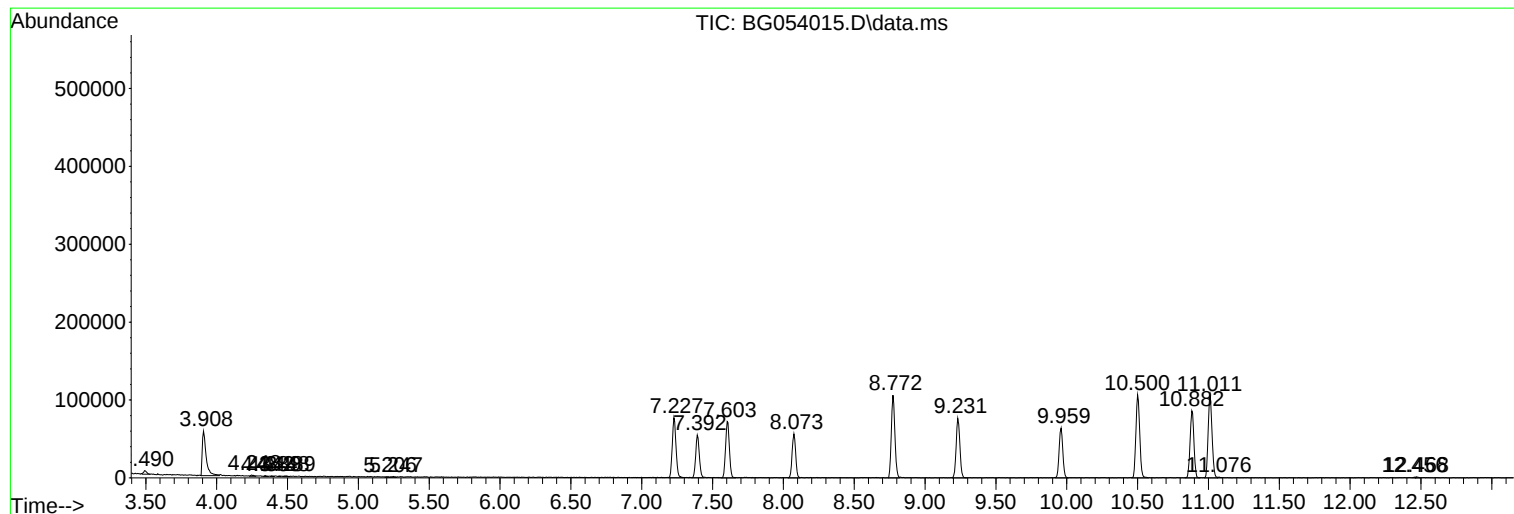

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054015.D
Acq On : 23 Jun 2022 16:20
Operator : CG/JU
Sample : PB145673BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK673

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054015.D
Acq On : 23 Jun 2022 16:20
Operator : CG/JU
Sample : PB145673BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK673

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------