

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054017.D
 Acq On : 23 Jun 2022 17:38
 Operator : CG/JU
 Sample : N3355-21
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EY0C8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054017.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.471	9	14	25	rVB3	16963	36978	3.72%	0.488%
2	3.700	49	53	54	rBV2	1153	1166	0.12%	0.015%
3	3.918	86	90	96	rBV	15460	27673	2.78%	0.365%
4	4.141	126	128	130	rBV2	1229	1468	0.15%	0.019%
5	4.793	236	239	241	rBV2	809	1057	0.11%	0.014%
6	6.062	454	455	459	rVB3	994	1016	0.10%	0.013%
7	7.232	649	654	660	rBV2	13238	24075	2.42%	0.318%
8	7.390	676	681	691	rBV	55987	100768	10.13%	1.330%
9	7.608	710	718	728	rBV	56751	100577	10.11%	1.328%
10	8.072	790	797	804	rVB	55996	100516	10.10%	1.327%
11	8.771	910	916	924	rBV2	46949	84822	8.53%	1.120%
12	9.235	987	995	1004	rVV	80784	151357	15.21%	1.998%
13	9.664	1067	1068	1071	rBV2	1073	1164	0.12%	0.015%
14	9.958	1111	1118	1126	rVB2	65781	118967	11.96%	1.571%
15	10.498	1203	1210	1220	rBV2	104198	192078	19.31%	2.536%
16	10.880	1266	1275	1284	rBB	90180	166664	16.75%	2.200%
17	11.010	1289	1297	1308	rBV	97393	184770	18.57%	2.440%
18	12.467	1541	1545	1550	rBB3	1626	2927	0.29%	0.039%
19	14.094	1815	1822	1832	rBV	253973	398899	40.10%	5.267%
20	14.388	1865	1872	1880	rBV	268437	451622	45.40%	5.963%
21	14.699	1918	1925	1932	rBV	173049	283212	28.47%	3.739%
22	14.887	1952	1957	1970	rVB2	11107	20578	2.07%	0.272%
23	15.686	2085	2093	2102	rVB	410771	640135	64.35%	8.452%
24	15.798	2106	2112	2120	rBV	109636	164377	16.52%	2.170%
25	15.927	2130	2134	2138	rVB3	3131	4539	0.46%	0.060%
26	16.468	2224	2226	2231	rVB3	1629	2273	0.23%	0.030%
27	17.232	2353	2356	2359	rBV	800	1041	0.10%	0.014%
28	17.443	2384	2392	2399	rBV	247681	384632	38.66%	5.078%
29	17.537	2401	2408	2416	rBV	483950	769341	77.33%	10.158%
30	18.330	2540	2543	2548	rBV3	3938	7081	0.71%	0.093%
31	18.401	2554	2555	2558	rVB	1902	1312	0.13%	0.017%
32	18.607	2587	2590	2594	rBV2	617	1114	0.11%	0.015%
33	19.388	2719	2723	2728	rBV2	6777	9991	1.00%	0.132%
34	19.458	2731	2735	2740	rBV2	6555	8986	0.90%	0.119%
35	19.599	2757	2759	2765	rBV3	2169	4516	0.45%	0.060%
36	19.741	2781	2783	2787	rBV3	1151	1620	0.16%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054017.D
 Acq On : 23 Jun 2022 17:38
 Operator : CG/JU
 Sample : N3355-21
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EY0C8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.823	2790	2797	2805	rBV	649138	993467	99.86%	13.117%
38	19.917	2811	2813	2816	rBV4	811	1006	0.10%	0.013%
39	19.952	2816	2819	2822	rVB4	920	1103	0.11%	0.015%
40	20.722	2948	2950	2952	rBV2	1284	1018	0.10%	0.013%
41	20.786	2958	2961	2963	rBV4	1320	1680	0.17%	0.022%
42	21.027	2999	3002	3003	rBV3	1193	1414	0.14%	0.019%
43	21.062	3006	3008	3011	rBV4	1305	1154	0.12%	0.015%
44	21.151	3022	3023	3026	rBV2	1148	1317	0.13%	0.017%
45	21.292	3045	3047	3048	rBV2	1759	1409	0.14%	0.019%
46	21.356	3054	3058	3067	rBV5	12045	25402	2.55%	0.335%
47	21.439	3067	3072	3081	rVB	22978	41858	4.21%	0.553%
48	21.515	3083	3085	3087	rBV3	1655	1485	0.15%	0.020%
49	21.656	3108	3109	3112	rBV3	1747	1546	0.16%	0.020%
50	21.715	3112	3119	3127	rVV2	276814	475953	47.84%	6.284%
51	22.525	3255	3257	3261	rVB5	2932	3455	0.35%	0.046%
52	22.778	3298	3300	3305	rBV5	1559	1682	0.17%	0.022%
53	22.996	3335	3337	3339	rVB3	1767	1109	0.11%	0.015%
54	23.236	3375	3378	3382	rVB4	5018	6852	0.69%	0.090%
55	23.330	3392	3394	3395	rVB2	1814	1178	0.12%	0.016%
56	23.348	3395	3397	3398	rBV2	1754	1141	0.11%	0.015%
57	24.053	3513	3517	3524	rVB5	7835	17351	1.74%	0.229%
58	24.752	3624	3636	3649	rBV	340705	994825	100.00%	13.135%
59	24.970	3662	3673	3694	rVB2	152074	479932	48.24%	6.337%
60	25.581	3774	3777	3781	rBV6	1954	3290	0.33%	0.043%
61	26.168	3872	3877	3892	rVB7	9014	25710	2.58%	0.339%
62	26.480	3928	3930	3934	rVB4	2128	1954	0.20%	0.026%
63	26.650	3957	3959	3963	rBV4	1563	1130	0.11%	0.015%
64	27.555	4107	4113	4123	rVB10	6175	18156	1.83%	0.240%
65	28.142	4211	4213	4215	rBV3	1909	1525	0.15%	0.020%
66	28.513	4274	4276	4279	rVB4	1741	1123	0.11%	0.015%
67	29.212	4393	4395	4398	rBV4	2879	3668	0.37%	0.048%
68	30.516	4616	4617	4619	rBV2	2227	1373	0.14%	0.018%
69	31.444	4774	4775	4777	rVB	2242	1056	0.11%	0.014%
70	31.627	4804	4806	4808	rBV2	1736	1324	0.13%	0.017%
71	31.944	4858	4860	4862	rBV2	1788	1919	0.19%	0.025%
72	32.349	4927	4929	4930	rBV2	1731	1186	0.12%	0.016%




Sum of corrected areas: 7574063

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054017.D
Acq On : 23 Jun 2022 17:38
Operator : CG/JU
Sample : N3355-21
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EY0C8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

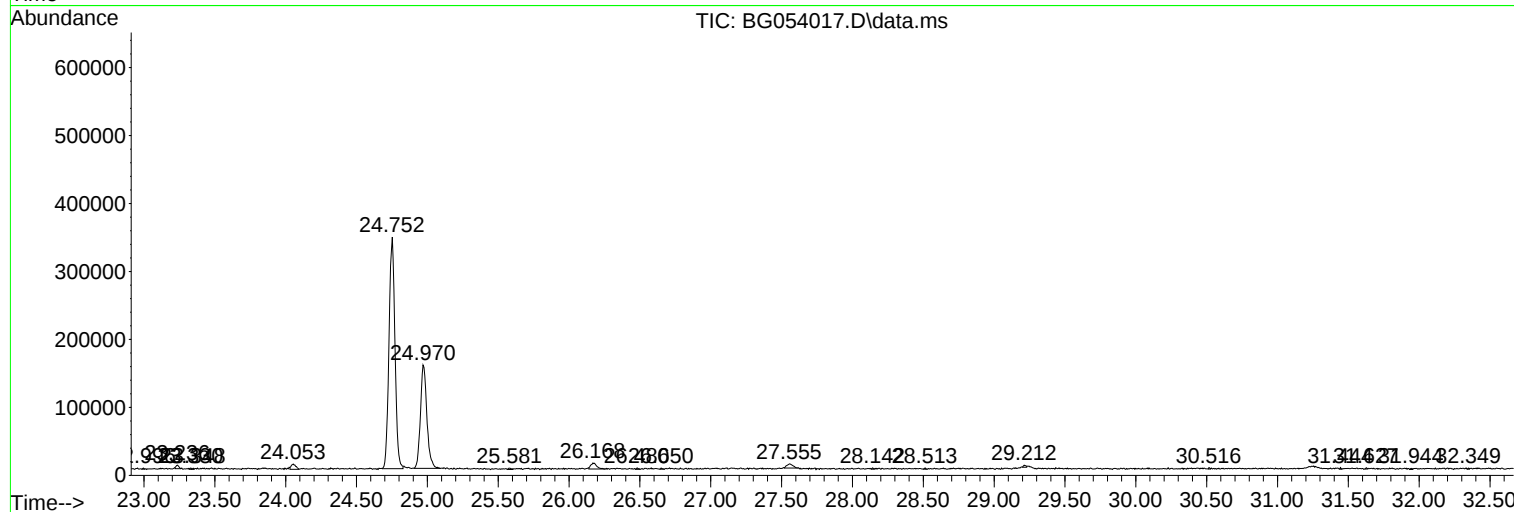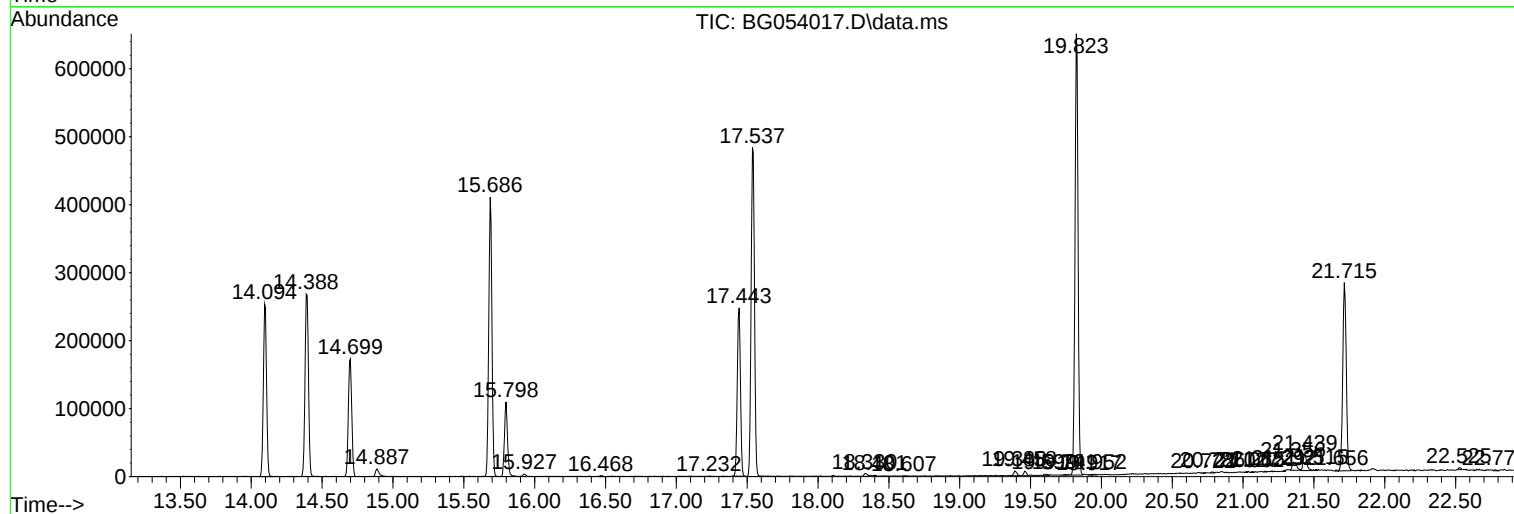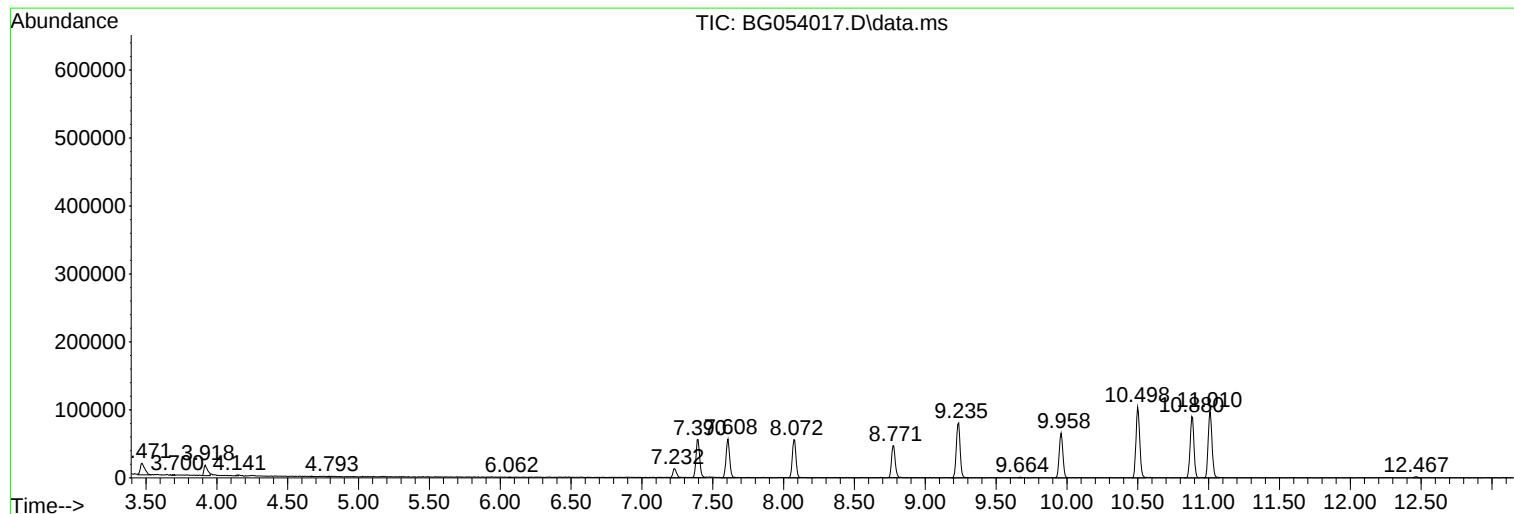

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054017.D
Acq On : 23 Jun 2022 17:38
Operator : CG/JU
Sample : N3355-21
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EY0C8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054017.D
Acq On : 23 Jun 2022 17:38
Operator : CG/JU
Sample : N3355-21
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EY0C8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------