

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054019.D
 Acq On : 23 Jun 2022 18:56
 Operator : CG/JU
 Sample : N3371-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 VNJ-211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.493	15	18	20	rBV3	3147	3213	0.19%	0.029%
2	3.910	85	89	101	rBV	32593	60783	3.55%	0.542%
3	4.151	126	130	134	rBV3	1865	3259	0.19%	0.029%
4	4.251	143	147	152	rVB5	2306	3477	0.20%	0.031%
5	7.230	647	654	663	rBV	65524	117034	6.84%	1.044%
6	7.395	675	682	691	rBV	100642	180158	10.53%	1.607%
7	7.465	691	694	697	rVB3	1424	1822	0.11%	0.016%
8	7.606	712	718	726	rVB	56862	105124	6.14%	0.938%
9	8.076	791	798	805	rBV	60869	106591	6.23%	0.951%
10	8.775	909	917	924	rBV	88755	157377	9.20%	1.404%
11	9.234	987	995	1003	rBV	143069	265896	15.54%	2.372%
12	9.956	1111	1118	1127	rVB2	51971	96828	5.66%	0.864%
13	10.497	1202	1210	1221	rBV	91155	172803	10.10%	1.542%
14	10.885	1268	1276	1282	rBV	92980	180308	10.54%	1.609%
15	11.008	1290	1297	1306	rBV	198557	376987	22.04%	3.363%
16	12.465	1541	1545	1549	rVB	1444	2035	0.12%	0.018%
17	14.098	1815	1823	1833	rBV	447560	662806	38.74%	5.914%
18	14.392	1864	1873	1883	rBV	475544	766004	44.77%	6.834%
19	14.698	1918	1925	1932	rBV	189574	310788	18.17%	2.773%
20	14.886	1950	1957	1967	rBV	63875	116812	6.83%	1.042%
21	14.956	1967	1969	1975	rVB2	1558	2294	0.13%	0.020%
22	15.432	2044	2050	2054	rBV3	2395	3710	0.22%	0.033%
23	15.691	2086	2094	2101	rBV	673582	1057468	61.81%	9.435%
24	15.796	2106	2112	2118	rBV	76805	114479	6.69%	1.021%
25	15.926	2129	2134	2139	rVB	6557	8917	0.52%	0.080%
26	16.472	2221	2227	2232	rBV2	2626	3853	0.23%	0.034%
27	17.442	2385	2392	2399	rBV	270057	429526	25.11%	3.832%
28	17.541	2401	2409	2418	rVB	830633	1284045	75.05%	11.456%
29	17.718	2434	2439	2442	rVB	1901	2965	0.17%	0.026%
30	18.335	2539	2544	2546	rBV2	1421	1728	0.10%	0.015%
31	18.399	2551	2555	2558	rVB2	1533	1890	0.11%	0.017%
32	19.392	2719	2724	2730	rBV2	7715	11995	0.70%	0.107%
33	19.457	2730	2735	2740	rBV	7468	11017	0.64%	0.098%
34	19.715	2772	2779	2783	rBV3	3729	6531	0.38%	0.058%
35	19.827	2791	2798	2805	rBV	1088819	1645490	96.18%	14.681%
36	20.426	2896	2900	2905	rBV4	1138	2216	0.13%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054019.D
 Acq On : 23 Jun 2022 18:56
 Operator : CG/JU
 Sample : N3371-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 VNJ-211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	21.314	3046	3051	3054	rBV5	3075	5696	0.33%	0.051%
38	21.355	3054	3058	3066	rVV6	11845	26424	1.54%	0.236%
39	21.437	3067	3072	3080	rVB	24572	39330	2.30%	0.351%
40	21.713	3112	3119	3129	rBV2	314042	533524	31.19%	4.760%
41	21.919	3150	3154	3156	rBV3	2806	2869	0.17%	0.026%
42	22.377	3230	3232	3236	rBV4	1913	1835	0.11%	0.016%
43	22.536	3255	3259	3264	rBV7	3020	4737	0.28%	0.042%
44	23.147	3361	3363	3366	rBV4	1763	2445	0.14%	0.022%
45	23.241	3374	3379	3383	rVB6	4187	7531	0.44%	0.067%
46	23.493	3418	3422	3424	rBV5	2233	2320	0.14%	0.021%
47	24.051	3512	3517	3522	rBV4	6446	10203	0.60%	0.091%
48	24.398	3575	3576	3580	rBV4	1953	2579	0.15%	0.023%
49	24.757	3624	3637	3655	rBV2	583292	1710832	100.00%	15.264%
50	24.974	3661	3674	3690	rBV2	171038	544646	31.84%	4.859%
51	26.167	3871	3877	3888	rVB7	7973	22798	1.33%	0.203%
52	26.578	3945	3947	3950	rBV4	2083	2435	0.14%	0.022%
53	27.718	4139	4141	4145	rBV4	1793	1893	0.11%	0.017%
54	29.022	4361	4363	4367	rBV5	1608	2015	0.12%	0.018%
55	30.062	4538	4540	4544	rBV4	1523	1766	0.10%	0.016%
56	31.149	4723	4725	4727	rBV3	1937	1823	0.11%	0.016%
57	32.260	4912	4914	4918	rBV5	1783	2422	0.14%	0.022%




Sum of corrected areas: 11208352

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054019.D
Acq On : 23 Jun 2022 18:56
Operator : CG/JU
Sample : N3371-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VNJ-211

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

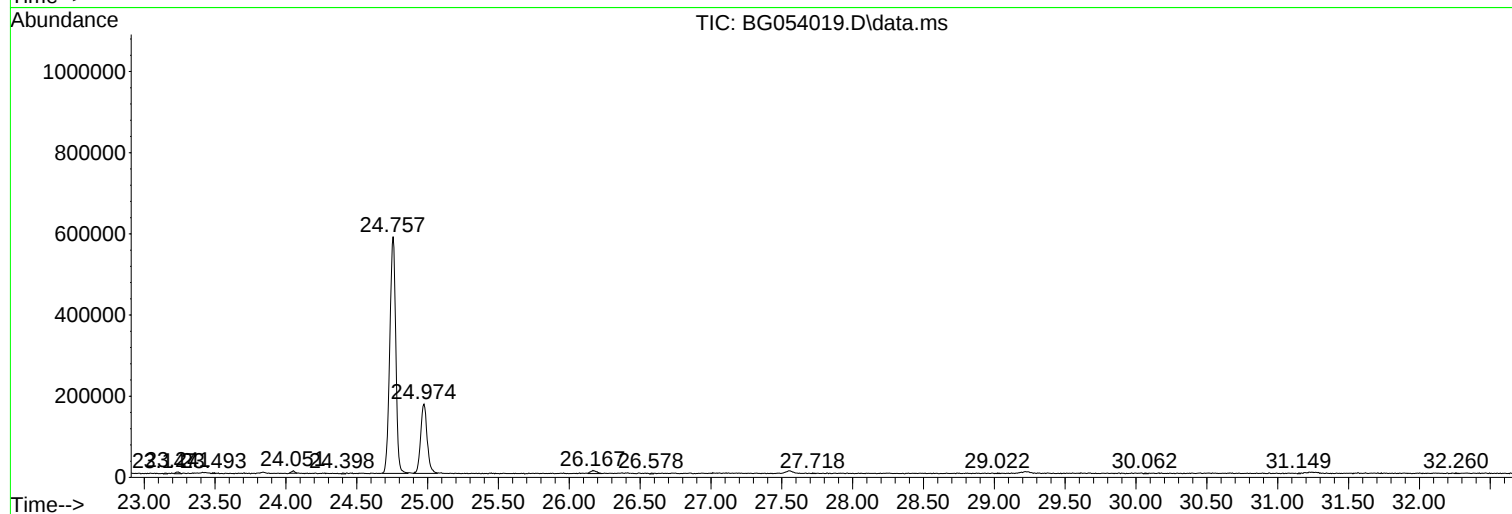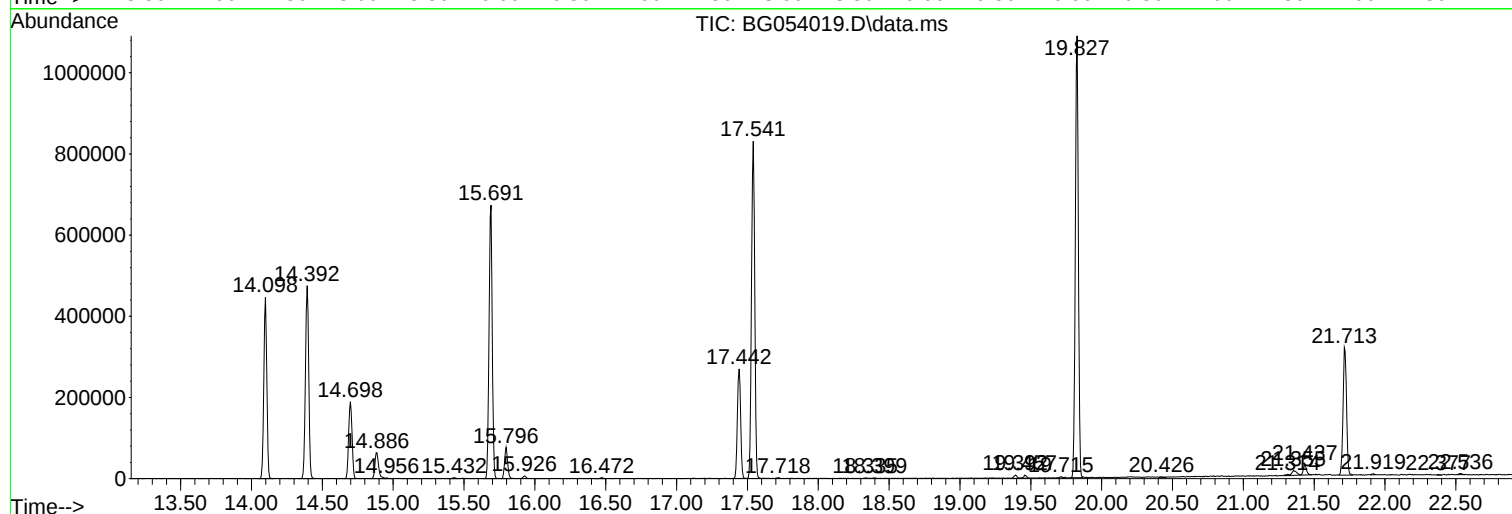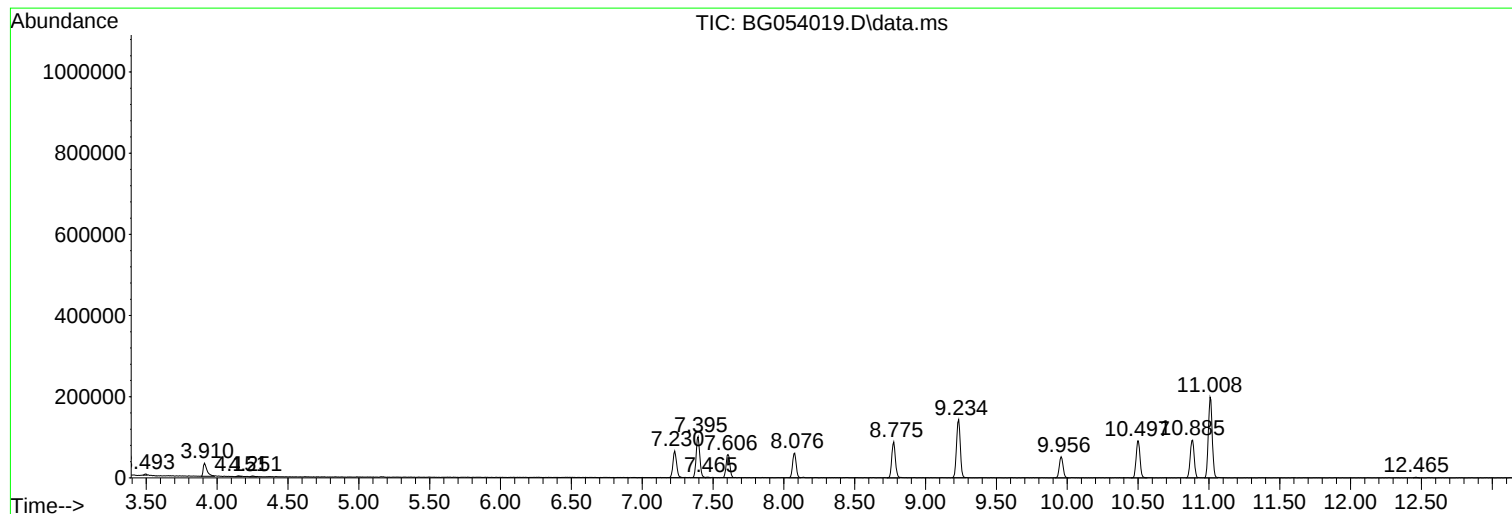

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054019.D
Acq On : 23 Jun 2022 18:56
Operator : CG/JU
Sample : N3371-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VNJ-211

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054019.D
Acq On : 23 Jun 2022 18:56
Operator : CG/JU
Sample : N3371-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VNJ-211

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc