

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054021.D
 Acq On : 23 Jun 2022 20:14
 Operator : CG/JU
 Sample : N3400-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.494	14	18	23	rVB3	4319	6703	0.68%	0.085%
2	3.876	79	83	86	rBV4	904	1156	0.12%	0.015%
3	3.917	86	90	98	rBV	13611	24252	2.45%	0.307%
4	4.141	126	128	129	rBV2	1613	1046	0.11%	0.013%
5	4.158	129	131	135	rVB2	1972	1704	0.17%	0.022%
6	5.163	298	302	306	rVB3	1028	1374	0.14%	0.017%
7	7.231	648	654	662	rVB2	21082	36696	3.71%	0.465%
8	7.396	674	682	691	rBV	58728	104768	10.59%	1.326%
9	7.607	711	718	728	rVB	65422	117502	11.88%	1.487%
10	8.077	791	798	806	rVB	60666	110087	11.13%	1.394%
11	8.770	909	916	927	rVB	62277	114014	11.53%	1.443%
12	9.229	987	994	1004	rBV	83369	157821	15.96%	1.998%
13	9.957	1110	1118	1127	rVB2	66596	127211	12.86%	1.610%
14	10.498	1203	1210	1221	rBV	110953	210159	21.25%	2.660%
15	10.880	1266	1275	1283	rBV	102660	188959	19.11%	2.392%
16	11.009	1290	1297	1309	rBV	92209	174201	17.61%	2.205%
17	12.466	1540	1545	1549	rBV2	1917	2743	0.28%	0.035%
18	14.099	1816	1823	1831	rVB	266451	405137	40.97%	5.129%
19	14.393	1866	1873	1882	rVB	277629	449384	45.44%	5.689%
20	14.699	1918	1925	1934	rVB	191925	317292	32.08%	4.017%
21	14.881	1952	1956	1963	rBV2	18226	33059	3.34%	0.418%
22	14.934	1963	1965	1969	rVB3	1504	1811	0.18%	0.023%
23	15.492	2058	2060	2065	rBV3	799	1200	0.12%	0.015%
24	15.686	2086	2093	2101	rBV	408084	644617	65.18%	8.160%
25	15.797	2106	2112	2121	rBV	116845	174808	17.68%	2.213%
26	15.927	2130	2134	2138	rVB	3753	5279	0.53%	0.067%
27	16.467	2221	2226	2231	rVV3	1539	1849	0.19%	0.023%
28	17.443	2383	2392	2399	rBV	275023	431345	43.62%	5.460%
29	17.542	2402	2409	2419	rVB	471523	760338	76.88%	9.625%
30	18.107	2501	2505	2511	rVB	8523	10465	1.06%	0.132%
31	18.330	2540	2543	2550	rBV2	4504	7110	0.72%	0.090%
32	18.400	2553	2555	2560	rVB	1517	1471	0.15%	0.019%
33	19.393	2718	2724	2730	rVB	7121	10732	1.09%	0.136%
34	19.458	2730	2735	2741	rBV	6333	10988	1.11%	0.139%
35	19.605	2756	2760	2763	rVV4	2762	4027	0.41%	0.051%
36	19.628	2763	2764	2769	rVV3	1248	1583	0.16%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054021.D
 Acq On : 23 Jun 2022 20:14
 Operator : CG/JU
 Sample : N3400-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COAFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.740	2781	2783	2788	rBV4	1176	1525	0.15%	0.019%
38	19.822	2790	2797	2807	rBV	634569	988961	100.00%	12.519%
39	20.128	2848	2849	2852	rBV3	908	1109	0.11%	0.014%
40	20.357	2883	2888	2890	rVV4	1600	1980	0.20%	0.025%
41	20.668	2938	2941	2942	rBV2	1607	1324	0.13%	0.017%
42	20.745	2951	2954	2955	rBV3	1294	1146	0.12%	0.015%
43	20.815	2964	2966	2968	rBV2	1001	1019	0.10%	0.013%
44	20.962	2987	2991	2996	rVB6	1705	3028	0.31%	0.038%
45	21.326	3050	3053	3054	rBV3	1484	1674	0.17%	0.021%
46	21.350	3054	3057	3067	rVV9	8798	20938	2.12%	0.265%
47	21.438	3067	3072	3081	rVB	18403	32099	3.25%	0.406%
48	21.514	3081	3085	3087	rBV5	1758	2056	0.21%	0.026%
49	21.714	3112	3119	3132	rVB	314713	535213	54.12%	6.775%
50	21.867	3144	3145	3147	rBV2	1835	1403	0.14%	0.018%
51	21.920	3150	3154	3161	rVB6	3347	5281	0.53%	0.067%
52	22.243	3207	3209	3211	rVB3	1894	1756	0.18%	0.022%
53	22.266	3211	3213	3214	rBV	1984	1399	0.14%	0.018%
54	22.531	3254	3258	3263	rVB6	4154	7036	0.71%	0.089%
55	23.230	3374	3377	3383	rVB5	5376	9387	0.95%	0.119%
56	23.488	3420	3421	3423	rBV2	1918	1335	0.13%	0.017%
57	23.624	3442	3444	3447	rVB2	1686	1425	0.14%	0.018%
58	23.747	3463	3465	3466	rBV2	1944	1589	0.16%	0.020%
59	23.917	3492	3494	3495	rBV2	1427	1207	0.12%	0.015%
60	24.052	3512	3517	3524	rVB6	9544	20836	2.11%	0.264%
61	24.746	3625	3635	3650	rBV2	334330	985229	99.62%	12.472%
62	24.975	3663	3674	3692	rVB	178864	552248	55.84%	6.991%
63	25.410	3746	3748	3750	rBV3	1556	1215	0.12%	0.015%
64	26.021	3848	3852	3853	rBV4	1601	2006	0.20%	0.025%
65	26.168	3870	3877	3889	rVB4	10526	29277	2.96%	0.371%
66	26.356	3907	3909	3912	rVB3	2428	2029	0.21%	0.026%
67	26.585	3946	3948	3950	rBV3	1730	1411	0.14%	0.018%
68	26.908	4001	4003	4005	rBV3	1638	1673	0.17%	0.021%
69	27.554	4105	4113	4115	rBV8	6749	15862	1.60%	0.201%
70	29.182	4388	4390	4391	rBV2	1943	1110	0.11%	0.014%
71	30.028	4532	4534	4536	rBV3	1747	1496	0.15%	0.019%
72	30.198	4561	4563	4565	rBV2	1831	1483	0.15%	0.019%
73	31.197	4731	4733	4734	rBV	2473	1867	0.19%	0.024%
74	31.432	4771	4773	4775	rVB3	1614	1097	0.11%	0.014%
75	32.155	4894	4896	4899	rVB4	1959	1824	0.18%	0.023%
76	32.184	4899	4901	4904	rBV4	1497	2120	0.21%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054021.D
Acq On : 23 Jun 2022 20:14
Operator : CG/JU
Sample : N3400-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 7899564

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054021.D
Acq On : 23 Jun 2022 20:14
Operator : CG/JU
Sample : N3400-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AFO

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

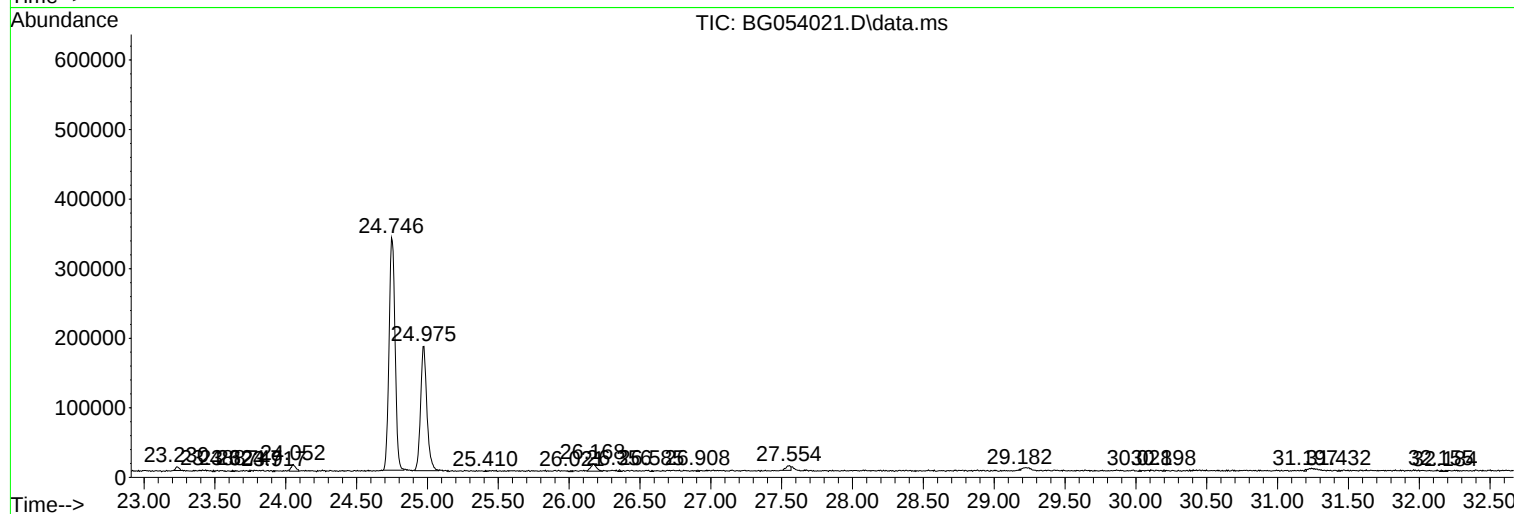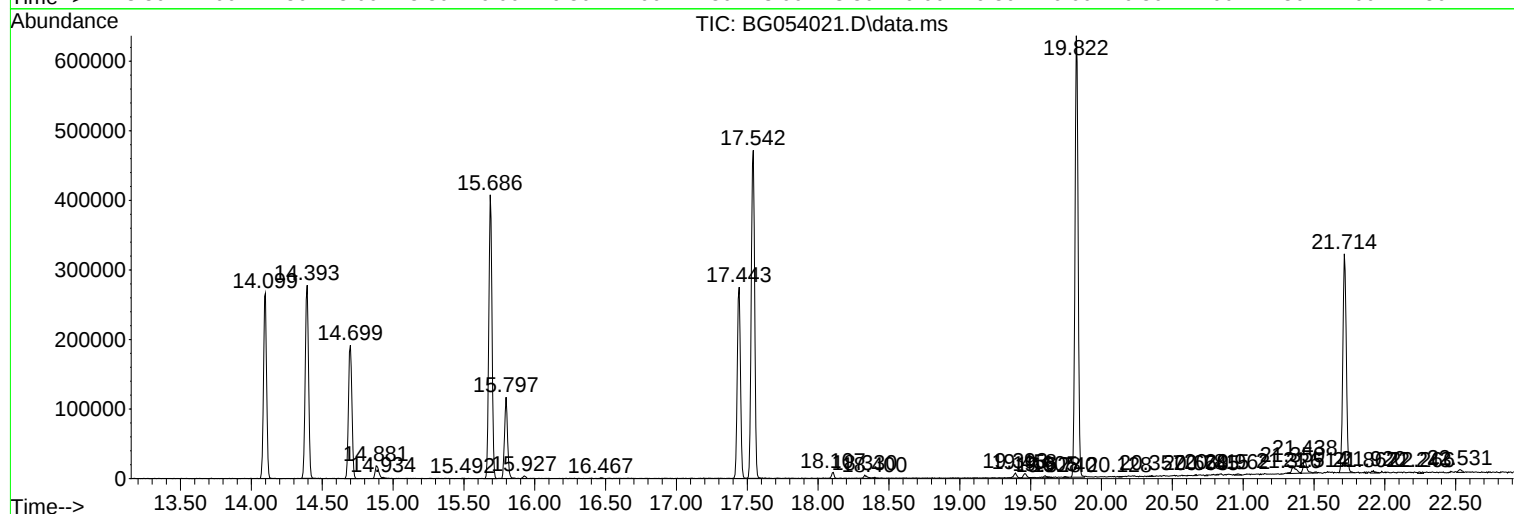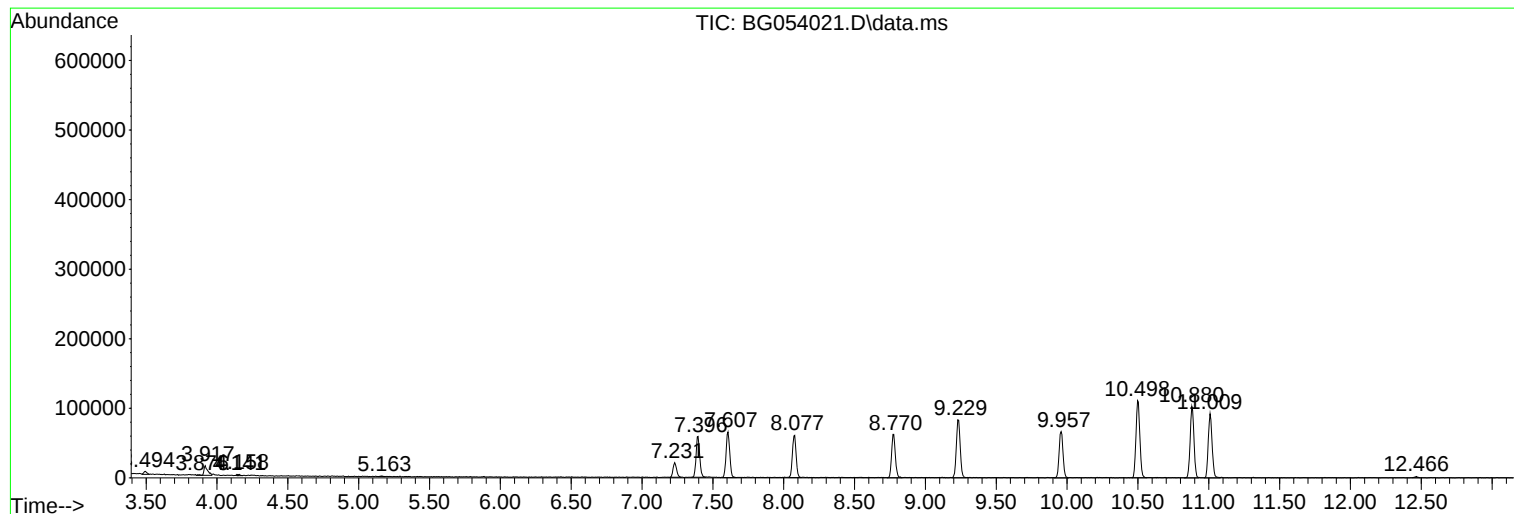

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054021.D
Acq On : 23 Jun 2022 20:14
Operator : CG/JU
Sample : N3400-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054021.D
Acq On : 23 Jun 2022 20:14
Operator : CG/JU
Sample : N3400-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------