

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054023.D
 Acq On : 23 Jun 2022 21:32
 Operator : CG/JU
 Sample : N3400-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.494	15	18	22	rVB2	4259	5596	0.51%	0.064%
2	3.782	62	67	69	rBV4	2102	3286	0.30%	0.038%
3	3.917	87	90	100	rBV	12003	23249	2.12%	0.266%
4	4.146	127	129	134	rVB2	1768	2145	0.20%	0.025%
5	4.246	143	146	152	rBV3	2527	4370	0.40%	0.050%
6	5.163	298	302	306	rBV3	1314	2112	0.19%	0.024%
7	7.231	648	654	660	rVV	20527	39533	3.61%	0.452%
8	7.395	675	682	692	rBV	63495	115876	10.59%	1.326%
9	7.607	711	718	726	rBV	69782	121073	11.06%	1.385%
10	8.071	789	797	805	rBB	62873	114725	10.48%	1.313%
11	8.153	809	811	816	rVB3	1105	1772	0.16%	0.020%
12	8.776	910	917	927	rBV	65543	119929	10.96%	1.372%
13	8.893	934	937	943	rVB3	1597	2683	0.25%	0.031%
14	9.228	987	994	1003	rVV	87187	164224	15.00%	1.879%
15	9.957	1111	1118	1125	rBV	74093	133310	12.18%	1.525%
16	10.497	1203	1210	1223	rBV	121666	232985	21.28%	2.666%
17	10.644	1226	1235	1244	rBV	16212	30691	2.80%	0.351%
18	10.703	1244	1245	1252	rVB2	1244	1992	0.18%	0.023%
19	10.756	1252	1254	1261	rBV2	1158	1771	0.16%	0.020%
20	10.885	1267	1276	1282	rBV	99425	187966	17.17%	2.151%
21	10.932	1282	1284	1291	rVB3	2741	4201	0.38%	0.048%
22	11.009	1291	1297	1305	rBV	31704	57617	5.26%	0.659%
23	11.408	1360	1365	1366	rBV2	1048	1216	0.11%	0.014%
24	11.526	1378	1385	1394	rVB2	33856	61918	5.66%	0.708%
25	12.460	1539	1544	1550	rVB	1988	3353	0.31%	0.038%
26	13.535	1722	1727	1733	rVV	8560	12470	1.14%	0.143%
27	13.594	1733	1737	1743	rVB	2686	3618	0.33%	0.041%
28	14.093	1816	1822	1829	rBV	282509	439818	40.18%	5.032%
29	14.228	1840	1845	1850	rBV2	4632	5316	0.49%	0.061%
30	14.393	1865	1873	1880	rBV	300591	490327	44.79%	5.610%
31	14.698	1918	1925	1933	rVB	203696	323325	29.54%	3.699%
32	14.886	1951	1957	1964	rBV3	26738	49193	4.49%	0.563%
33	14.933	1964	1965	1970	rVB2	978	1336	0.12%	0.015%
34	15.427	2042	2049	2055	rBV	88487	125700	11.48%	1.438%
35	15.492	2057	2060	2066	rVB4	1400	2048	0.19%	0.023%
36	15.685	2086	2093	2100	rBV	437669	694139	63.41%	7.942%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054023.D
 Acq On : 23 Jun 2022 21:32
 Operator : CG/JU
 Sample : N3400-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	15.797	2106	2112	2119	rBV	130263	199628	18.24%	2.284%
38	15.926	2128	2134	2141	rBV4	4176	7152	0.65%	0.082%
39	16.355	2202	2207	2214	rBV2	7049	12324	1.13%	0.141%
40	16.467	2223	2226	2229	rVB3	1495	1912	0.17%	0.022%
41	16.520	2229	2235	2241	rBV2	1559	2379	0.22%	0.027%
42	16.579	2241	2245	2247	rBV2	1301	1548	0.14%	0.018%
43	16.643	2252	2256	2260	rVB2	1242	2005	0.18%	0.023%
44	16.902	2297	2300	2305	rVB2	1581	2363	0.22%	0.027%
45	16.984	2309	2314	2318	rBV	1791	1741	0.16%	0.020%
46	17.031	2318	2322	2326	rVB2	5550	6960	0.64%	0.080%
47	17.190	2346	2349	2352	rBV	936	1234	0.11%	0.014%
48	17.442	2386	2392	2401	rVV	269171	432665	39.53%	4.950%
49	17.542	2401	2409	2416	rVV	522306	824616	75.33%	9.434%
50	18.106	2500	2505	2510	rVB	24427	31568	2.88%	0.361%
51	18.171	2514	2516	2521	rBV4	887	1523	0.14%	0.017%
52	18.224	2521	2525	2529	rBV4	933	1745	0.16%	0.020%
53	18.329	2539	2543	2549	rBV3	14367	23518	2.15%	0.269%
54	18.388	2551	2553	2556	rVB2	1013	1361	0.12%	0.016%
55	18.494	2568	2571	2575	rVB4	1072	1368	0.12%	0.016%
56	18.653	2592	2598	2610	rBV	38498	70932	6.48%	0.812%
57	18.729	2610	2611	2617	rVV3	1381	1395	0.13%	0.016%
58	18.823	2623	2627	2631	rBV4	893	1545	0.14%	0.018%
59	19.093	2671	2673	2680	rVB4	3338	4690	0.43%	0.054%
60	19.211	2690	2693	2698	rVB2	9517	11730	1.07%	0.134%
61	19.393	2719	2724	2729	rBV3	7357	10951	1.00%	0.125%
62	19.458	2730	2735	2739	rVV2	6452	9780	0.89%	0.112%
63	19.528	2744	2747	2750	rBV5	1484	2025	0.18%	0.023%
64	19.599	2753	2759	2763	rBV4	9148	14577	1.33%	0.167%
65	19.745	2781	2784	2790	rVB4	2038	3159	0.29%	0.036%
66	19.822	2790	2797	2806	rBV	706131	1069907	97.74%	12.241%
67	20.356	2886	2888	2891	rVB4	1741	1746	0.16%	0.020%
68	20.480	2906	2909	2910	rBV3	1076	1149	0.10%	0.013%
69	20.544	2915	2920	2923	rBV5	5866	8489	0.78%	0.097%
70	20.785	2959	2961	2963	rBV3	2595	2096	0.19%	0.024%
71	20.844	2968	2971	2976	rVV7	2021	3676	0.34%	0.042%
72	20.921	2981	2984	2985	rBV3	1162	1306	0.12%	0.015%
73	21.167	3024	3026	3029	rVV4	2402	2708	0.25%	0.031%
74	21.355	3053	3058	3063	rBV4	21783	35377	3.23%	0.405%
75	21.432	3067	3071	3078	rVB	17213	26305	2.40%	0.301%
76	21.643	3106	3107	3109	rBV2	2246	1908	0.17%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054023.D
 Acq On : 23 Jun 2022 21:32
 Operator : CG/JU
 Sample : N3400-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	21.714	3113	3119	3129	rVB2	318370	540569	49.38%	6.185%
78	21.913	3149	3153	3158	rVB6	5392	8214	0.75%	0.094%
79	22.530	3253	3258	3261	rBV5	5401	8818	0.81%	0.101%
80	22.671	3280	3282	3284	rVB3	2003	1330	0.12%	0.015%
81	23.024	3340	3342	3344	rBV3	1571	1718	0.16%	0.020%
82	23.188	3367	3370	3372	rBV3	2112	2821	0.26%	0.032%
83	23.230	3372	3377	3385	rVB5	7622	15742	1.44%	0.180%
84	23.423	3406	3410	3411	rBV4	3436	4626	0.42%	0.053%
85	23.564	3432	3434	3439	rVB6	2249	2359	0.22%	0.027%
86	24.052	3511	3517	3525	rBV4	7939	18403	1.68%	0.211%
87	24.751	3623	3636	3649	rBV2	371086	1094639	100.00%	12.524%
88	24.975	3663	3674	3688	rVB2	178768	545375	49.82%	6.240%
89	26.161	3870	3876	3886	rVB9	9015	28191	2.58%	0.323%
90	26.338	3904	3906	3907	rBV2	1991	1201	0.11%	0.014%
91	27.201	4051	4053	4055	rVB2	1895	1243	0.11%	0.014%
92	27.548	4107	4112	4123	rVB7	7008	22686	2.07%	0.260%
93	28.077	4200	4202	4205	rBV3	1676	1540	0.14%	0.018%
94	28.835	4329	4331	4332	rBV2	1584	1333	0.12%	0.015%
95	29.328	4414	4415	4420	rBV4	1725	2222	0.20%	0.025%
96	29.505	4443	4445	4451	rVB7	1877	2506	0.23%	0.029%
97	30.545	4620	4622	4624	rBV2	1982	2010	0.18%	0.023%
98	30.973	4693	4695	4697	rBV2	1626	1415	0.13%	0.016%
99	31.367	4760	4762	4766	rBV3	1743	2288	0.21%	0.026%
100	32.231	4907	4909	4911	rBV2	1619	1267	0.12%	0.014%


Sum of corrected areas: 8740460

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054023.D
Acq On : 23 Jun 2022 21:32
Operator : CG/JU
Sample : N3400-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

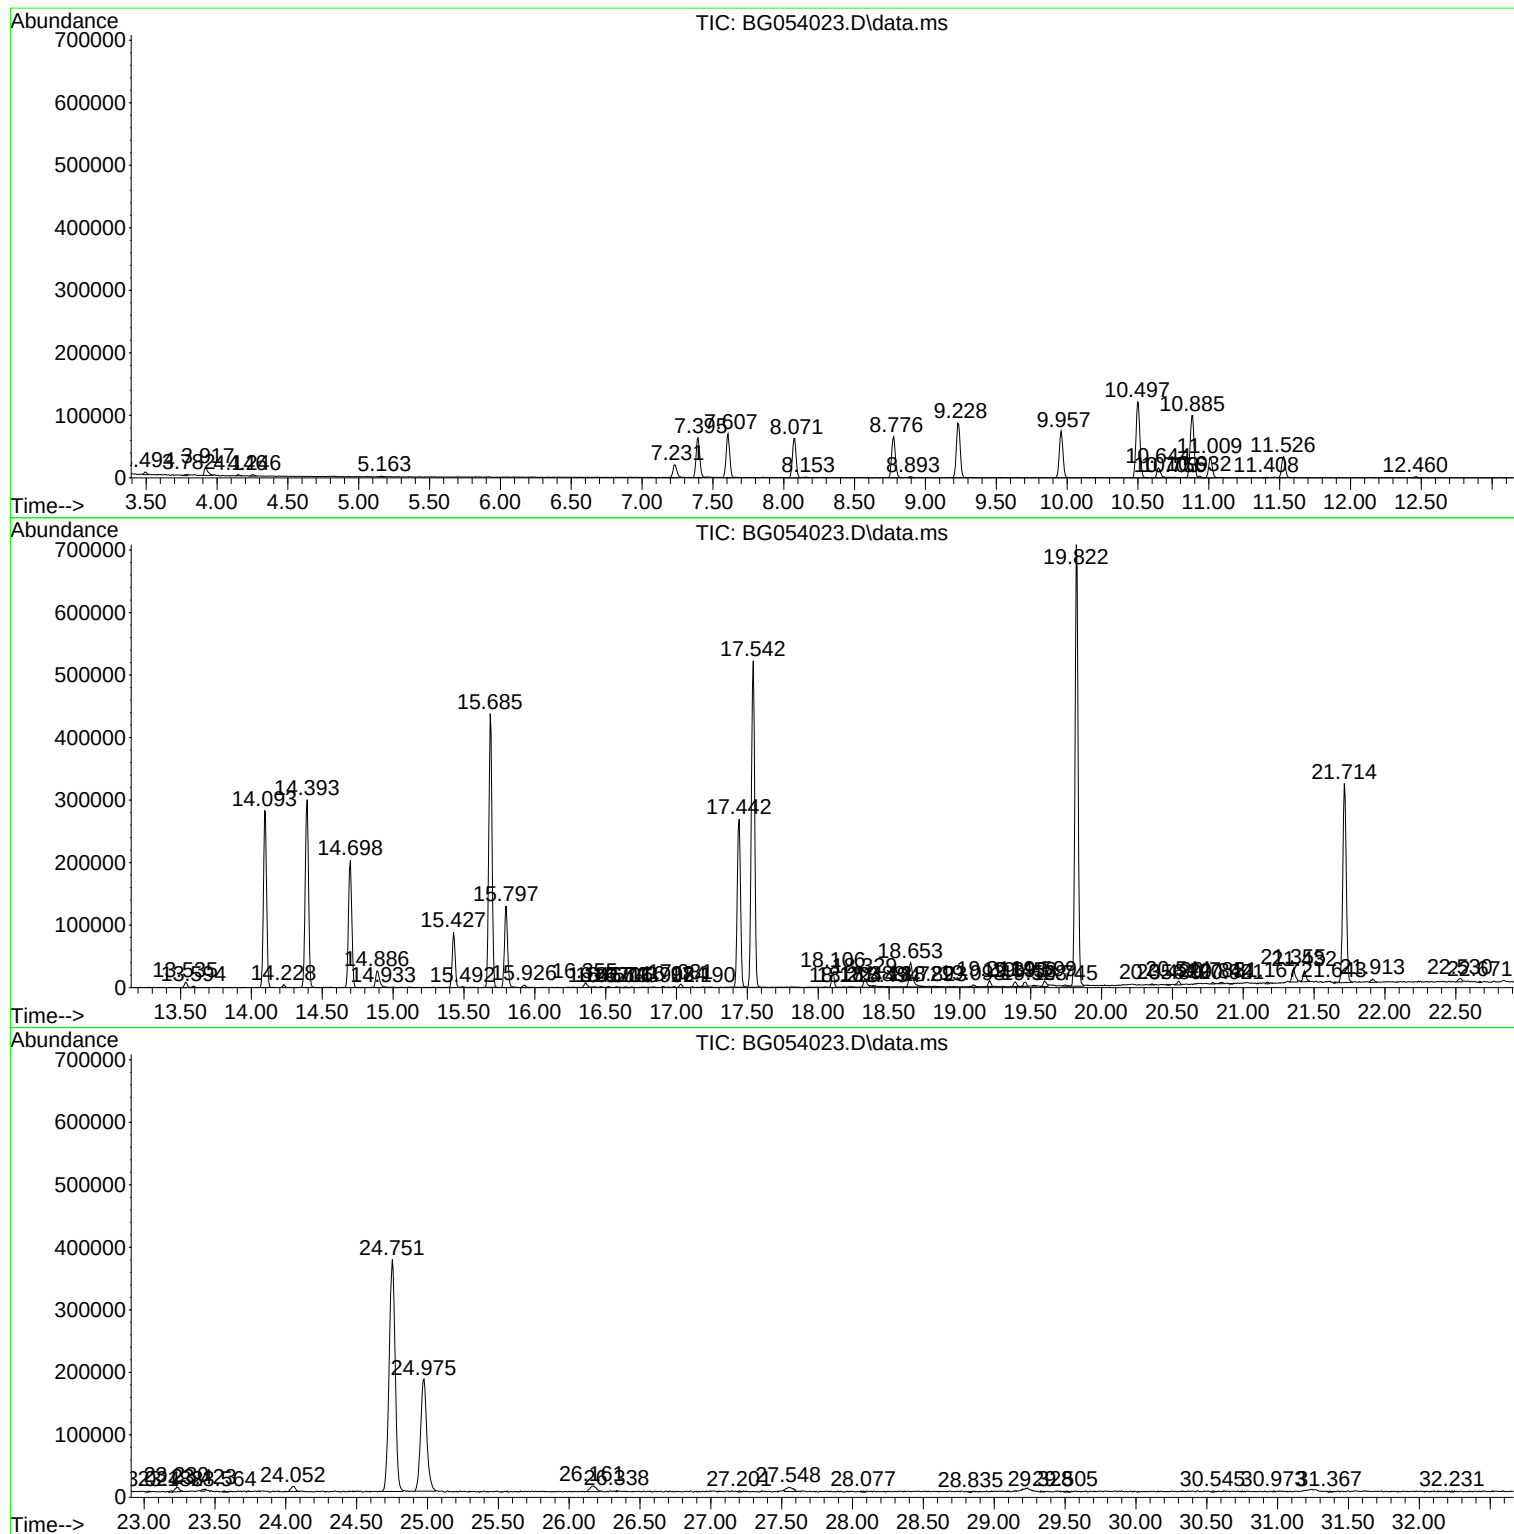

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054023.D
Acq On : 23 Jun 2022 21:32
Operator : CG/JU
Sample : N3400-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054023.D
Acq On : 23 Jun 2022 21:32
Operator : CG/JU
Sample : N3400-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc