

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054025.D
 Acq On : 23 Jun 2022 22:50
 Operator : CG/JU
 Sample : N3400-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.493	14	18	23	rBV3	4159	5627	0.52%	0.057%
2	3.910	86	89	99	rBV	22682	41047	3.77%	0.413%
3	4.151	124	130	135	rVB2	2291	4449	0.41%	0.045%
4	5.708	391	395	402	rVV	8565	13693	1.26%	0.138%
5	6.566	534	541	547	rVB2	5644	10161	0.93%	0.102%
6	7.054	617	624	631	rBV2	4120	6400	0.59%	0.064%
7	7.230	649	654	662	rVB	23909	42276	3.89%	0.426%
8	7.395	675	682	689	rBV	65277	114357	10.51%	1.151%
9	7.606	710	718	725	rBV2	71454	128790	11.84%	1.296%
10	7.730	734	739	744	rVB3	2568	3810	0.35%	0.038%
11	8.076	790	798	809	rBV	62134	111301	10.23%	1.120%
12	8.194	812	818	825	rVB	19990	33637	3.09%	0.339%
13	8.288	829	834	841	rVB2	8117	12811	1.18%	0.129%
14	8.452	854	862	869	rBV	23033	40988	3.77%	0.413%
15	8.570	876	882	886	rBV	6576	9350	0.86%	0.094%
16	8.722	901	908	911	rBV4	3909	6691	0.61%	0.067%
17	8.775	911	917	924	rVB2	74628	130061	11.95%	1.309%
18	9.187	980	987	990	rVV2	23452	42816	3.93%	0.431%
19	9.234	990	995	1009	rVB	87302	185367	17.04%	1.866%
20	9.516	1037	1043	1051	rVB4	6863	11908	1.09%	0.120%
21	9.710	1071	1076	1081	rVV	16089	25099	2.31%	0.253%
22	9.768	1081	1086	1092	rVB2	17235	26706	2.45%	0.269%
23	9.956	1112	1118	1128	rVB	74446	138134	12.69%	1.390%
24	10.127	1142	1147	1153	rVB3	6984	12738	1.17%	0.128%
25	10.279	1165	1173	1182	rBB2	52072	97754	8.98%	0.984%
26	10.497	1204	1210	1220	rVV	127927	244573	22.48%	2.462%
27	10.885	1267	1276	1282	rBV	98796	191847	17.63%	1.931%
28	10.932	1282	1284	1290	rVV	17440	23943	2.20%	0.241%
29	11.008	1290	1297	1308	rVV	96838	194974	17.92%	1.963%
30	11.690	1409	1413	1417	rVV2	2895	3646	0.34%	0.037%
31	11.866	1438	1443	1449	rVB4	2336	4169	0.38%	0.042%
32	12.130	1482	1488	1494	rBB2	2661	4549	0.42%	0.046%
33	12.430	1534	1539	1542	rBV3	2349	4199	0.39%	0.042%
34	12.589	1562	1566	1571	rBV2	6664	9213	0.85%	0.093%
35	12.683	1578	1582	1584	rVV3	2489	3471	0.32%	0.035%
36	12.741	1585	1592	1598	rVV2	17750	31708	2.91%	0.319%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054025.D
 Acq On : 23 Jun 2022 22:50
 Operator : CG/JU
 Sample : N3400-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	12.871	1606	1614	1618	rVV6	3890	8270	0.76%	0.083%
38	13.047	1637	1644	1649	rBV3	8141	13452	1.24%	0.135%
39	13.158	1658	1663	1668	rVV	17822	30569	2.81%	0.308%
40	13.276	1679	1683	1687	rVB3	3645	5103	0.47%	0.051%

41	13.505	1718	1722	1729	rVB5	6143	10240	0.94%	0.103%
42	13.564	1729	1732	1736	rBV3	2189	3331	0.31%	0.034%
43	13.658	1742	1748	1753	rBV2	15774	25278	2.32%	0.254%
44	13.711	1753	1757	1766	rVV3	39864	74093	6.81%	0.746%
45	13.822	1769	1776	1781	rVV3	13395	26302	2.42%	0.265%

46	13.864	1781	1783	1787	rVV3	6677	7969	0.73%	0.080%
47	13.934	1790	1795	1803	rVV2	59244	129725	11.92%	1.306%
48	14.005	1803	1807	1817	rVV4	21284	51369	4.72%	0.517%
49	14.099	1817	1823	1829	rVB	300727	449954	41.35%	4.529%
50	14.198	1835	1840	1844	rBV7	3155	6636	0.61%	0.067%

51	14.292	1851	1856	1858	rBV4	4523	6922	0.64%	0.070%
52	14.339	1858	1864	1868	rVV	78323	141952	13.05%	1.429%
53	14.392	1868	1873	1880	rVV	289889	497644	45.74%	5.009%
54	14.463	1880	1885	1890	rVV2	15353	27968	2.57%	0.282%
55	14.516	1890	1894	1906	rVB2	20227	43778	4.02%	0.441%

56	14.616	1906	1911	1914	rBV4	3362	5389	0.50%	0.054%
57	14.698	1917	1925	1932	rVB	196626	330801	30.40%	3.330%
58	14.780	1934	1939	1940	rBV4	4353	4781	0.44%	0.048%
59	14.886	1945	1957	1967	rVV5	48625	141880	13.04%	1.428%
60	15.039	1977	1983	1986	rBV6	5548	6695	0.62%	0.067%

61	15.097	1989	1993	1996	rBV3	4739	9179	0.84%	0.092%
62	15.203	2007	2011	2018	rVB3	8528	13516	1.24%	0.136%
63	15.391	2036	2043	2048	rVV2	24918	43166	3.97%	0.435%
64	15.579	2068	2075	2080	rVB4	5542	13212	1.21%	0.133%
65	15.685	2086	2093	2104	rBV	429064	692357	63.63%	6.969%

66	15.797	2106	2112	2120	rBV	145789	227673	20.92%	2.292%
67	15.926	2130	2134	2143	rVB2	4606	8542	0.79%	0.086%
68	16.020	2143	2150	2154	rBV5	2535	4945	0.45%	0.050%
69	16.084	2154	2161	2169	rBV	17495	31740	2.92%	0.319%
70	16.249	2184	2189	2195	rBV4	6964	13720	1.26%	0.138%

71	16.995	2310	2316	2319	rBV2	3628	7518	0.69%	0.076%
72	17.025	2319	2321	2328	rVB4	4178	7786	0.72%	0.078%
73	17.113	2333	2336	2339	rBV2	2925	4294	0.39%	0.043%
74	17.171	2344	2346	2350	rVV4	3082	4576	0.42%	0.046%
75	17.224	2352	2355	2361	rVV6	3387	6677	0.61%	0.067%

76	17.442	2384	2392	2399	rBV	269485	433250	39.82%	4.361%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054025.D
 Acq On : 23 Jun 2022 22:50
 Operator : CG/JU
 Sample : N3400-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	17.542	2402	2409	2416	rBV	512186	820717	75.43%	8.261%
78	18.106	2500	2505	2508	rVV5	2561	4116	0.38%	0.041%
79	18.241	2525	2528	2534	rVB4	3998	7550	0.69%	0.076%
80	18.329	2539	2543	2549	rBV3	25924	42301	3.89%	0.426%
81	18.817	2621	2626	2630	rBV3	3795	6052	0.56%	0.061%
82	18.922	2638	2644	2647	rBV5	6835	13504	1.24%	0.136%
83	18.975	2651	2653	2661	rVB6	5207	9345	0.86%	0.094%
84	19.275	2700	2704	2708	rBV5	2009	4203	0.39%	0.042%
85	19.386	2719	2723	2728	rBV4	10164	14302	1.31%	0.144%
86	19.457	2731	2735	2741	rBV	9135	16958	1.56%	0.171%
87	19.598	2755	2759	2769	rBV3	21168	40264	3.70%	0.405%
88	19.821	2790	2797	2809	rBV	719721	1084581	99.68%	10.917%
89	20.039	2832	2834	2837	rBV4	3360	3793	0.35%	0.038%
90	20.432	2893	2901	2902	rBV8	8922	17152	1.58%	0.173%
91	20.450	2902	2904	2909	rVV5	6278	13351	1.23%	0.134%
92	20.838	2965	2970	2973	rBV7	4359	7559	0.69%	0.076%
93	21.355	3053	3058	3063	rBV5	18194	32394	2.98%	0.326%
94	21.431	3068	3071	3076	rVV3	17333	25160	2.31%	0.253%
95	21.713	3112	3119	3128	rBV	324744	545082	50.09%	5.487%
96	23.235	3374	3378	3383	rBV7	6003	9223	0.85%	0.093%
97	24.040	3513	3515	3516	rBV2	7434	5757	0.53%	0.058%
98	24.751	3625	3636	3653	rVB2	370598	1088102	100.00%	10.953%
99	24.968	3663	3673	3692	rVB2	172677	566362	52.05%	5.701%
100	26.173	3872	3878	3882	rBV8	5151	12070	1.11%	0.121%




Sum of corrected areas: 9934413

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054025.D
Acq On : 23 Jun 2022 22:50
Operator : CG/JU
Sample : N3400-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

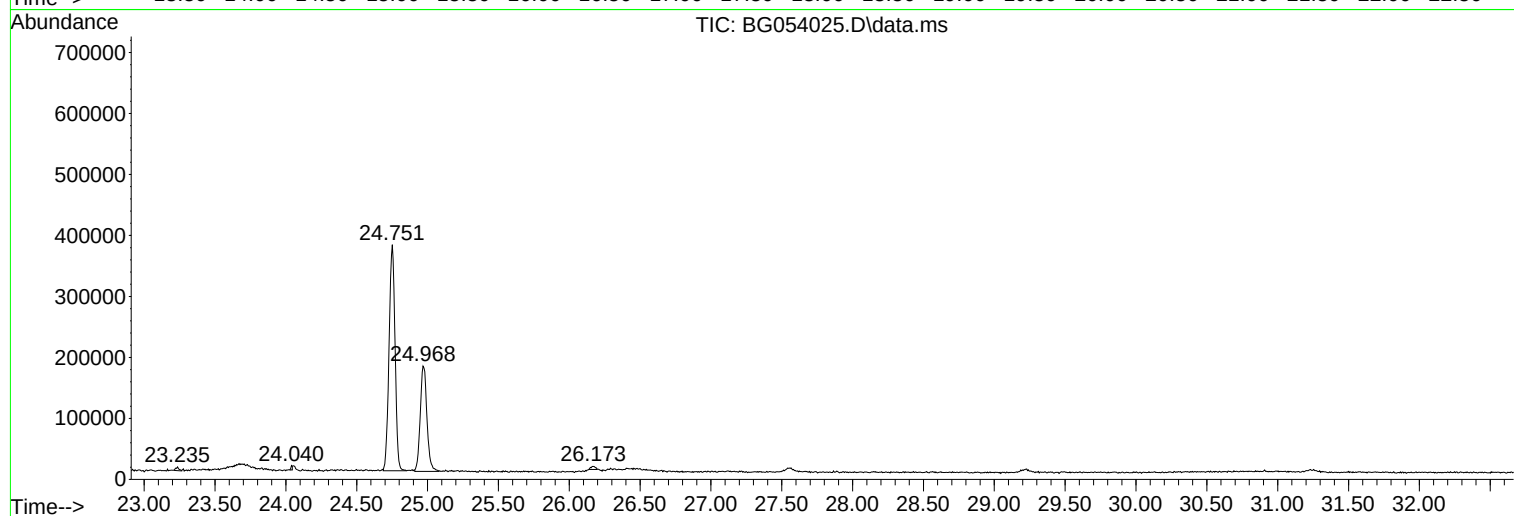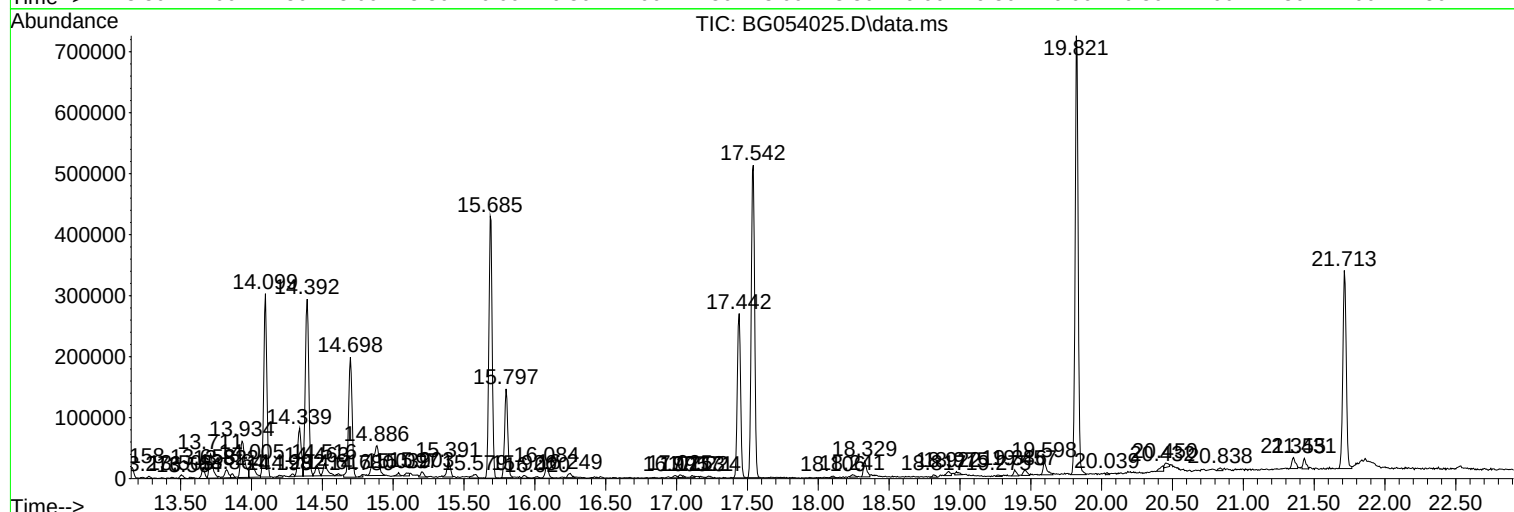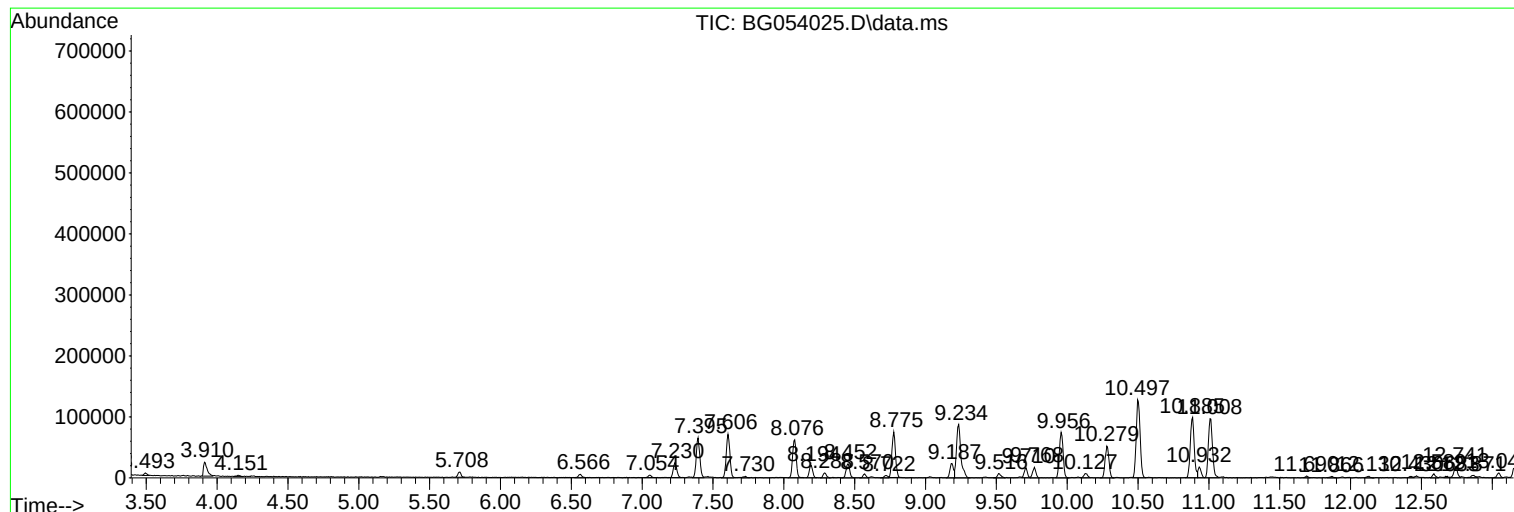

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054025.D
Acq On : 23 Jun 2022 22:50
Operator : CG/JU
Sample : N3400-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054025.D
Acq On : 23 Jun 2022 22:50
Operator : CG/JU
Sample : N3400-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc