

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054026.D
 Acq On : 23 Jun 2022 23:29
 Operator : CG/JU
 Sample : N3400-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.916	87	90	103	rBV	25169	49233	4.29%	0.336%
2	4.509	187	191	200	rBV	5867	9716	0.85%	0.066%
3	5.579	366	373	387	rVB	547095	915282	79.75%	6.251%
4	5.720	388	397	398	rBV	558100	1022547	89.10%	6.984%
5	5.849	414	419	425	rBV2	5865	8983	0.78%	0.061%
6	6.008	444	446	458	rBV2	9473	25960	2.26%	0.177%
7	6.566	535	541	543	rBV2	7478	12342	1.08%	0.084%
8	6.595	543	546	554	rVB2	9108	15189	1.32%	0.104%
9	7.047	619	623	629	rBV2	4671	8653	0.75%	0.059%
10	7.159	637	642	648	rBV2	11066	16635	1.45%	0.114%
11	7.230	648	654	662	rBV2	30658	59371	5.17%	0.406%
12	7.294	662	665	670	rVV	9168	12955	1.13%	0.088%
13	7.394	675	682	689	rBV	73044	124634	10.86%	0.851%
14	7.465	689	694	696	rBV	10918	16233	1.41%	0.111%
15	7.606	711	718	728	rVB	78266	145390	12.67%	0.993%
16	7.723	732	738	744	rBV	42101	70008	6.10%	0.478%
17	7.794	746	750	757	rVB3	4262	7456	0.65%	0.051%
18	8.076	789	798	804	rBV	67606	118704	10.34%	0.811%
19	8.134	804	808	813	rVV3	9034	17519	1.53%	0.120%
20	8.193	813	818	831	rVB	25590	52611	4.58%	0.359%
21	8.452	856	862	864	rBV2	14631	24100	2.10%	0.165%
22	8.499	864	870	878	rVB	338905	611987	53.32%	4.180%
23	8.628	887	892	896	rVB4	6618	10605	0.92%	0.072%
24	8.693	896	903	912	rBV2	115810	231928	20.21%	1.584%
25	8.775	912	917	926	rVB	80861	147210	12.83%	1.005%
26	8.869	926	933	945	rVB	77258	137284	11.96%	0.938%
27	9.045	953	963	966	rBV3	33661	64850	5.65%	0.443%
28	9.180	981	986	990	rBV	23984	43328	3.78%	0.296%
29	9.233	990	995	1007	rVB	100497	200284	17.45%	1.368%
30	9.515	1037	1043	1052	rVB4	8097	16923	1.47%	0.116%
31	9.709	1071	1076	1081	rBV	20413	33758	2.94%	0.231%
32	9.768	1081	1086	1095	rVV	37732	65654	5.72%	0.448%
33	9.838	1095	1098	1109	rVB5	7033	14600	1.27%	0.100%
34	9.956	1109	1118	1126	rBV	84086	165433	14.41%	1.130%
35	10.050	1129	1134	1137	rVV4	5171	10473	0.91%	0.072%
36	10.079	1137	1139	1144	rVV4	5943	7936	0.69%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054026.D
 Acq On : 23 Jun 2022 23:29
 Operator : CG/JU
 Sample : N3400-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	10.132	1144	1148	1150	rVV2	8548	13769	1.20%	0.094%
38	10.167	1150	1154	1161	rVB2	24178	42401	3.69%	0.290%
39	10.285	1167	1174	1183	rBV4	35870	78565	6.85%	0.537%
40	10.502	1199	1211	1219	rVB	145269	273993	23.87%	1.871%
41	10.884	1268	1276	1280	rBV	101961	190864	16.63%	1.304%
42	10.931	1280	1284	1291	rVV	81581	151972	13.24%	1.038%
43	11.013	1291	1298	1308	rVV	85528	166853	14.54%	1.140%
44	11.560	1385	1391	1398	rVB7	4049	11321	0.99%	0.077%
45	11.689	1408	1413	1416	rBV2	3828	6163	0.54%	0.042%
46	12.042	1466	1473	1480	rVB6	6090	13426	1.17%	0.092%
47	12.253	1502	1509	1516	rVB	46903	85761	7.47%	0.586%
48	12.535	1552	1557	1562	rBV5	5749	11569	1.01%	0.079%
49	12.588	1562	1566	1570	rVV3	6396	10687	0.93%	0.073%
50	12.635	1571	1574	1579	rVB3	4250	7407	0.65%	0.051%
51	12.741	1584	1592	1598	rBV5	19966	40180	3.50%	0.274%
52	12.835	1606	1608	1615	rVB6	5136	8889	0.77%	0.061%
53	13.158	1655	1663	1671	rVB2	45824	95556	8.33%	0.653%
54	13.234	1671	1676	1681	rBV4	4672	7053	0.61%	0.048%
55	13.505	1714	1722	1730	rVB7	14448	33644	2.93%	0.230%
56	13.657	1741	1748	1753	rBV2	31302	54491	4.75%	0.372%
57	13.716	1753	1758	1771	rVV	89281	164367	14.32%	1.123%
58	13.828	1771	1777	1780	rBV3	40087	77688	6.77%	0.531%
59	13.863	1780	1783	1788	rVB2	39138	58200	5.07%	0.398%
60	13.904	1788	1790	1792	rBV2	6441	6182	0.54%	0.042%
61	14.004	1803	1807	1814	rBV5	10273	19415	1.69%	0.133%
62	14.098	1814	1823	1833	rVB	317061	550051	47.93%	3.757%
63	14.239	1843	1847	1850	rBV4	4077	5435	0.47%	0.037%
64	14.333	1859	1863	1867	rBV2	33004	54270	4.73%	0.371%
65	14.392	1867	1873	1880	rVV	326095	549027	47.84%	3.750%
66	14.462	1880	1885	1890	rVB5	9797	18359	1.60%	0.125%
67	14.697	1919	1925	1932	rVB	200264	332819	29.00%	2.273%
68	14.797	1939	1942	1946	rBV3	4049	7299	0.64%	0.050%
69	14.850	1947	1951	1954	rVV6	8301	16691	1.45%	0.114%
70	14.897	1954	1959	1971	rVB	37297	75195	6.55%	0.514%
71	15.044	1981	1984	1989	rVB6	4637	6719	0.59%	0.046%
72	15.156	2001	2003	2008	rVV4	4142	6791	0.59%	0.046%
73	15.203	2008	2011	2016	rVV4	7609	12649	1.10%	0.086%
74	15.391	2039	2043	2050	rVV5	5588	10795	0.94%	0.074%
75	15.502	2056	2062	2068	rBV	84535	127289	11.09%	0.869%
76	15.690	2087	2094	2102	rVB	472046	772211	67.28%	5.274%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054026.D
 Acq On : 23 Jun 2022 23:29
 Operator : CG/JU
 Sample : N3400-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	15.796	2106	2112	2115	rBV	154219	236207	20.58%	1.613%
78	15.837	2115	2119	2132	rVB	334756	562477	49.01%	3.842%
79	16.078	2158	2160	2166	rVB6	4773	7776	0.68%	0.053%
80	16.448	2218	2223	2227	rBV2	15820	21261	1.85%	0.145%
81	17.030	2318	2322	2324	rBV3	4374	5500	0.48%	0.038%
82	17.112	2332	2336	2338	rBV2	7353	8748	0.76%	0.060%
83	17.236	2351	2357	2362	rVB	96021	143084	12.47%	0.977%
84	17.441	2385	2392	2399	rBV	277380	436941	38.07%	2.984%
85	17.541	2402	2409	2418	rBV	566331	886204	77.22%	6.053%
86	17.800	2449	2453	2459	rVB4	3442	5462	0.48%	0.037%
87	18.328	2539	2543	2552	rBV2	38800	67931	5.92%	0.464%
88	18.452	2561	2564	2572	rVB	18978	25481	2.22%	0.174%
89	18.546	2576	2580	2586	rBV3	9761	17473	1.52%	0.119%
90	18.922	2638	2644	2646	rBV4	8705	14690	1.28%	0.100%
91	18.981	2651	2654	2656	rBV3	9209	12775	1.11%	0.087%
92	19.133	2678	2680	2685	rVB3	5650	7715	0.67%	0.053%
93	19.392	2719	2724	2729	rVB3	10373	15680	1.37%	0.107%
94	19.456	2732	2735	2740	rVV	9154	14103	1.23%	0.096%
95	19.597	2755	2759	2771	rBV3	24425	46523	4.05%	0.318%
96	19.827	2791	2798	2810	rBV	719502	1147691	100.00%	7.839%
97	21.354	3054	3058	3067	rBV3	24828	47209	4.11%	0.322%
98	21.719	3113	3120	3127	rBV2	305881	532670	46.41%	3.638%
99	24.750	3625	3636	3649	rVB2	405843	1145734	99.83%	7.825%
100	24.974	3664	3674	3691	rVB	174000	560017	48.80%	3.825%




Sum of corrected areas: 14641142

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054026.D
Acq On : 23 Jun 2022 23:29
Operator : CG/JU
Sample : N3400-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

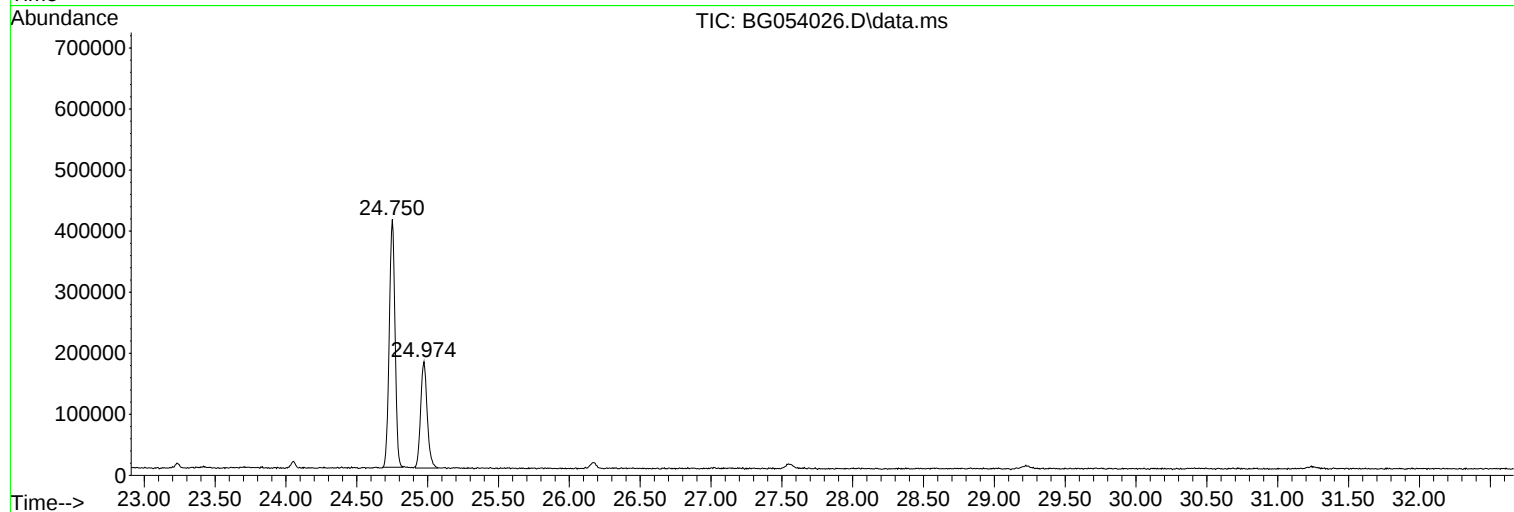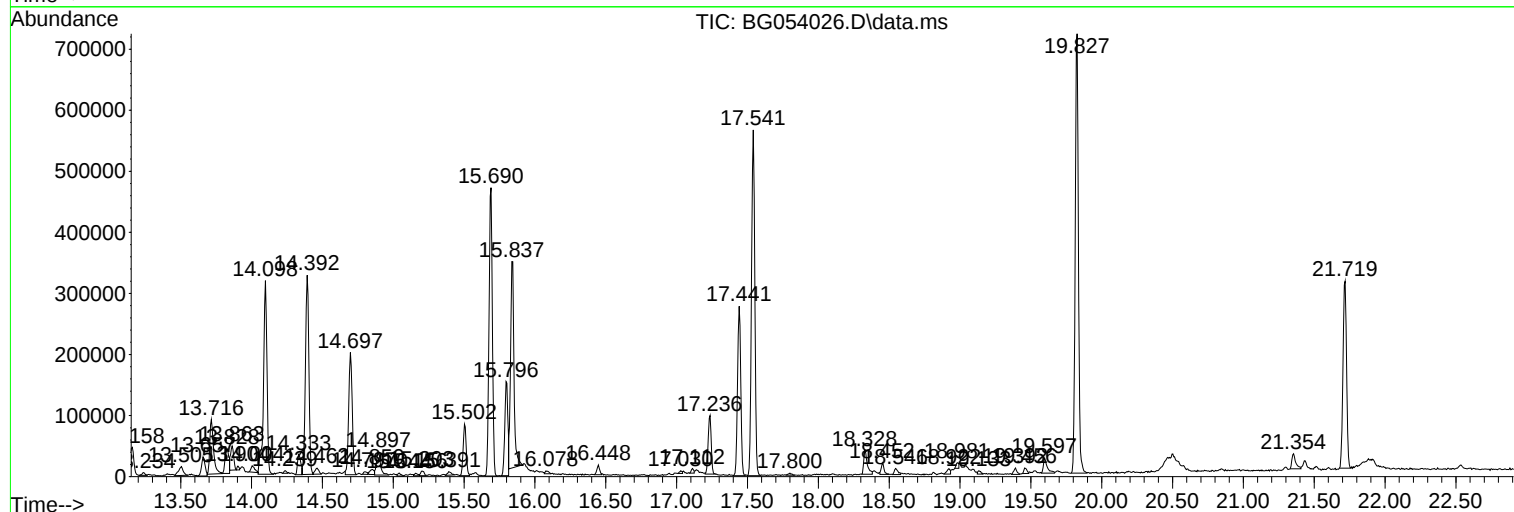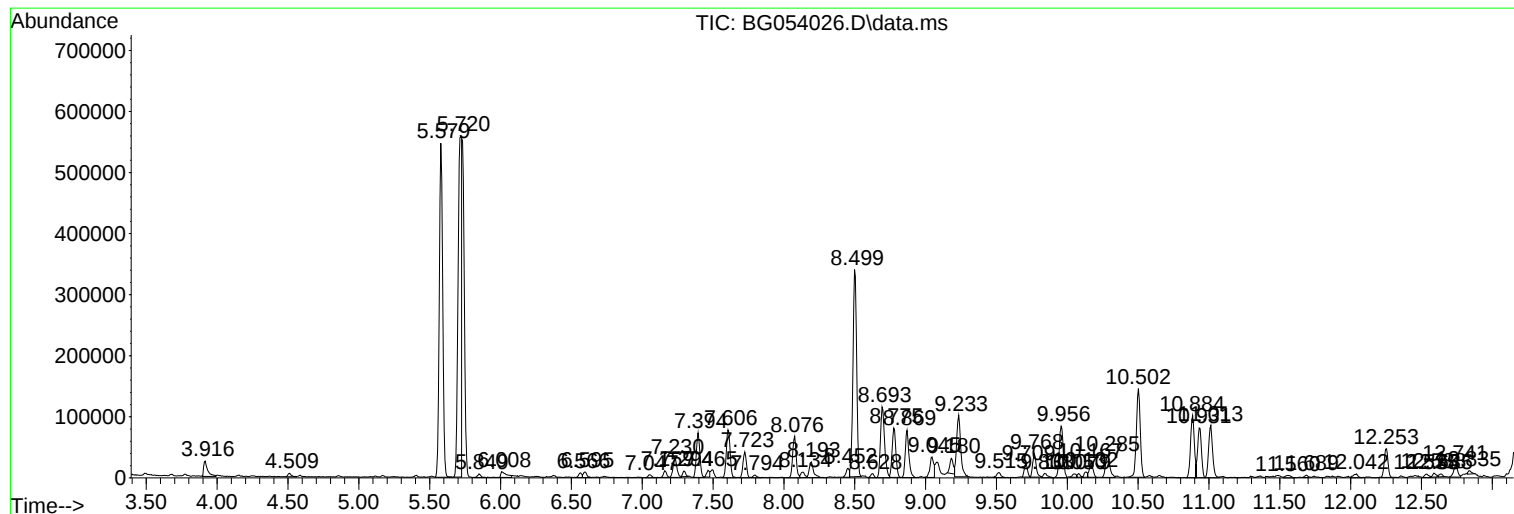

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054026.D
Acq On : 23 Jun 2022 23:29
Operator : CG/JU
Sample : N3400-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054026.D
Acq On : 23 Jun 2022 23:29
Operator : CG/JU
Sample : N3400-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------