

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054027.D
 Acq On : 24 Jun 2022 00:08
 Operator : CG/JU
 Sample : N3400-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.499	15	19	22	rBV3	3718	6006	0.52%	0.070%
2	3.917	87	90	103	rBV2	11785	22926	1.98%	0.265%
3	4.152	127	130	135	rVB3	1992	2688	0.23%	0.031%
4	4.246	142	146	147	rBV3	1088	1602	0.14%	0.019%
5	5.168	297	303	307	rVV4	1528	2840	0.25%	0.033%
6	7.042	617	622	630	rBV4	1720	3499	0.30%	0.040%
7	7.230	648	654	663	rVB2	20428	37764	3.26%	0.437%
8	7.307	663	667	671	rBV2	830	1572	0.14%	0.018%
9	7.395	675	682	690	rBV	71363	126137	10.90%	1.460%
10	7.606	711	718	726	rVV	73193	128839	11.13%	1.491%
11	8.071	792	797	805	rVB	61964	109803	9.49%	1.271%
12	8.776	910	917	926	rVB	66533	118244	10.21%	1.368%
13	8.899	934	938	941	rBV	970	1661	0.14%	0.019%
14	9.234	988	995	1005	rVB	97721	183326	15.84%	2.122%
15	9.957	1108	1118	1128	rVB	77927	143257	12.38%	1.658%
16	10.503	1203	1211	1219	rBV	127189	239636	20.70%	2.773%
17	10.885	1269	1276	1284	rVB	99410	185977	16.07%	2.152%
18	11.008	1290	1297	1308	rVB	78440	150764	13.02%	1.745%
19	11.478	1372	1377	1380	rBV2	1006	1463	0.13%	0.017%
20	12.354	1521	1526	1529	rBV2	1568	2152	0.19%	0.025%
21	12.459	1539	1544	1549	rBV3	1922	3478	0.30%	0.040%
22	14.099	1816	1823	1830	rBV	313171	467214	40.36%	5.407%
23	14.393	1864	1873	1881	rBV	339172	533234	46.06%	6.171%
24	14.698	1917	1925	1934	rVB	204964	321535	27.78%	3.721%
25	14.886	1952	1957	1970	rVB2	16216	31405	2.71%	0.363%
26	15.685	2086	2093	2102	rVB	454703	743498	64.23%	8.605%
27	15.797	2106	2112	2121	rBV	120230	186150	16.08%	2.154%
28	15.926	2129	2134	2139	rVB	4207	5566	0.48%	0.064%
29	16.361	2205	2208	2215	rVB	1607	2663	0.23%	0.031%
30	16.472	2224	2227	2231	rBV	1582	1972	0.17%	0.023%
31	17.442	2385	2392	2400	rVB	283756	442840	38.25%	5.125%
32	17.542	2400	2409	2419	rBV2	551256	887549	76.67%	10.272%
33	18.329	2539	2543	2552	rBV3	7259	12623	1.09%	0.146%
34	18.400	2552	2555	2562	rVB	1433	1918	0.17%	0.022%
35	19.393	2716	2724	2729	rBV3	8145	13846	1.20%	0.160%
36	19.463	2729	2736	2740	rVV	7087	10755	0.93%	0.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054027.D
 Acq On : 24 Jun 2022 00:08
 Operator : CG/JU
 Sample : N3400-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.551	2748	2751	2753	rBV2	982	1182	0.10%	0.014%
38	19.604	2755	2760	2761	rBV3	2031	2328	0.20%	0.027%
39	19.692	2768	2775	2779	rVB5	1425	3370	0.29%	0.039%
40	19.745	2779	2784	2786	rBV4	1905	2739	0.24%	0.032%
41	19.827	2790	2798	2806	rVV	737868	1141567	98.61%	13.212%
42	20.403	2894	2896	2899	rBV4	1045	1274	0.11%	0.015%
43	20.432	2899	2901	2904	rVB4	1225	1379	0.12%	0.016%
44	20.573	2923	2925	2928	rVV3	1111	1340	0.12%	0.016%
45	20.785	2958	2961	2963	rVB3	3250	2686	0.23%	0.031%
46	20.850	2969	2972	2974	rBV4	1865	1760	0.15%	0.020%
47	21.161	3024	3025	3027	rBV2	1381	1378	0.12%	0.016%
48	21.373	3056	3061	3064	rBV5	3335	5545	0.48%	0.064%
49	21.437	3068	3072	3076	rVV2	11274	17353	1.50%	0.201%
50	21.713	3112	3119	3127	rVB2	320903	545001	47.08%	6.307%
51	21.966	3160	3162	3167	rBV5	1987	2807	0.24%	0.032%
52	22.166	3194	3196	3197	rBV2	1549	1209	0.10%	0.014%
53	22.530	3253	3258	3262	rBV6	3179	4997	0.43%	0.058%
54	22.718	3288	3290	3293	rBV3	1887	1885	0.16%	0.022%
55	23.235	3373	3378	3385	rBV7	4963	11524	1.00%	0.133%
56	23.300	3387	3389	3392	rBV3	1945	1852	0.16%	0.021%
57	24.046	3511	3516	3526	rVB6	6082	15497	1.34%	0.179%
58	24.310	3559	3561	3566	rBV5	1621	1747	0.15%	0.020%
59	24.751	3622	3636	3657	rBV2	387521	1157626	100.00%	13.397%
60	24.974	3663	3674	3687	rVB2	175760	539404	46.60%	6.243%
61	25.750	3804	3806	3810	rVB4	1772	1200	0.10%	0.014%
62	26.132	3869	3871	3872	rBV2	2077	1251	0.11%	0.014%
63	26.167	3872	3877	3885	rVB7	6976	17314	1.50%	0.200%
64	26.719	3970	3971	3974	rBV3	1930	1715	0.15%	0.020%
65	27.142	4041	4043	4045	rBV3	1816	1610	0.14%	0.019%
66	27.665	4130	4132	4133	rBV2	2327	1674	0.14%	0.019%
67	28.112	4206	4208	4211	rBV3	1532	1174	0.10%	0.014%
68	28.517	4275	4277	4280	rBV3	1622	1479	0.13%	0.017%
69	29.545	4450	4452	4454	rBV3	1772	1841	0.16%	0.021%
70	31.196	4731	4733	4734	rBV2	2289	2095	0.18%	0.024%
71	31.373	4761	4763	4767	rBV4	1938	2962	0.26%	0.034%
72	31.948	4860	4861	4864	rBV3	2292	2500	0.22%	0.029%




Sum of corrected areas: 8640667

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054027.D
Acq On : 24 Jun 2022 00:08
Operator : CG/JU
Sample : N3400-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

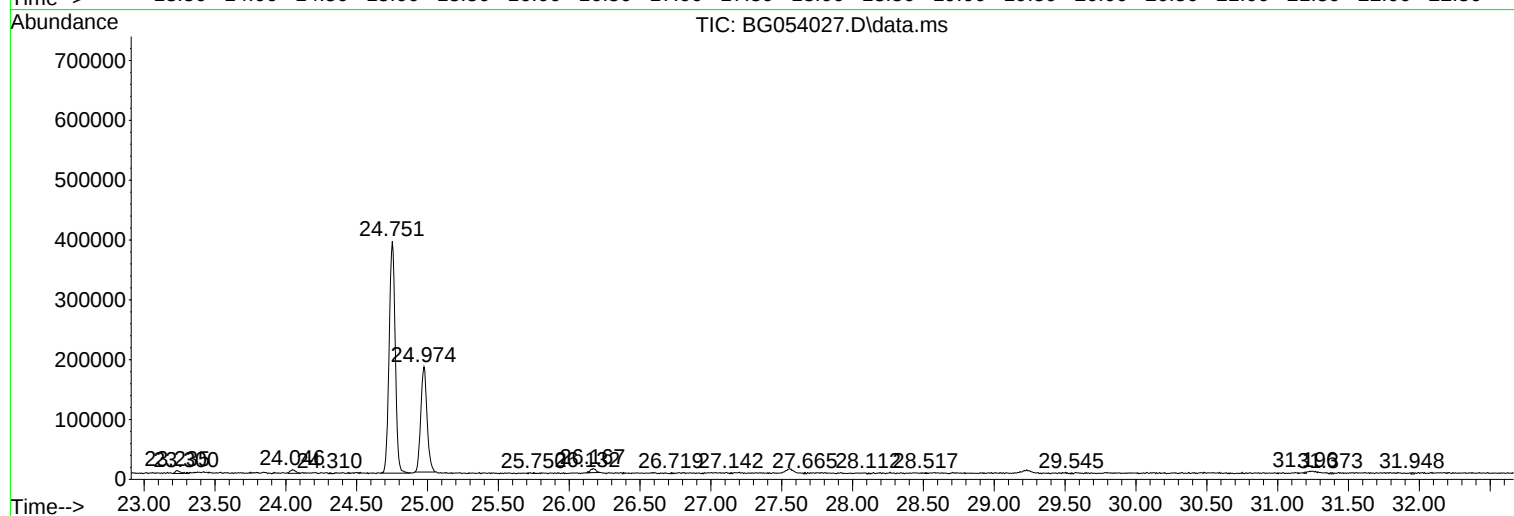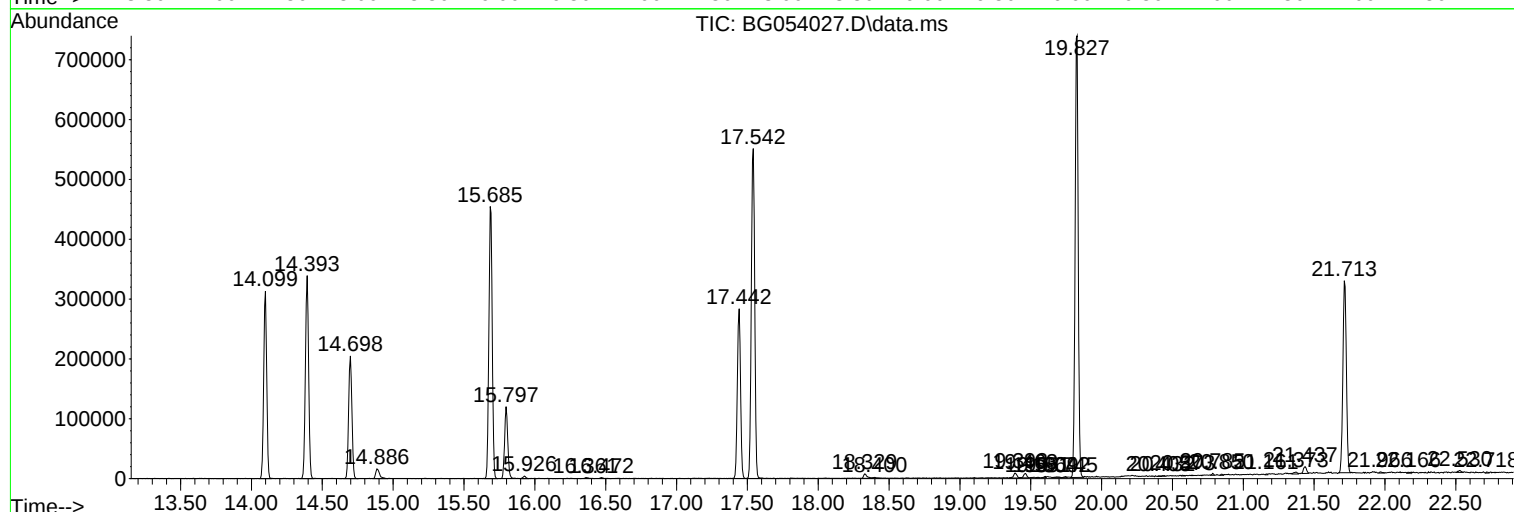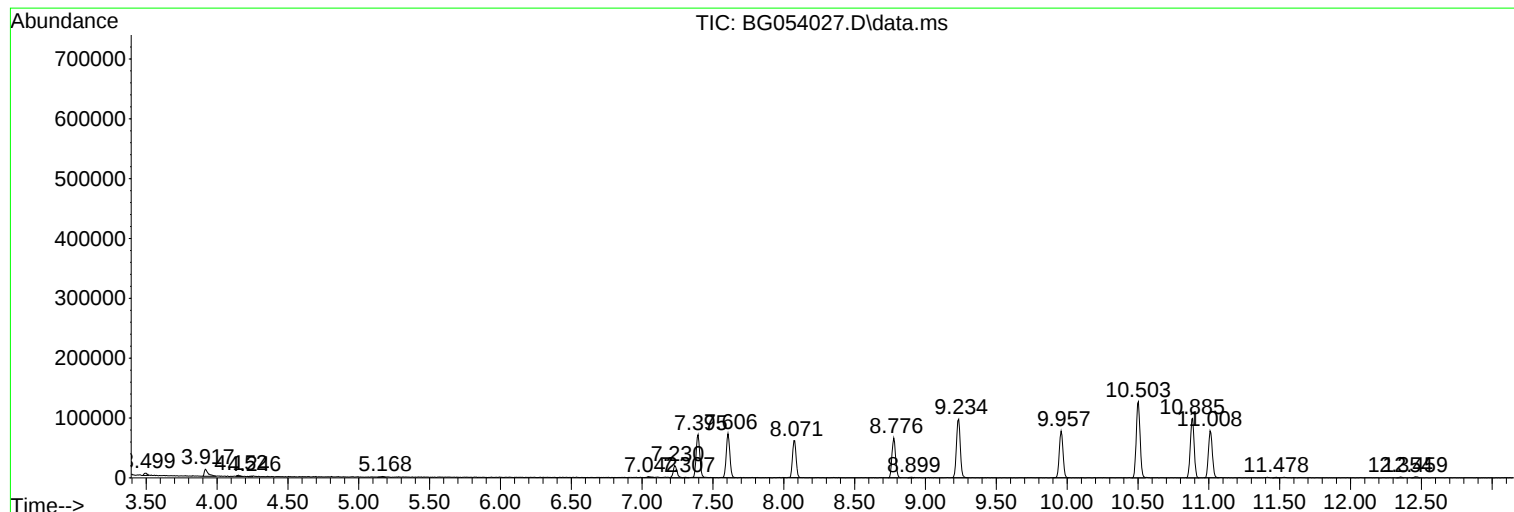

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054027.D
Acq On : 24 Jun 2022 00:08
Operator : CG/JU
Sample : N3400-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054027.D
Acq On : 24 Jun 2022 00:08
Operator : CG/JU
Sample : N3400-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------