

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054030.D
 Acq On : 24 Jun 2022 2:44
 Operator : CG/JU
 Sample : PB145691BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK691

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.494	14	18	23	rVB	6362	9215	0.77%	0.095%
2	3.588	32	34	37	rVB3	1119	1260	0.11%	0.013%
3	3.729	55	58	62	rVV4	798	1414	0.12%	0.015%
4	3.905	85	88	102	rVV	77223	141639	11.81%	1.453%
5	4.252	145	147	151	rVB2	1191	1278	0.11%	0.013%
6	7.231	646	654	664	rBV	113040	199791	16.66%	2.050%
7	7.395	673	682	692	rVB	78952	139012	11.59%	1.426%
8	7.607	710	718	728	rBV	102922	185323	15.46%	1.901%
9	8.071	791	797	805	rVV	62614	110143	9.19%	1.130%
10	8.776	909	917	928	rBV2	144559	265400	22.13%	2.723%
11	9.234	987	995	1003	rVB	106926	197695	16.49%	2.028%
12	9.957	1112	1118	1126	rBV2	91882	168886	14.08%	1.733%
13	10.497	1203	1210	1220	rBV	150276	285027	23.77%	2.924%
14	10.885	1267	1276	1284	rBV	97805	185868	15.50%	1.907%
15	11.009	1290	1297	1307	rBV	154334	285910	23.84%	2.933%
16	12.466	1537	1545	1549	rBV2	2358	4207	0.35%	0.043%
17	14.099	1814	1823	1831	rBV	323725	505556	42.16%	5.187%
18	14.393	1865	1873	1881	rBV	345759	573341	47.81%	5.882%
19	14.698	1918	1925	1933	rBV	196865	316850	26.42%	3.251%
20	14.881	1951	1956	1968	rBV	126489	223313	18.62%	2.291%
21	15.685	2086	2093	2103	rVB	506775	788547	65.76%	8.090%
22	15.797	2106	2112	2120	rBV	147506	224499	18.72%	2.303%
23	15.926	2128	2134	2138	rVB3	5203	6927	0.58%	0.071%
24	16.467	2224	2226	2230	rVB	1989	2039	0.17%	0.021%
25	17.442	2385	2392	2399	rVB	274915	438866	36.60%	4.503%
26	17.542	2401	2409	2416	rBV	588081	917909	76.55%	9.417%
27	19.393	2717	2724	2729	rBV3	8423	12935	1.08%	0.133%
28	19.457	2729	2735	2742	rBV	7370	12353	1.03%	0.127%
29	19.822	2791	2797	2808	rBV	763135	1182234	98.59%	12.129%
30	20.168	2852	2856	2857	rVV4	1523	1936	0.16%	0.020%
31	20.215	2857	2864	2867	rVV6	2071	4909	0.41%	0.050%
32	20.574	2921	2925	2927	rBV4	1481	1721	0.14%	0.018%
33	21.203	3031	3032	3035	rBV3	1870	2087	0.17%	0.021%
34	21.244	3037	3039	3044	rVV4	1338	1731	0.14%	0.018%
35	21.438	3068	3072	3081	rVB2	7391	11840	0.99%	0.121%
36	21.714	3112	3119	3130	rBV	319782	537179	44.80%	5.511%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054030.D
 Acq On : 24 Jun 2022 2:44
 Operator : CG/JU
 Sample : PB145691BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK691

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	21.919	3149	3154	3156	rBV5	2184	3856	0.32%	0.040%
38	22.524	3255	3257	3261	rBV4	1903	2135	0.18%	0.022%
39	23.230	3373	3377	3386	rVB9	3743	7943	0.66%	0.081%
40	23.294	3386	3388	3389	rBV2	1772	1221	0.10%	0.013%
41	23.353	3396	3398	3401	rBV4	2579	2941	0.25%	0.030%
42	24.669	3620	3622	3624	rBV3	1735	2119	0.18%	0.022%
43	24.751	3624	3636	3655	rVV2	400914	1199108	100.00%	12.302%
44	24.975	3663	3674	3692	rVB2	172969	543520	45.33%	5.576%
45	25.445	3752	3754	3755	rBV2	1570	1403	0.12%	0.014%
46	26.285	3895	3897	3899	rBV2	1614	1353	0.11%	0.014%
47	27.548	4106	4112	4120	rVB10	5384	15154	1.26%	0.155%
48	28.030	4192	4194	4197	rBV2	2142	2319	0.19%	0.024%
49	28.858	4333	4335	4336	rBV2	1560	1628	0.14%	0.017%
50	29.422	4429	4431	4433	rBV3	1944	1365	0.11%	0.014%
51	29.493	4441	4443	4446	rBV2	1692	2582	0.22%	0.026%
52	29.704	4477	4479	4482	rBV4	1637	1921	0.16%	0.020%
53	30.315	4581	4583	4586	rBV4	1680	2027	0.17%	0.021%
54	30.556	4622	4624	4626	rVB3	1858	1503	0.13%	0.015%
55	31.584	4797	4799	4802	rBV3	2018	2271	0.19%	0.023%
56	31.966	4861	4864	4867	rVB3	1761	1943	0.16%	0.020%




Sum of corrected areas: 9747152

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054030.D
Acq On : 24 Jun 2022 2:44
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

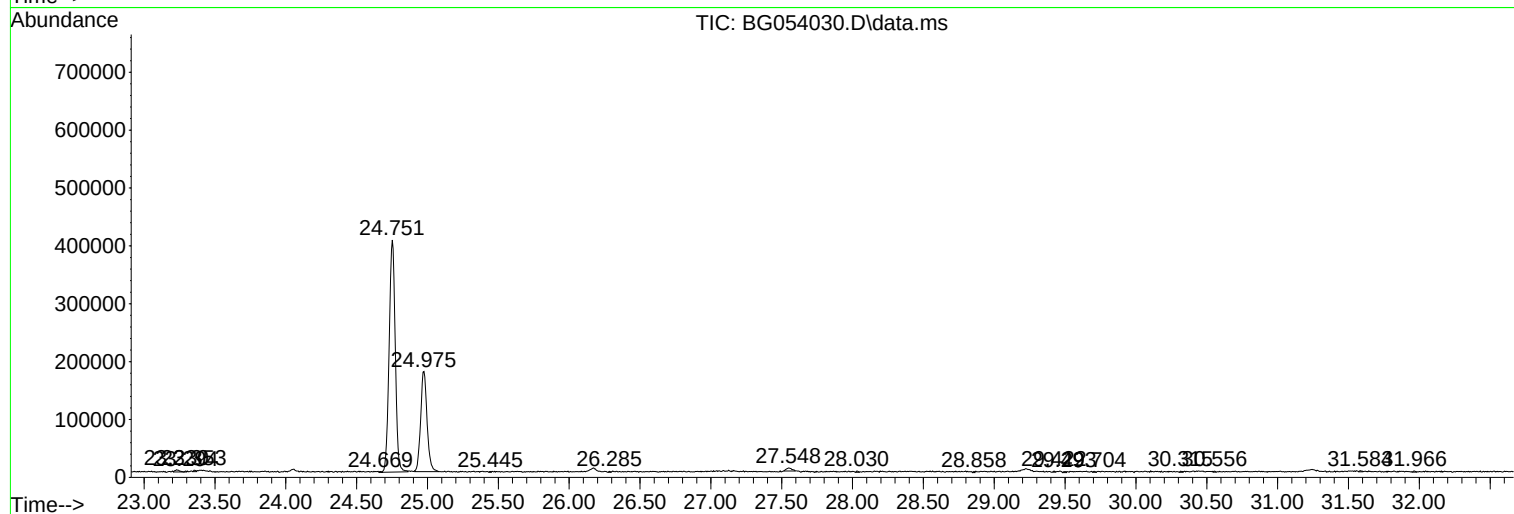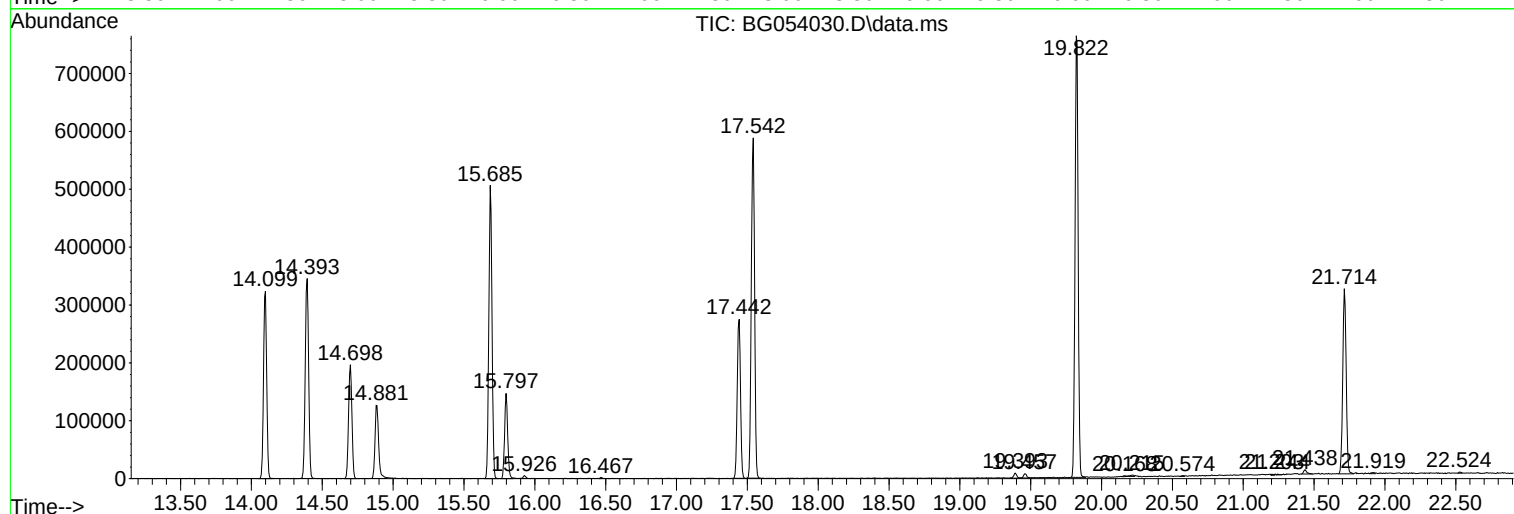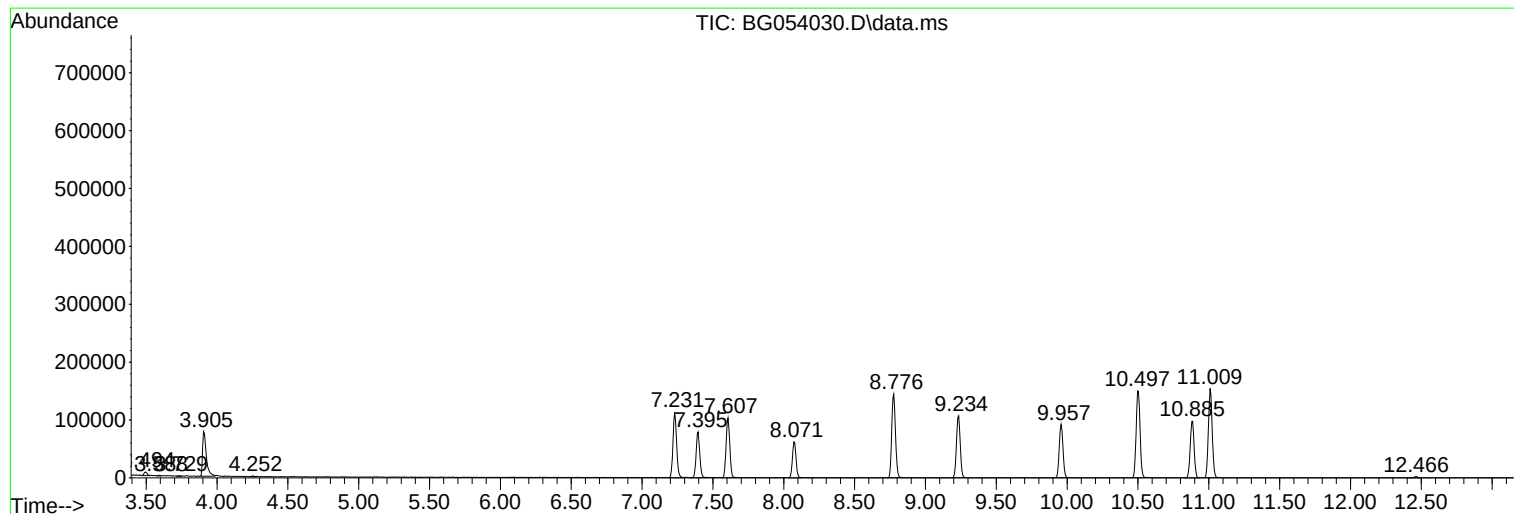

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054030.D
Acq On : 24 Jun 2022 2:44
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054030.D
Acq On : 24 Jun 2022 2:44
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc