

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054031.D
 Acq On : 24 Jun 2022 3:23
 Operator : CG/JU
 Sample : PB145702BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK702

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.412	3	4	8	rBV4	1338	1382	0.14%	0.016%
2	3.494	14	18	25	rVB2	5816	9098	0.93%	0.104%
3	3.905	84	88	104	rBV	62162	117778	11.98%	1.345%
4	4.252	143	147	150	rBV2	1417	1724	0.18%	0.020%
5	6.308	492	497	502	rBV4	642	1621	0.16%	0.019%
6	7.231	646	654	665	rVV	92452	165091	16.79%	1.885%
7	7.395	675	682	692	rBV	64102	114869	11.68%	1.311%
8	7.607	711	718	728	rVB	82335	152528	15.52%	1.741%
9	7.854	755	760	765	rBV	673	1623	0.17%	0.019%
10	8.071	791	797	806	rVB	71612	128565	13.08%	1.468%
11	8.776	910	917	928	rVB	121773	220199	22.40%	2.514%
12	9.229	987	994	1006	rVB	88792	165486	16.83%	1.889%
13	9.957	1110	1118	1127	rBV	76471	139792	14.22%	1.596%
14	10.498	1203	1210	1220	rBV	123397	236615	24.07%	2.701%
15	10.885	1267	1276	1284	rBB	113156	212954	21.66%	2.431%
16	11.009	1290	1297	1309	rBV	128811	239549	24.37%	2.735%
17	12.460	1540	1544	1549	rBV2	1922	3156	0.32%	0.036%
18	14.099	1816	1823	1830	rBV	277146	417036	42.42%	4.761%
19	14.393	1865	1873	1880	rBV	296964	478110	48.63%	5.458%
20	14.699	1917	1925	1933	rBV	223282	362211	36.84%	4.135%
21	14.887	1950	1957	1969	rBV	98647	176121	17.92%	2.011%
22	15.686	2086	2093	2102	rVB	407742	656981	66.83%	7.500%
23	15.797	2106	2112	2122	rBV	116599	173965	17.70%	1.986%
24	15.927	2131	2134	2140	rVB2	3586	5181	0.53%	0.059%
25	16.473	2222	2227	2232	rVB2	1536	2500	0.25%	0.029%
26	17.443	2385	2392	2398	rBV	318630	493016	50.15%	5.629%
27	17.542	2401	2409	2419	rVB2	466681	759429	77.25%	8.670%
28	18.929	2642	2645	2650	rVV3	739	1267	0.13%	0.014%
29	19.105	2669	2675	2678	rBV3	801	1128	0.11%	0.013%
30	19.393	2720	2724	2728	rVB4	6648	8964	0.91%	0.102%
31	19.464	2729	2736	2742	rVV	6212	8211	0.84%	0.094%
32	19.569	2750	2754	2756	rBV4	809	1083	0.11%	0.012%
33	19.822	2791	2797	2809	rVV	649416	982582	99.95%	11.218%
34	20.145	2850	2852	2855	rBV2	945	1190	0.12%	0.014%
35	20.180	2855	2858	2859	rBV3	1005	1205	0.12%	0.014%
36	20.797	2960	2963	2964	rBV3	1242	1245	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054031.D
 Acq On : 24 Jun 2022 3:23
 Operator : CG/JU
 Sample : PB145702BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK702

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.950	2985	2989	2992	rBV4	1527	1938	0.20%	0.022%
38	21.191	3028	3030	3033	rVB4	1465	1159	0.12%	0.013%
39	21.350	3053	3057	3058	rBV3	1136	997	0.10%	0.011%
40	21.432	3067	3071	3076	rBV2	6258	10685	1.09%	0.122%
41	21.714	3112	3119	3127	rBV	365818	614588	62.52%	7.016%
42	22.213	3202	3204	3207	rBV4	1603	1901	0.19%	0.022%
43	23.142	3360	3362	3366	rBV4	1565	1629	0.17%	0.019%
44	23.230	3375	3377	3384	rVB5	4638	6688	0.68%	0.076%
45	24.052	3513	3517	3523	rVB4	5099	9194	0.94%	0.105%
46	24.170	3536	3537	3540	rBV3	1536	1651	0.17%	0.019%
47	24.628	3614	3615	3619	rBV4	1608	1995	0.20%	0.023%
48	24.746	3625	3635	3651	rBV2	338705	983073	100.00%	11.223%
49	24.969	3662	3673	3690	rBV2	192428	617962	62.86%	7.055%
50	26.162	3871	3876	3888	rVB8	8496	23361	2.38%	0.267%
51	26.614	3951	3953	3956	rBV4	1737	1430	0.15%	0.016%
52	26.890	3998	4000	4002	rBV3	1566	1423	0.14%	0.016%
53	27.460	4095	4097	4098	rVB2	1933	1146	0.12%	0.013%
54	27.548	4108	4112	4121	rVB9	8053	20399	2.08%	0.233%
55	28.136	4210	4212	4214	rVB3	2502	1543	0.16%	0.018%
56	28.353	4248	4249	4252	rBV2	1868	1871	0.19%	0.021%
57	29.329	4413	4415	4416	rBV2	1809	1175	0.12%	0.013%
58	29.716	4480	4481	4484	rBV3	1513	1232	0.13%	0.014%
59	29.746	4484	4486	4487	rBV2	2048	990	0.10%	0.011%
60	29.869	4505	4507	4508	rVB	2298	1129	0.11%	0.013%
61	30.051	4536	4538	4539	rVB2	2162	1030	0.10%	0.012%
62	30.175	4557	4559	4560	rBV2	1775	1314	0.13%	0.015%
63	30.427	4600	4602	4604	rBV3	1801	1527	0.16%	0.017%
64	30.527	4617	4619	4621	rBV2	1430	1036	0.11%	0.012%
65	31.661	4810	4812	4814	rBV3	1706	1691	0.17%	0.019%




Sum of corrected areas: 8759212

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054031.D
Acq On : 24 Jun 2022 3:23
Operator : CG/JU
Sample : PB145702BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK702

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

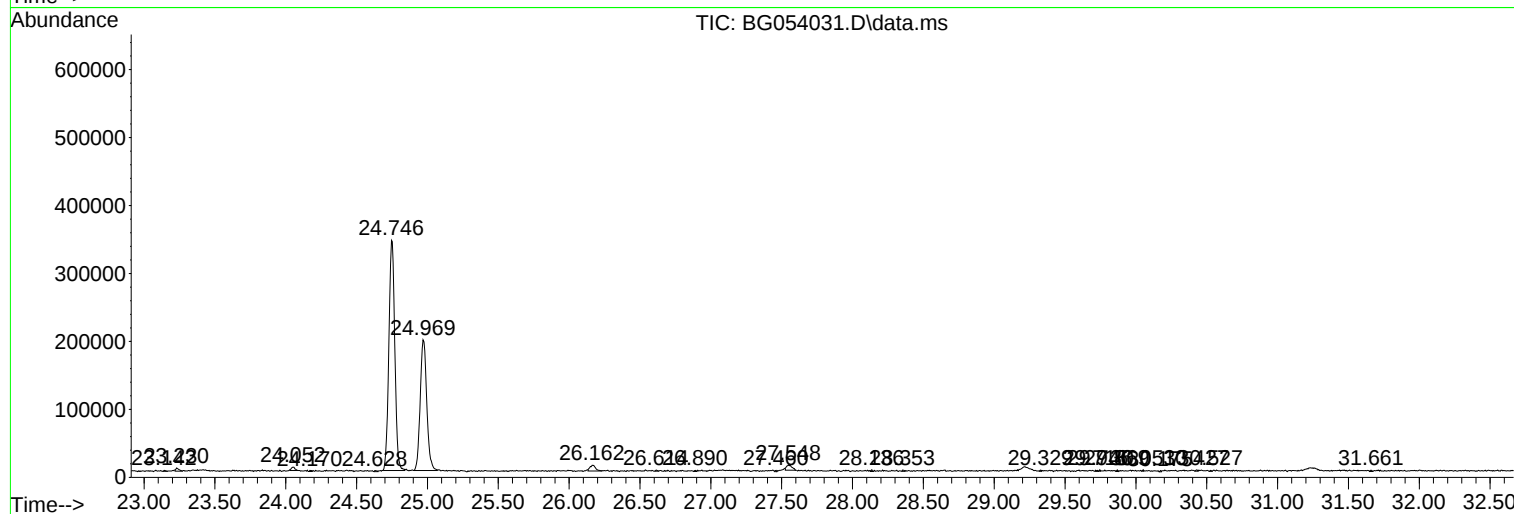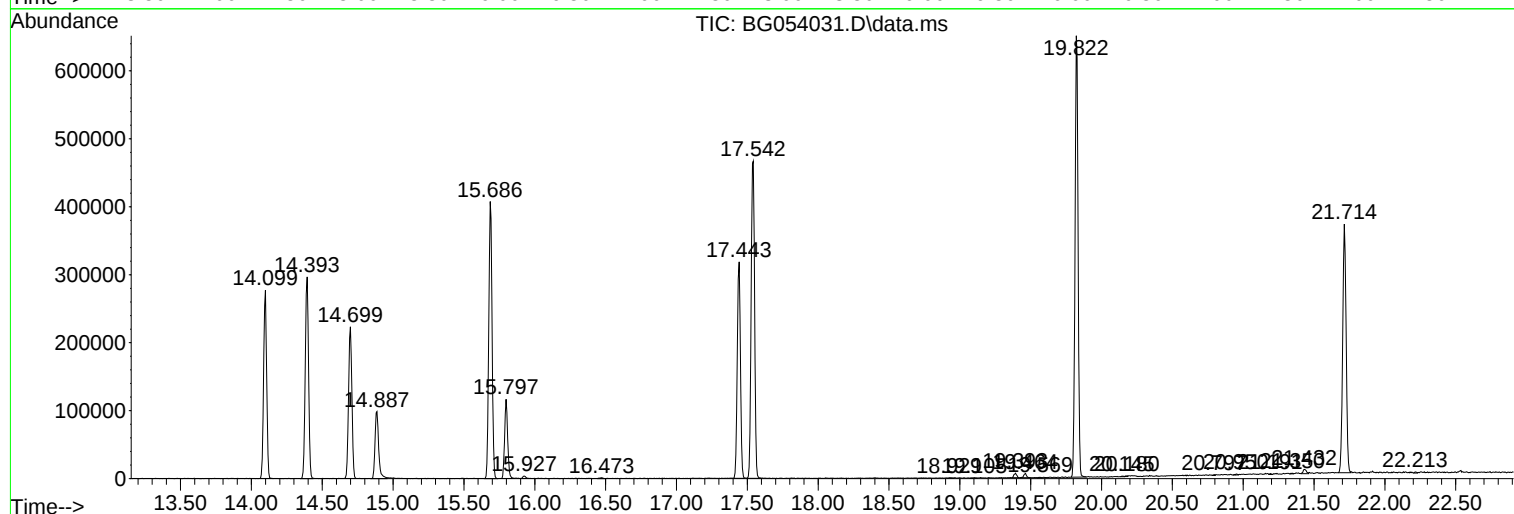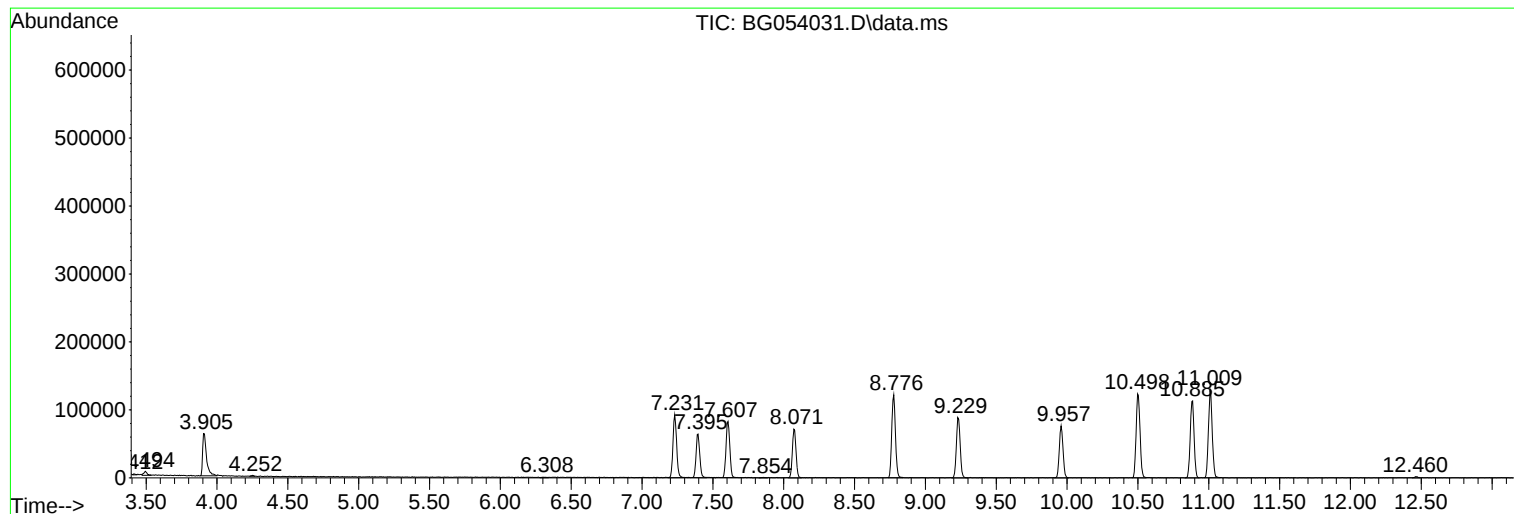

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054031.D
Acq On : 24 Jun 2022 3:23
Operator : CG/JU
Sample : PB145702BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK702

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054031.D
Acq On : 24 Jun 2022 3:23
Operator : CG/JU
Sample : PB145702BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK702

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
