

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054033.D
 Acq On : 24 Jun 2022 4:41
 Operator : CG/JU
 Sample : N3395-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.491	14	17	23	rVB2	4840	7763	0.62%	0.081%
2	3.914	85	89	100	rVV	24559	44491	3.54%	0.466%
3	4.149	124	129	134	rVB4	2016	3691	0.29%	0.039%
4	4.255	142	147	150	rVB5	947	1610	0.13%	0.017%
5	5.160	300	301	306	rVB3	1323	1517	0.12%	0.016%
6	7.234	647	654	661	rBV	28251	51977	4.13%	0.544%
7	7.392	674	681	691	rBV	81938	143226	11.39%	1.500%
8	7.604	711	717	727	rBV	79361	147240	11.71%	1.542%
9	8.074	791	797	806	rVB	66168	114509	9.11%	1.199%
10	8.773	910	916	926	rBV2	79932	144299	11.48%	1.511%
11	9.231	985	994	1005	rBV	110984	204572	16.27%	2.142%
12	9.960	1111	1118	1127	rBV	89568	163393	12.99%	1.711%
13	10.501	1203	1210	1225	rBV	148231	274776	21.85%	2.877%
14	10.882	1265	1275	1283	rBB	103066	193411	15.38%	2.025%
15	11.012	1289	1297	1307	rBV	117409	221630	17.63%	2.320%
16	12.463	1539	1544	1549	rVB3	2078	3609	0.29%	0.038%
17	13.521	1721	1724	1728	rVB	1074	1271	0.10%	0.013%
18	14.096	1816	1822	1831	rVB	343174	520623	41.41%	5.451%
19	14.390	1865	1872	1881	rBV	349932	592103	47.09%	6.199%
20	14.696	1918	1924	1932	rBB	197819	330711	26.30%	3.463%
21	14.884	1951	1956	1967	rBV3	29159	51382	4.09%	0.538%
22	15.424	2043	2048	2052	rBV2	1153	1509	0.12%	0.016%
23	15.489	2056	2059	2062	rBV	1460	1722	0.14%	0.018%
24	15.689	2085	2093	2100	rBV	533972	829970	66.01%	8.690%
25	15.794	2105	2111	2120	rBV	145373	231027	18.37%	2.419%
26	15.929	2129	2134	2138	rVB2	4763	6867	0.55%	0.072%
27	16.470	2222	2226	2231	rVB3	1360	1947	0.15%	0.020%
28	17.439	2384	2391	2399	rBV	292415	452325	35.97%	4.736%
29	17.539	2401	2408	2418	rBV	619237	969173	77.08%	10.147%
30	18.103	2499	2504	2510	rBV	8139	9492	0.75%	0.099%
31	18.327	2539	2542	2547	rBV4	6081	8409	0.67%	0.088%
32	18.397	2550	2554	2558	rVB3	1815	3394	0.27%	0.036%
33	19.267	2697	2702	2705	rBV3	3631	5006	0.40%	0.052%
34	19.390	2719	2723	2728	rBV3	9086	12479	0.99%	0.131%
35	19.461	2730	2735	2740	rBV	7798	12723	1.01%	0.133%
36	19.596	2754	2758	2764	rBV4	2309	5475	0.44%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054033.D
 Acq On : 24 Jun 2022 4:41
 Operator : CG/JU
 Sample : N3395-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0161

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.737	2780	2782	2787	rVB3	1828	2149	0.17%	0.023%
38	19.825	2790	2797	2807	rVV	833396	1239379	98.57%	12.976%
39	20.113	2842	2846	2849	rBV3	992	1283	0.10%	0.013%
40	20.142	2849	2851	2854	rVB3	1342	1298	0.10%	0.014%
41	20.318	2877	2881	2885	rVV6	1805	2479	0.20%	0.026%
42	20.659	2937	2939	2941	rBV3	1362	1295	0.10%	0.014%
43	21.023	2999	3001	3005	rBV3	1420	1882	0.15%	0.020%
44	21.106	3013	3015	3018	rBV4	1409	1373	0.11%	0.014%
45	21.353	3053	3057	3066	rVV5	22061	40976	3.26%	0.429%
46	21.435	3068	3071	3081	rVB2	7498	13096	1.04%	0.137%
47	21.717	3112	3119	3128	rVB2	316136	549754	43.72%	5.756%
48	22.528	3255	3257	3259	rBV3	2561	2229	0.18%	0.023%
49	22.780	3298	3300	3302	rBV3	1416	1281	0.10%	0.013%
50	22.868	3313	3315	3317	rBV3	1458	1276	0.10%	0.013%
51	23.233	3372	3377	3382	rVB5	4888	7174	0.57%	0.075%
52	23.468	3415	3417	3420	rBV4	1391	1274	0.10%	0.013%
53	23.785	3469	3471	3474	rBV3	1534	1872	0.15%	0.020%
54	24.055	3511	3517	3522	rVB7	9540	17455	1.39%	0.183%
55	24.196	3537	3541	3544	rBV4	1539	2256	0.18%	0.024%
56	24.749	3623	3635	3650	rBV2	433152	1257387	100.00%	13.165%
57	24.895	3658	3660	3661	rBV	1971	1311	0.10%	0.014%
58	24.972	3662	3673	3692	rVB2	181198	567156	45.11%	5.938%
59	25.136	3700	3701	3706	rBV4	1801	2396	0.19%	0.025%
60	26.170	3871	3877	3881	rBV5	7638	16845	1.34%	0.176%
61	27.475	4097	4099	4101	rBV2	1597	1684	0.13%	0.018%
62	27.551	4106	4112	4126	rVB7	9344	32659	2.60%	0.342%
63	29.032	4362	4364	4367	rBV3	1334	1454	0.12%	0.015%
64	29.202	4389	4393	4395	rBV5	4181	6504	0.52%	0.068%
65	30.242	4568	4570	4572	rBV3	1829	1719	0.14%	0.018%
66	31.823	4837	4839	4840	rBV2	1767	1336	0.11%	0.014%
67	31.858	4843	4845	4846	rBV2	1570	1481	0.12%	0.016%




Sum of corrected areas: 9551035

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054033.D
Acq On : 24 Jun 2022 4:41
Operator : CG/JU
Sample : N3395-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0161

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

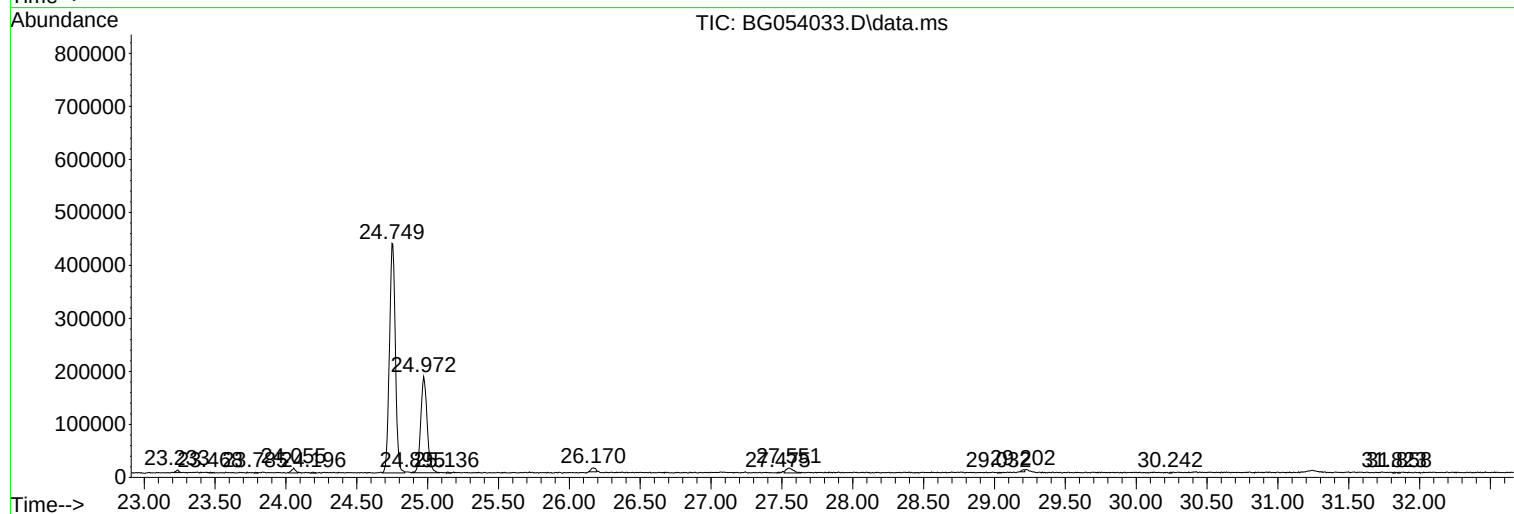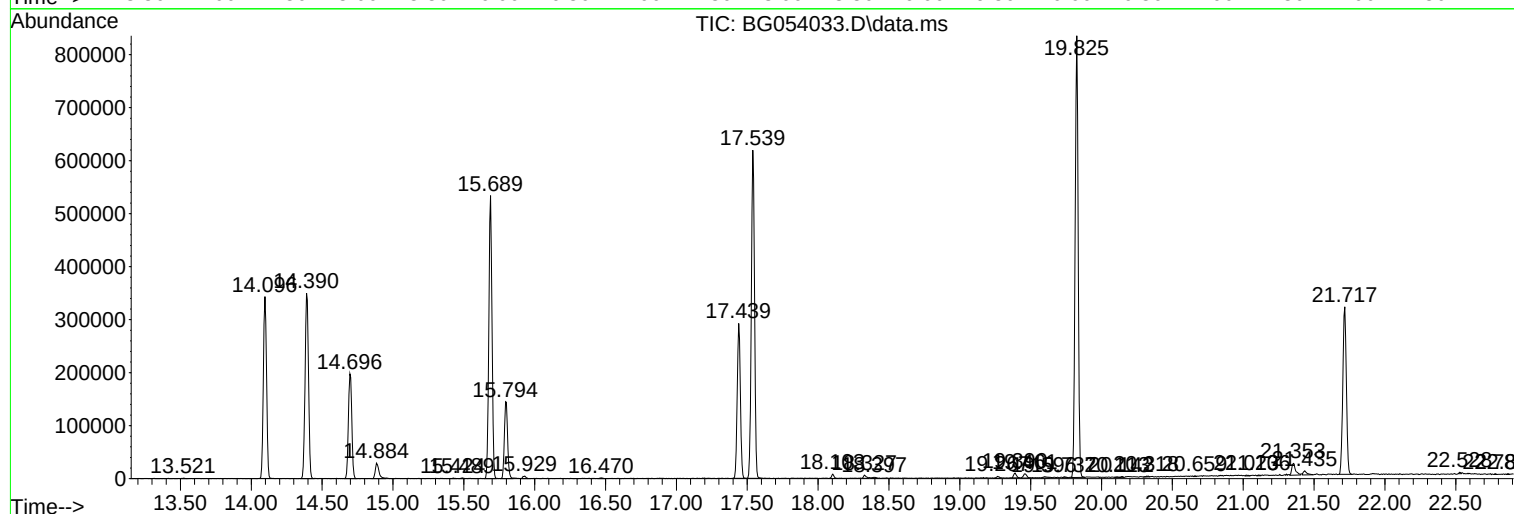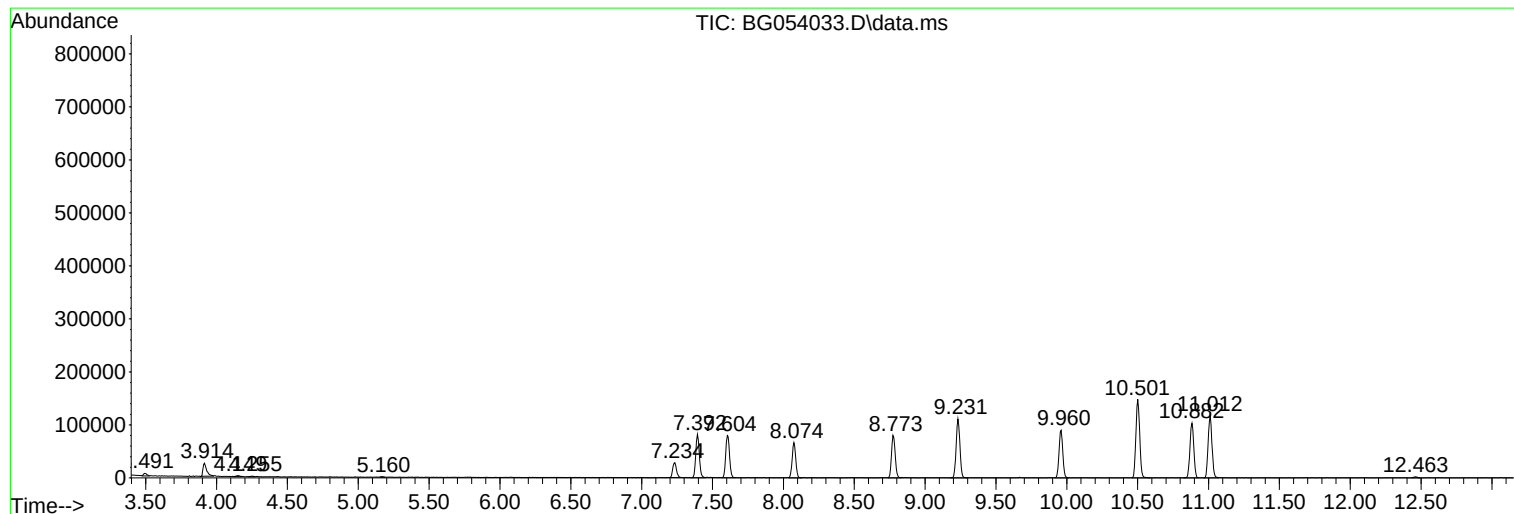

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054033.D
Acq On : 24 Jun 2022 4:41
Operator : CG/JU
Sample : N3395-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0161

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054033.D
Acq On : 24 Jun 2022 4:41
Operator : CG/JU
Sample : N3395-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0161

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
