

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054035.D
 Acq On : 24 Jun 2022 5:59
 Operator : CG/JU
 Sample : N3395-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.494	14	18	25	rVB5	3479	6344	0.57%	0.077%
2	3.917	87	90	99	rBV	10054	19325	1.75%	0.235%
3	4.146	125	129	131	rBV6	2065	2487	0.22%	0.030%
4	4.246	141	146	150	rBV4	1339	2535	0.23%	0.031%
5	4.575	199	202	204	rBV4	971	1368	0.12%	0.017%
6	5.392	337	341	344	rBV2	1054	1428	0.13%	0.017%
7	7.231	649	654	664	rVB2	18314	34930	3.16%	0.424%
8	7.319	664	669	672	rBV	720	1468	0.13%	0.018%
9	7.395	674	682	690	rBV	60443	108717	9.83%	1.321%
10	7.607	711	718	728	rVB	63716	113568	10.27%	1.380%
11	8.071	791	797	806	rVB	59222	103869	9.39%	1.262%
12	8.776	911	917	928	rVB	60912	108569	9.82%	1.319%
13	9.228	987	994	1002	rBV	84677	158817	14.36%	1.929%
14	9.957	1111	1118	1127	rVB	71736	127853	11.56%	1.553%
15	10.503	1200	1211	1222	rBV	111525	213957	19.34%	2.599%
16	10.879	1267	1275	1284	rBB	96353	180118	16.28%	2.188%
17	11.009	1290	1297	1306	rBV	96976	182701	16.52%	2.220%
18	12.466	1540	1545	1548	rBV2	1881	2908	0.26%	0.035%
19	14.093	1816	1822	1830	rBV	273266	420012	37.97%	5.103%
20	14.393	1866	1873	1881	rBV	282354	462857	41.85%	5.623%
21	14.699	1918	1925	1933	rVB	195566	310338	28.06%	3.770%
22	14.887	1952	1957	1967	rBV2	20018	35621	3.22%	0.433%
23	15.427	2043	2049	2055	rVV2	10686	15260	1.38%	0.185%
24	15.492	2055	2060	2066	rVB	1067	2034	0.18%	0.025%
25	15.686	2086	2093	2103	rVB	413752	669054	60.49%	8.128%
26	15.797	2106	2112	2125	rVB	128829	195389	17.67%	2.374%
27	15.926	2131	2134	2138	rVB2	3502	4375	0.40%	0.053%
28	16.467	2223	2226	2232	rVB3	1232	1937	0.18%	0.024%
29	17.225	2350	2355	2358	rBV3	841	1195	0.11%	0.015%
30	17.442	2385	2392	2399	rBV	271903	423403	38.28%	5.144%
31	17.542	2402	2409	2418	rVV	522153	847415	76.62%	10.295%
32	17.630	2423	2424	2430	rVB2	1039	1250	0.11%	0.015%
33	18.053	2491	2496	2500	rBV3	2701	4361	0.39%	0.053%
34	18.100	2500	2504	2508	rVV2	7529	9501	0.86%	0.115%
35	18.330	2539	2543	2548	rBV3	3019	4697	0.42%	0.057%
36	18.400	2551	2555	2560	rVB2	1248	2064	0.19%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054035.D
 Acq On : 24 Jun 2022 5:59
 Operator : CG/JU
 Sample : N3395-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.064	2665	2668	2670	rBV3	952	1376	0.12%	0.017%
38	19.270	2697	2703	2706	rBV3	7164	9121	0.82%	0.111%
39	19.387	2717	2723	2730	rVB2	9270	13218	1.20%	0.161%
40	19.458	2730	2735	2742	rBV	7314	13047	1.18%	0.159%
41	19.593	2755	2758	2760	rBV4	2361	2669	0.24%	0.032%
42	19.652	2765	2768	2772	rBV3	1176	1481	0.13%	0.018%
43	19.822	2789	2797	2804	rBV	723859	1092297	98.76%	13.270%
44	20.010	2827	2829	2831	rBV2	1364	1444	0.13%	0.018%
45	20.174	2854	2857	2858	rBV	1749	1280	0.12%	0.016%
46	20.233	2865	2867	2870	rVB4	1968	1564	0.14%	0.019%
47	20.386	2889	2893	2894	rBV3	1258	1255	0.11%	0.015%
48	20.780	2958	2960	2965	rVB5	1817	1892	0.17%	0.023%
49	21.179	3025	3028	3030	rVB3	2918	2861	0.26%	0.035%
50	21.308	3048	3050	3053	rBV4	1757	1811	0.16%	0.022%
51	21.355	3054	3058	3064	rVB6	6810	11224	1.01%	0.136%
52	21.438	3067	3072	3075	rBV2	5298	8720	0.79%	0.106%
53	21.508	3082	3084	3086	rBV2	1443	1341	0.12%	0.016%
54	21.714	3112	3119	3129	rVB2	301810	522598	47.25%	6.349%
55	21.908	3149	3152	3153	rBV3	2214	2446	0.22%	0.030%
56	22.055	3175	3177	3181	rBV5	1946	1821	0.16%	0.022%
57	22.125	3187	3189	3190	rBV2	1806	1584	0.14%	0.019%
58	22.407	3234	3237	3242	rBV6	1909	2669	0.24%	0.032%
59	22.525	3254	3257	3263	rVB5	2868	4816	0.44%	0.059%
60	22.689	3282	3285	3288	rBV5	1868	2905	0.26%	0.035%
61	22.777	3299	3300	3303	rBV2	2867	1830	0.17%	0.022%
62	23.089	3351	3353	3354	rBV2	1704	1347	0.12%	0.016%
63	23.236	3372	3378	3385	rBV7	6145	12153	1.10%	0.148%
64	23.994	3505	3507	3508	rBV2	1655	1335	0.12%	0.016%
65	24.046	3511	3516	3526	rVB5	9082	21154	1.91%	0.257%
66	24.605	3610	3611	3613	rBV2	1548	1321	0.12%	0.016%
67	24.751	3624	3636	3649	rBV2	383415	1106048	100.00%	13.437%
68	24.975	3663	3674	3692	rVB2	171498	538087	48.65%	6.537%
69	25.192	3710	3711	3712	rBV	2299	1380	0.12%	0.017%
70	25.862	3823	3825	3827	rBV3	1468	1262	0.11%	0.015%
71	26.021	3850	3852	3855	rBV4	1501	1168	0.11%	0.014%
72	26.925	4004	4006	4009	rVB4	1577	1365	0.12%	0.017%
73	27.554	4104	4113	4122	rVB8	8689	29535	2.67%	0.359%
74	28.112	4206	4208	4209	rBV	2279	1475	0.13%	0.018%
75	28.535	4278	4280	4281	rBV	1815	1296	0.12%	0.016%
76	28.617	4292	4294	4297	rBV4	1824	2507	0.23%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054035.D
 Acq On : 24 Jun 2022 5:59
 Operator : CG/JU
 Sample : N3395-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	28.712	4308	4310	4311	rBV2	1656	1188	0.11%	0.014%
78	29.187	4388	4391	4393	rBV3	2844	4326	0.39%	0.053%
79	29.452	4434	4436	4437	rBV2	1639	1125	0.10%	0.014%
80	30.468	4607	4609	4610	rBV	2128	1272	0.12%	0.015%
81	30.633	4633	4637	4639	rVB4	1426	1743	0.16%	0.021%
82	30.656	4639	4641	4644	rBV3	1895	1536	0.14%	0.019%
83	30.803	4664	4666	4667	rBV	1556	1226	0.11%	0.015%
84	31.003	4698	4700	4703	rBV3	1851	1921	0.17%	0.023%
85	31.214	4734	4736	4738	rBV2	2385	2202	0.20%	0.027%
86	32.419	4940	4941	4944	rBV3	1742	2217	0.20%	0.027%
87	32.472	4948	4950	4953	rBV3	1818	1968	0.18%	0.024%




Sum of corrected areas: 8231152

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054035.D
Acq On : 24 Jun 2022 5:59
Operator : CG/JU
Sample : N3395-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0162

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

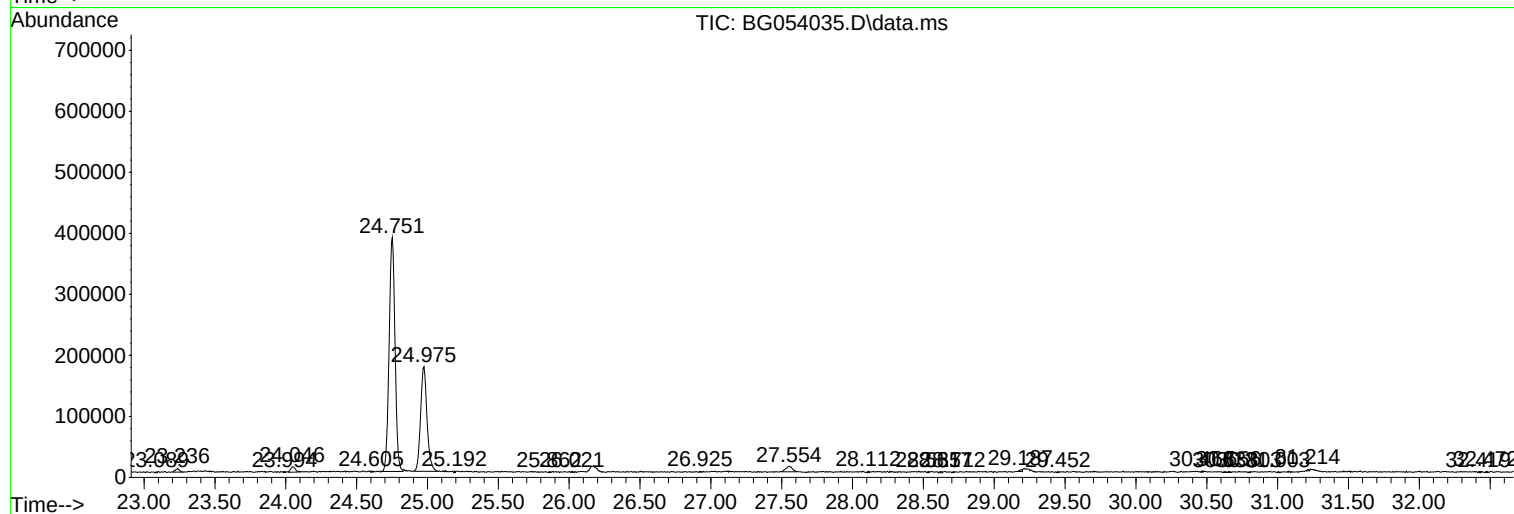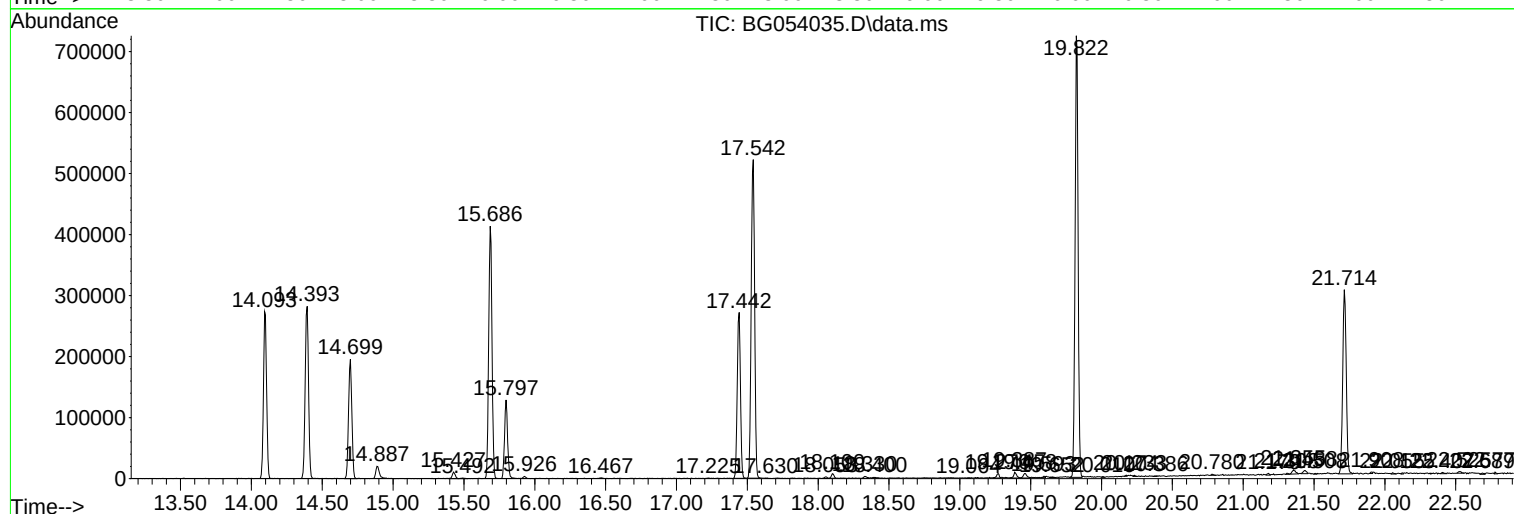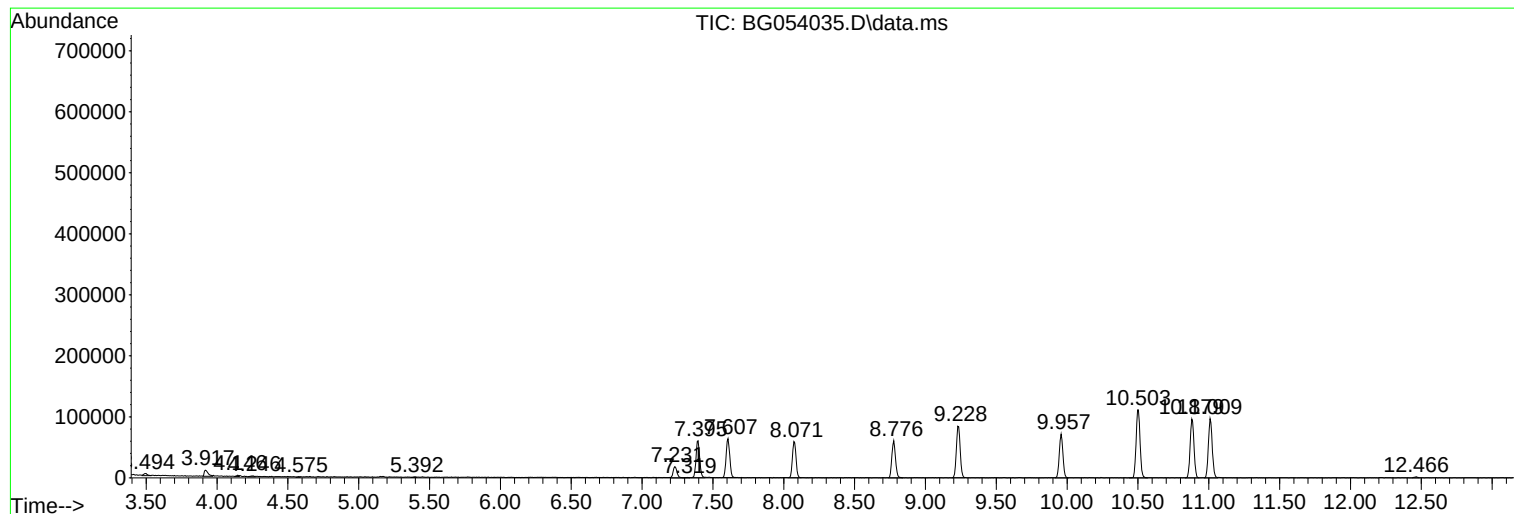

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054035.D
Acq On : 24 Jun 2022 5:59
Operator : CG/JU
Sample : N3395-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0162

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054035.D
Acq On : 24 Jun 2022 5:59
Operator : CG/JU
Sample : N3395-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0162

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------