

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054036.D
 Acq On : 24 Jun 2022 6:38
 Operator : CG/JU
 Sample : N3400-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.493	14	18	22	rBV3	3718	5397	0.49%	0.060%
2	3.910	87	89	101	rBV	20998	40386	3.64%	0.452%
3	4.151	125	130	135	rVB4	1812	3076	0.28%	0.034%
4	4.251	143	147	155	rVB4	1692	3539	0.32%	0.040%
5	5.167	298	303	306	rBV4	1098	1735	0.16%	0.019%
6	5.420	343	346	350	rBV2	795	1389	0.13%	0.016%
7	5.573	369	372	375	rBV2	728	1199	0.11%	0.013%
8	7.230	649	654	669	rVB2	20417	37691	3.40%	0.422%
9	7.394	675	682	689	rBV	66254	116248	10.49%	1.302%
10	7.606	711	718	728	rBV	69706	123122	11.11%	1.379%
11	8.070	790	797	806	rBV	75695	136805	12.34%	1.532%
12	8.775	911	917	927	rVB2	59938	107155	9.67%	1.200%
13	9.233	987	995	1006	rVB	90443	168976	15.25%	1.892%
14	9.956	1112	1118	1128	rVB	74851	135502	12.23%	1.517%
15	10.502	1204	1211	1220	rBV	114180	215033	19.40%	2.408%
16	10.884	1268	1276	1285	rBB	123169	230350	20.78%	2.579%
17	11.008	1290	1297	1308	rBV	106132	200368	18.08%	2.244%
18	12.459	1541	1544	1552	rBB3	1859	3109	0.28%	0.035%
19	14.098	1815	1823	1830	rBV	293819	448489	40.47%	5.022%
20	14.392	1866	1873	1881	rBV	295193	492306	44.42%	5.512%
21	14.697	1917	1925	1932	rBV	249509	395178	35.66%	4.425%
22	14.891	1952	1958	1968	rBV2	17992	33531	3.03%	0.375%
23	15.684	2087	2093	2103	rBV	439535	713049	64.34%	7.984%
24	15.796	2107	2112	2121	rBV	122580	188372	17.00%	2.109%
25	15.925	2130	2134	2140	rVB	3451	4936	0.45%	0.055%
26	16.472	2224	2227	2230	rBV3	1321	1878	0.17%	0.021%
27	16.989	2313	2315	2321	rVB	662	1119	0.10%	0.013%
28	17.235	2353	2357	2360	rBV	728	1145	0.10%	0.013%
29	17.441	2385	2392	2399	rBV	350840	540234	48.74%	6.049%
30	17.541	2401	2409	2419	rVV	538944	848149	76.52%	9.497%
31	17.623	2419	2423	2428	rVB4	1806	2236	0.20%	0.025%
32	18.105	2499	2505	2509	rBV	8081	10314	0.93%	0.115%
33	18.328	2539	2543	2550	rBV4	2509	4440	0.40%	0.050%
34	18.399	2550	2555	2558	rVB2	1815	2958	0.27%	0.033%
35	19.392	2716	2724	2729	rBV4	7727	11847	1.07%	0.133%
36	19.462	2731	2736	2740	rBV	6652	9755	0.88%	0.109%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054036.D
 Acq On : 24 Jun 2022 6:38
 Operator : CG/JU
 Sample : N3400-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.562	2751	2753	2758	rBV3	998	1224	0.11%	0.014%
38	19.603	2758	2760	2764	rBV3	1032	1623	0.15%	0.018%
39	19.733	2780	2782	2787	rBV3	1350	2093	0.19%	0.023%
40	19.827	2789	2798	2807	rBV	743680	1108335	100.00%	12.410%
41	20.203	2859	2862	2867	rBV6	1363	2483	0.22%	0.028%
42	20.308	2875	2880	2881	rBV4	997	1270	0.11%	0.014%
43	20.784	2959	2961	2966	rVB5	2024	2413	0.22%	0.027%
44	20.908	2980	2982	2984	rBV3	1246	1152	0.10%	0.013%
45	21.354	3054	3058	3062	rBV6	6185	10340	0.93%	0.116%
46	21.436	3068	3072	3076	rVB3	3878	5420	0.49%	0.061%
47	21.542	3088	3090	3092	rBV3	1695	1417	0.13%	0.016%
48	21.566	3092	3094	3096	rBV2	1708	1639	0.15%	0.018%
49	21.713	3112	3119	3131	rBV2	386831	669106	60.37%	7.492%
50	22.324	3221	3223	3225	rBV4	1451	1379	0.12%	0.015%
51	22.535	3255	3259	3263	rVB6	3333	6003	0.54%	0.067%
52	23.058	3346	3348	3351	rBV4	1434	1360	0.12%	0.015%
53	23.105	3355	3356	3359	rBV3	1786	1994	0.18%	0.022%
54	23.176	3366	3368	3369	rBV2	2080	1366	0.12%	0.015%
55	23.234	3372	3378	3384	rVV7	6369	12151	1.10%	0.136%
56	24.051	3512	3517	3525	rVB7	7421	18411	1.66%	0.206%
57	24.468	3585	3588	3590	rBV3	1806	1995	0.18%	0.022%
58	24.750	3624	3636	3649	rBV2	366645	1099357	99.19%	12.309%
59	24.979	3663	3675	3693	rVB2	213993	675224	60.92%	7.560%
60	25.532	3767	3769	3771	rBV3	1553	1349	0.12%	0.015%
61	26.008	3848	3850	3852	rBV3	1446	1383	0.12%	0.015%
62	26.172	3872	3878	3887	rVB7	8000	21582	1.95%	0.242%
63	26.248	3889	3891	3896	rBV3	1671	2456	0.22%	0.027%
64	27.400	4085	4087	4088	rBV2	1497	1169	0.11%	0.013%
65	27.559	4105	4114	4120	rBV7	6732	20919	1.89%	0.234%
66	28.029	4192	4194	4198	rBV3	1633	2674	0.24%	0.030%
67	28.675	4302	4304	4306	rBV3	1678	1433	0.13%	0.016%
68	30.761	4657	4659	4663	rBV4	1573	1568	0.14%	0.018%
69	30.902	4681	4683	4685	rVB2	1828	1332	0.12%	0.015%
70	31.207	4733	4735	4737	rBV3	1931	1956	0.18%	0.022%
71	31.460	4777	4778	4783	rBV5	1656	2705	0.24%	0.030%
72	31.642	4807	4809	4813	rBV4	1550	1727	0.16%	0.019%




Sum of corrected areas: 8931024

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054036.D
Acq On : 24 Jun 2022 6:38
Operator : CG/JU
Sample : N3400-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

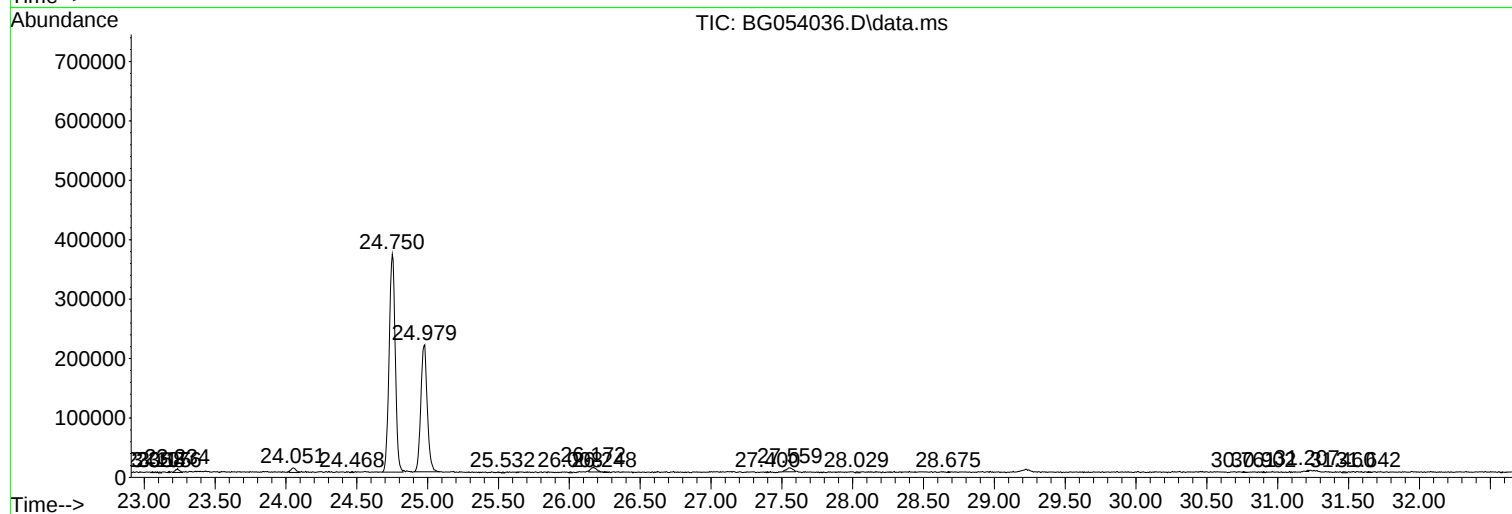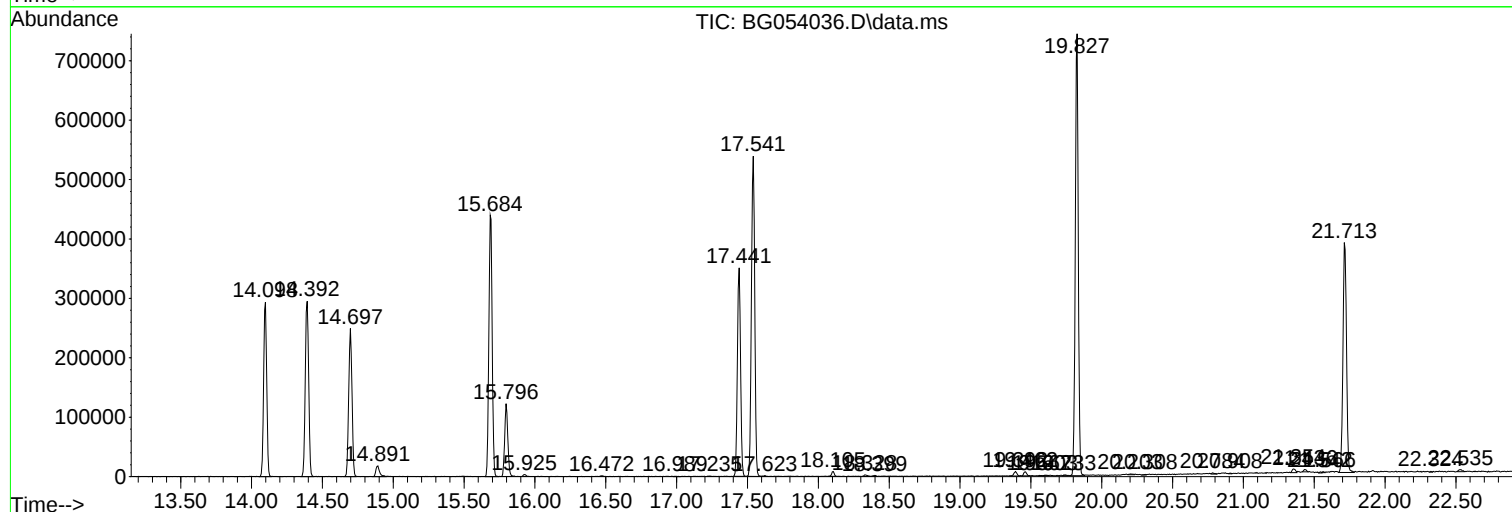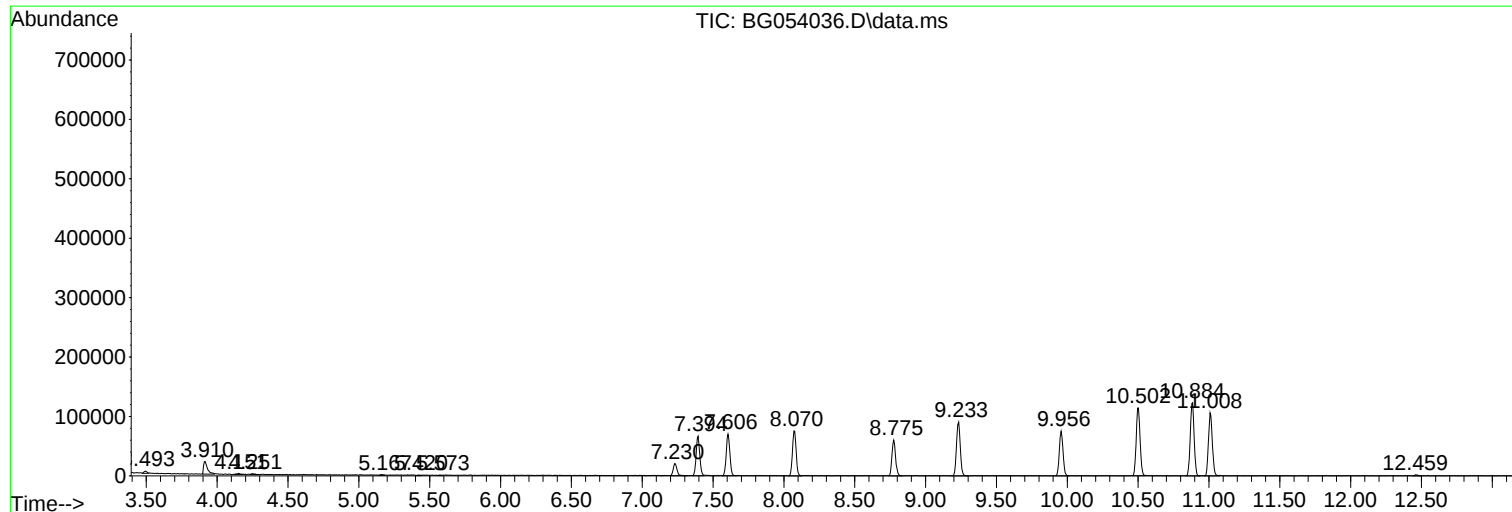

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054036.D
Acq On : 24 Jun 2022 6:38
Operator : CG/JU
Sample : N3400-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054036.D
Acq On : 24 Jun 2022 6:38
Operator : CG/JU
Sample : N3400-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc