

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054038.D
 Acq On : 24 Jun 2022 7:55
 Operator : CG/JU
 Sample : N3395-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.494	14	18	25	rVB3	6832	11277	1.01%	0.124%
2	3.641	41	43	49	rVB3	958	1123	0.10%	0.012%
3	3.912	86	89	104	rBV	19968	37852	3.38%	0.417%
4	4.152	126	130	137	rVB5	2572	4170	0.37%	0.046%
5	4.252	143	147	149	rBV2	1259	1778	0.16%	0.020%
6	5.163	300	302	309	rVB4	1551	1918	0.17%	0.021%
7	7.231	647	654	661	rBV	21717	39060	3.49%	0.430%
8	7.396	675	682	691	rBV	73447	133748	11.95%	1.472%
9	7.607	710	718	727	rBV	74381	139375	12.45%	1.534%
10	8.071	790	797	805	rVB	70255	127975	11.44%	1.408%
11	8.776	908	917	929	rBV	72070	129365	11.56%	1.424%
12	9.229	986	994	1005	rBV	102929	193572	17.30%	2.130%
13	9.957	1111	1118	1126	rBV	83983	154651	13.82%	1.702%
14	10.498	1202	1210	1222	rBV	132251	251774	22.50%	2.771%
15	10.880	1267	1275	1283	rBV	115837	212640	19.00%	2.340%
16	11.009	1289	1297	1306	rBV	117508	224074	20.02%	2.466%
17	12.460	1540	1544	1550	rVB2	1886	3116	0.28%	0.034%
18	13.524	1721	1725	1728	rBV3	931	1288	0.12%	0.014%
19	14.094	1816	1822	1829	rBV	316781	475984	42.53%	5.238%
20	14.393	1865	1873	1881	rBV	331108	550618	49.20%	6.059%
21	14.699	1918	1925	1932	rBV	223464	363622	32.49%	4.002%
22	14.887	1951	1957	1968	rBV2	17567	33979	3.04%	0.374%
23	15.087	1989	1991	1996	rVB2	754	1137	0.10%	0.013%
24	15.428	2046	2049	2053	rVB2	1851	2709	0.24%	0.030%
25	15.686	2084	2093	2100	rBV	477510	762109	68.10%	8.387%
26	15.798	2106	2112	2122	rBV	130835	197891	17.68%	2.178%
27	15.921	2130	2133	2140	rVB2	4478	6715	0.60%	0.074%
28	16.473	2223	2227	2230	rBV2	1800	1895	0.17%	0.021%
29	16.926	2301	2304	2311	rVB2	866	1841	0.16%	0.020%
30	17.437	2385	2391	2399	rBV	311209	492457	44.00%	5.419%
31	17.537	2402	2408	2417	rVV	545841	879631	78.60%	9.680%
32	18.101	2499	2504	2509	rBV2	6418	8296	0.74%	0.091%
33	18.330	2539	2543	2546	rBV2	1847	2547	0.23%	0.028%
34	18.401	2551	2555	2560	rVB2	1393	2174	0.19%	0.024%
35	19.393	2718	2724	2730	rVB3	7923	12186	1.09%	0.134%
36	19.458	2730	2735	2739	rVV2	7366	11548	1.03%	0.127%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054038.D
 Acq On : 24 Jun 2022 7:55
 Operator : CG/JU
 Sample : N3395-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.493	2739	2741	2745	rVB3	2452	3138	0.28%	0.035%
38	19.599	2757	2759	2762	rBV3	1022	1436	0.13%	0.016%
39	19.740	2778	2783	2789	rVB5	2156	3548	0.32%	0.039%
40	19.822	2789	2797	2809	rBV	755188	1116885	99.80%	12.291%
41	20.069	2835	2839	2843	rBV3	748	1345	0.12%	0.015%
42	20.163	2851	2855	2858	rBV4	1064	1306	0.12%	0.014%
43	20.410	2893	2897	2899	rBV3	850	1361	0.12%	0.015%
44	20.457	2901	2905	2906	rVB3	1153	1269	0.11%	0.014%
45	20.733	2951	2952	2956	rBV4	1705	1616	0.14%	0.018%
46	20.780	2956	2960	2963	rVV5	3010	3323	0.30%	0.037%
47	20.809	2963	2965	2967	rVB3	1367	1131	0.10%	0.012%
48	20.839	2967	2970	2971	rBV3	1615	1683	0.15%	0.019%
49	20.992	2993	2996	2998	rBV4	1144	1598	0.14%	0.018%
50	21.138	3018	3021	3023	rBV3	1889	2488	0.22%	0.027%
51	21.362	3054	3059	3062	rBV4	5689	9812	0.88%	0.108%
52	21.415	3065	3068	3069	rBV3	1742	1747	0.16%	0.019%
53	21.438	3069	3072	3081	rVB7	4355	8121	0.73%	0.089%
54	21.603	3097	3100	3104	rVB5	1528	1860	0.17%	0.020%
55	21.714	3112	3119	3130	rBV	352082	590005	52.72%	6.493%
56	21.902	3149	3151	3156	rVB5	2605	3918	0.35%	0.043%
57	22.449	3243	3244	3247	rBV3	1621	1898	0.17%	0.021%
58	22.525	3255	3257	3261	rVB4	3548	4229	0.38%	0.047%
59	23.236	3373	3378	3383	rVB6	5052	9952	0.89%	0.110%
60	23.401	3402	3406	3407	rBV3	1793	2130	0.19%	0.023%
61	23.418	3407	3409	3411	rBV3	1494	1733	0.15%	0.019%
62	23.982	3502	3505	3506	rBV2	1544	1450	0.13%	0.016%
63	24.053	3511	3517	3526	rVB4	8861	21057	1.88%	0.232%
64	24.282	3554	3556	3560	rBV5	1446	1766	0.16%	0.019%
65	24.605	3609	3611	3615	rBV5	1804	2914	0.26%	0.032%
66	24.746	3624	3635	3652	rBV2	379262	1119130	100.00%	12.316%
67	24.975	3663	3674	3691	rVB	198453	605820	54.13%	6.667%
68	26.162	3871	3876	3886	rVB6	11203	28316	2.53%	0.312%
69	27.149	4042	4044	4047	rVB3	1618	1174	0.10%	0.013%
70	27.549	4104	4112	4123	rVB5	9651	35865	3.20%	0.395%
71	29.200	4391	4393	4394	rBV2	2945	2117	0.19%	0.023%
72	29.699	4476	4478	4480	rBV3	1698	1888	0.17%	0.021%
73	30.545	4620	4622	4624	rVB3	2036	1299	0.12%	0.014%
74	30.604	4630	4632	4633	rVB2	1773	1236	0.11%	0.014%
75	30.621	4633	4635	4636	rBV2	1373	1283	0.11%	0.014%
76	30.745	4654	4656	4659	rBV4	1377	1483	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054038.D
Acq On : 24 Jun 2022 7:55
Operator : CG/JU
Sample : N3395-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0160

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	31.432	4771	4773	4775	rBV	1365	1126	0.10%	0.012%
78	31.538	4789	4791	4793	rVB2	2425	1950	0.17%	0.021%
79	31.562	4793	4795	4797	rBV2	2188	2095	0.19%	0.023%
80	31.708	4819	4820	4822	rBV	1632	1301	0.12%	0.014%




Sum of corrected areas: 9086897

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054038.D
Acq On : 24 Jun 2022 7:55
Operator : CG/JU
Sample : N3395-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

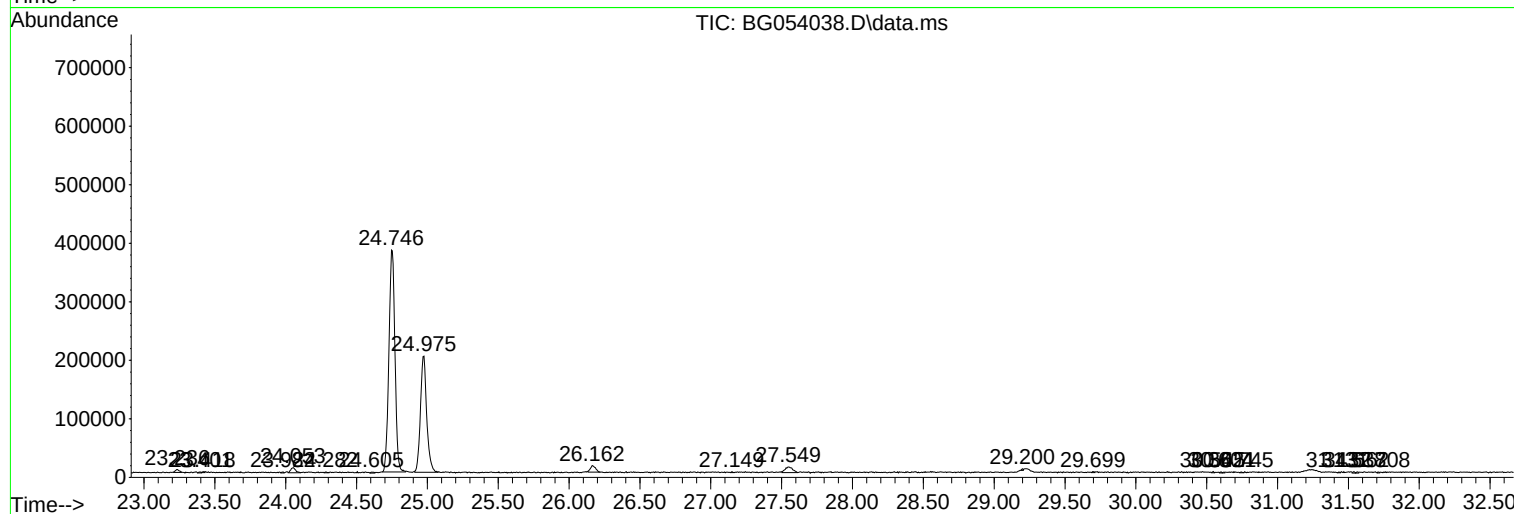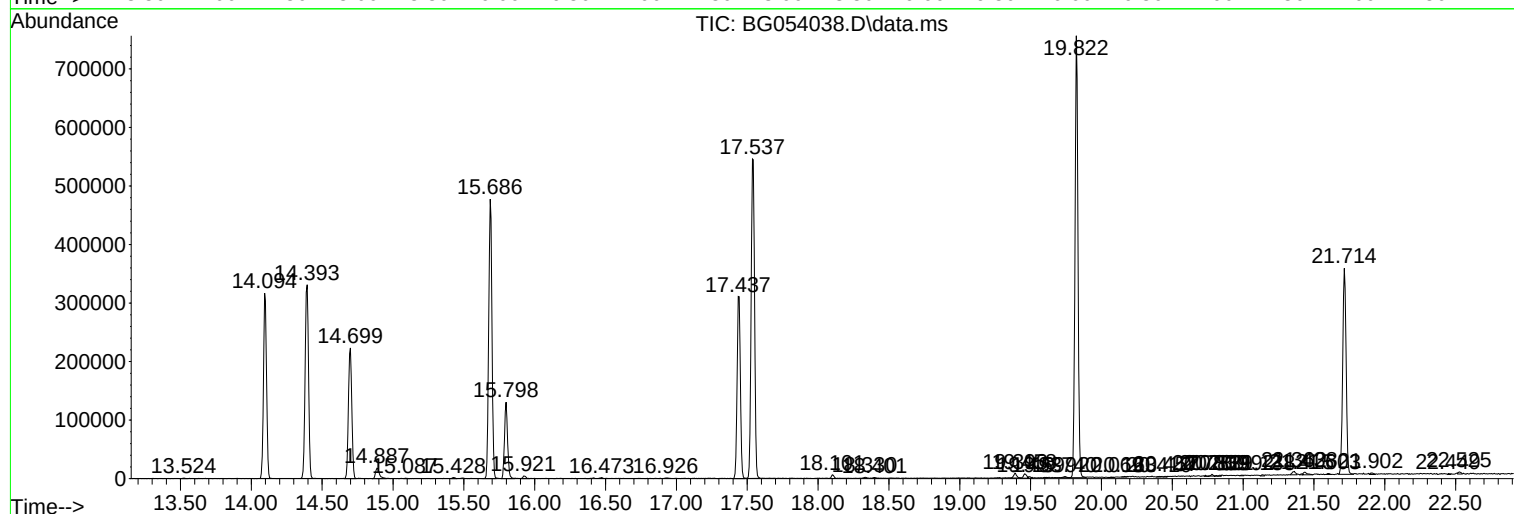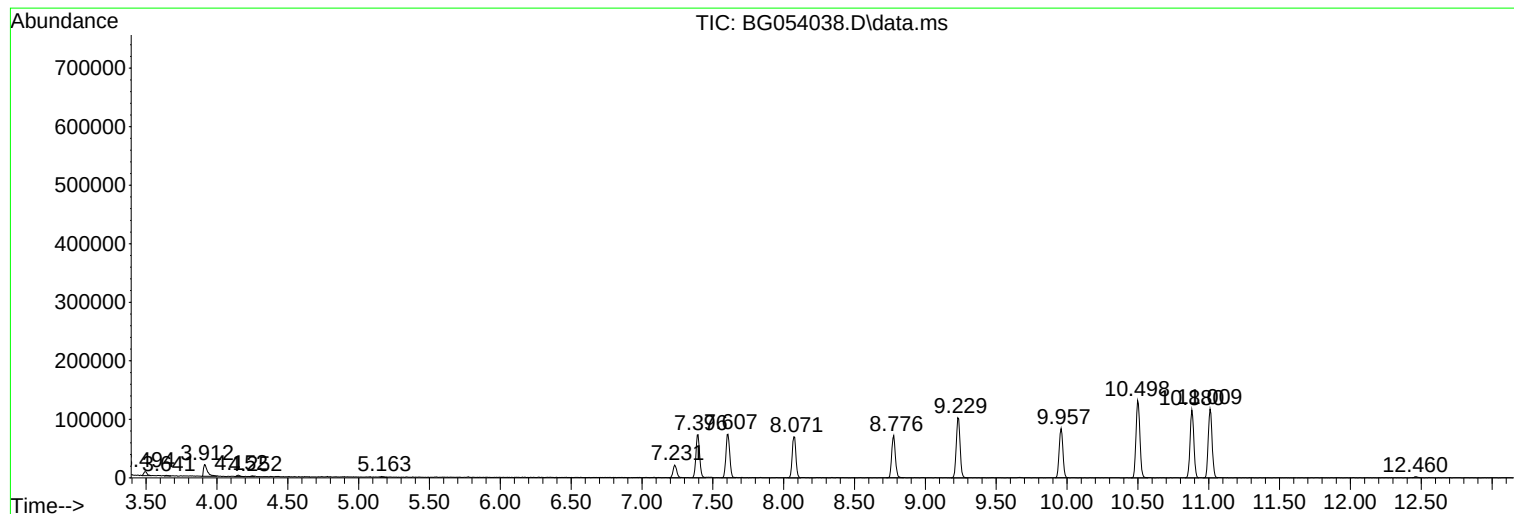

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054038.D
Acq On : 24 Jun 2022 7:55
Operator : CG/JU
Sample : N3395-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054038.D
Acq On : 24 Jun 2022 7:55
Operator : CG/JU
Sample : N3395-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------