

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054039.D
 Acq On : 24 Jun 2022 8:34
 Operator : CG/JU
 Sample : N3395-17
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0164

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.497	13	18	21	rBV2	4256	6165	0.51%	0.072%
2	3.920	86	90	101	rBV2	11689	22684	1.88%	0.264%
3	4.149	125	129	134	rVB3	2902	4280	0.35%	0.050%
4	5.160	298	301	306	rVB3	1303	1721	0.14%	0.020%
5	5.771	402	405	408	rBV4	945	1391	0.12%	0.016%
6	7.228	647	653	662	rBV	21706	38164	3.16%	0.443%
7	7.392	674	681	689	rBV	71171	123786	10.26%	1.438%
8	7.604	711	717	729	rVB	70557	130288	10.79%	1.514%
9	8.074	791	797	805	rVB	62055	107450	8.90%	1.249%
10	8.773	908	916	925	rBV	67459	121443	10.06%	1.411%
11	9.231	987	994	1003	rBV	97383	177711	14.72%	2.065%
12	9.954	1110	1117	1125	rBV	75802	142353	11.79%	1.654%
13	10.500	1201	1210	1219	rBV	122341	230762	19.12%	2.681%
14	10.882	1266	1275	1285	rBV	95822	178298	14.77%	2.072%
15	11.012	1290	1297	1306	rBV	106329	204928	16.98%	2.381%
16	12.463	1539	1544	1549	rVB2	1576	2797	0.23%	0.032%
17	14.096	1814	1822	1831	rBV	306321	460933	38.19%	5.356%
18	14.390	1865	1872	1881	rBV	307701	509262	42.19%	5.917%
19	14.696	1918	1924	1932	rVB	193593	305829	25.34%	3.554%
20	14.889	1952	1957	1968	rBV2	21067	41822	3.46%	0.486%
21	15.430	2045	2049	2052	rBV	1395	1340	0.11%	0.016%
22	15.495	2055	2060	2064	rBV2	802	1248	0.10%	0.015%
23	15.688	2084	2093	2102	rBV	467221	726990	60.23%	8.447%
24	15.794	2106	2111	2120	rVV	128515	207104	17.16%	2.406%
25	15.923	2130	2133	2138	rVV2	3750	5033	0.42%	0.058%
26	16.470	2222	2226	2230	rVB2	1743	2313	0.19%	0.027%
27	17.439	2380	2391	2400	rBV	272454	421892	34.95%	4.902%
28	17.539	2401	2408	2415	rVV2	559559	902711	74.79%	10.489%
29	18.103	2499	2504	2508	rVB3	954	1592	0.13%	0.018%
30	19.390	2718	2723	2728	rVB4	8161	12047	1.00%	0.140%
31	19.461	2730	2735	2740	rBV2	7505	11308	0.94%	0.131%
32	19.825	2790	2797	2806	rVV	819323	1184382	98.12%	13.762%
33	21.352	3056	3057	3061	rBV4	1844	2841	0.24%	0.033%
34	21.435	3067	3071	3075	rBV3	4937	6740	0.56%	0.078%
35	21.717	3112	3119	3126	rVB	308545	520887	43.15%	6.052%
36	23.233	3373	3377	3383	rVB5	3424	6307	0.52%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054039.D
 Acq On : 24 Jun 2022 8:34
 Operator : CG/JU
 Sample : N3395-17
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0164

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	24.049	3510	3516	3517	rBV6	5269	7371	0.61%	0.086%
38	24.537	3597	3599	3603	rBV5	2118	3097	0.26%	0.036%
39	24.754	3622	3636	3653	rBV2	406793	1207054	100.00%	14.025%
40	24.972	3663	3673	3692	rVB2	171637	532920	44.15%	6.192%
41	26.129	3868	3870	3872	rBV3	2323	2409	0.20%	0.028%
42	26.159	3872	3875	3876	rBV3	3729	4453	0.37%	0.052%
43	26.300	3895	3899	3900	rBV3	1728	1818	0.15%	0.021%
44	27.304	4067	4070	4075	rBV7	1770	2764	0.23%	0.032%
45	27.533	4103	4109	4110	rBV4	5202	7386	0.61%	0.086%
46	28.620	4292	4294	4296	rBV2	1484	1340	0.11%	0.016%
47	29.202	4391	4393	4395	rBV3	2038	2317	0.19%	0.027%
48	29.707	4477	4479	4482	rBV3	1674	1410	0.12%	0.016%
49	30.847	4672	4673	4675	rBV2	1528	1487	0.12%	0.017%
50	31.206	4732	4734	4736	rBV3	1835	2139	0.18%	0.025%
51	32.257	4911	4913	4915	rBV	2038	1515	0.13%	0.018%




Sum of corrected areas: 8606282

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054039.D
Acq On : 24 Jun 2022 8:34
Operator : CG/JU
Sample : N3395-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0164

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

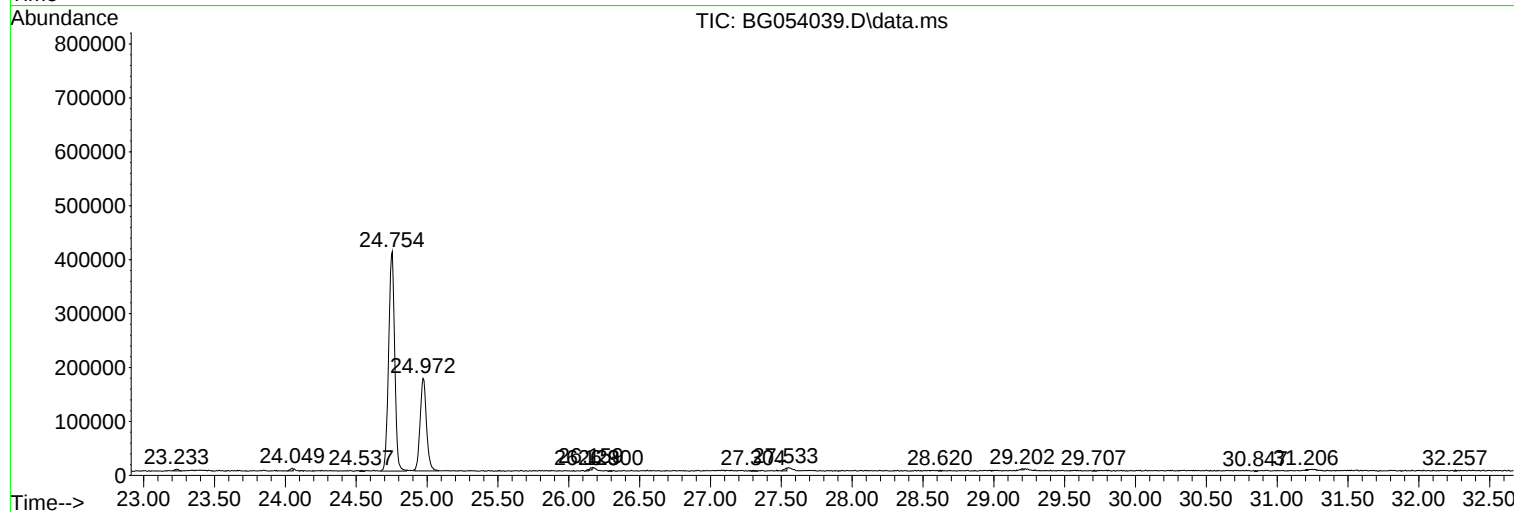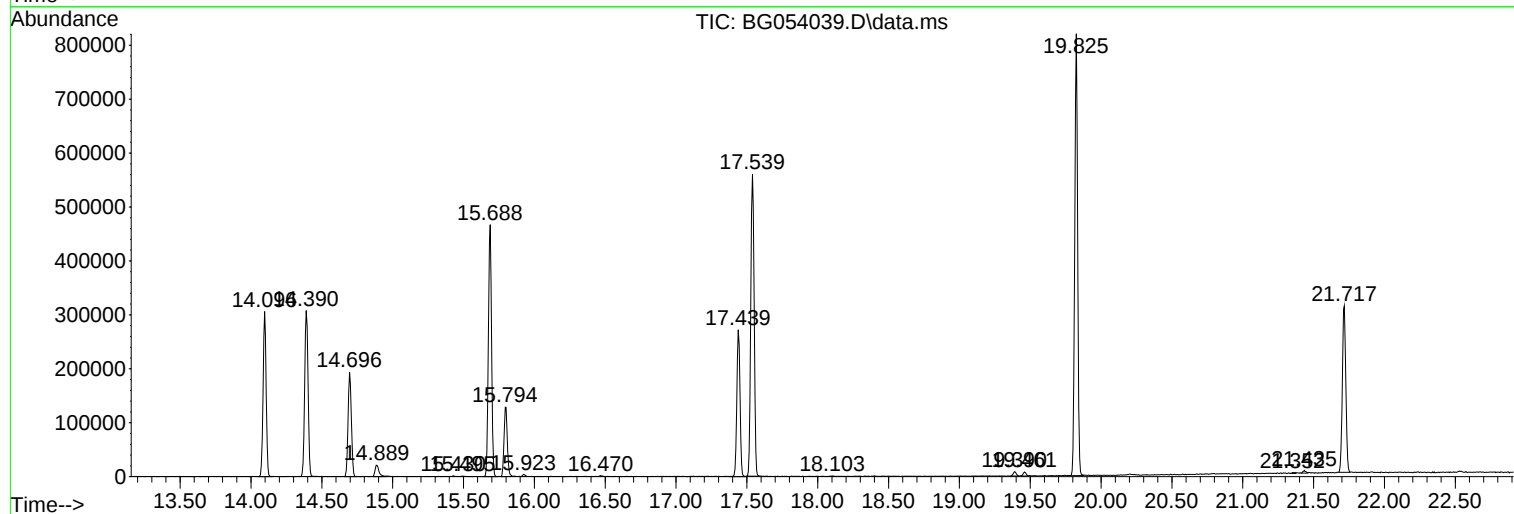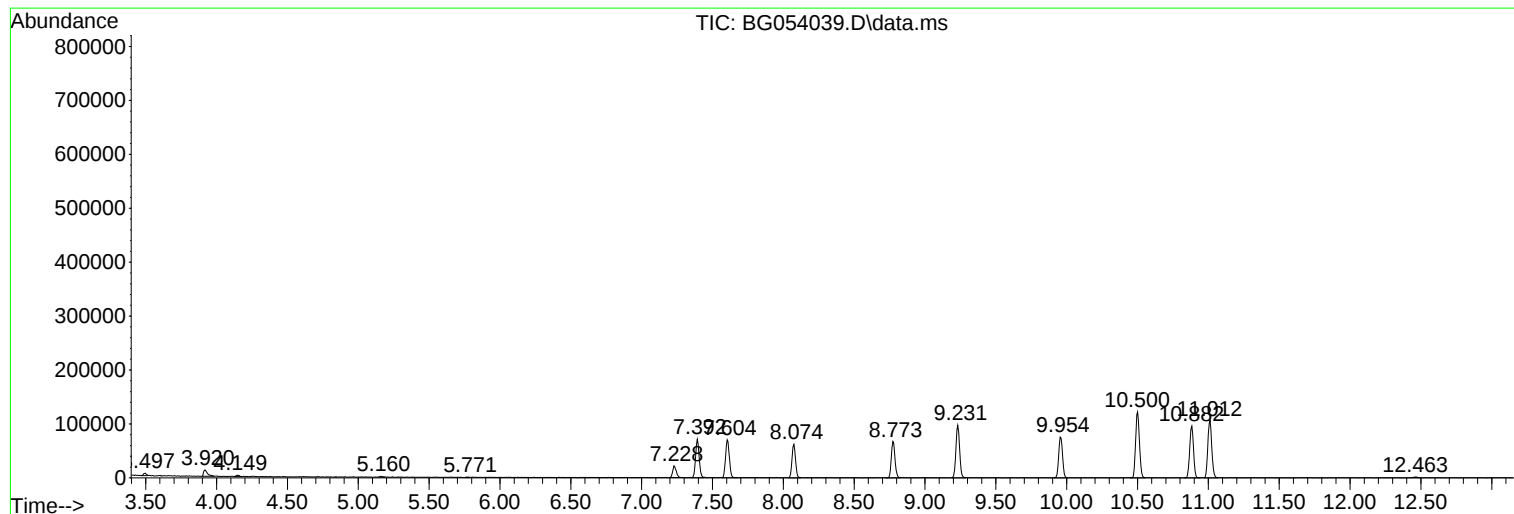

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054039.D
Acq On : 24 Jun 2022 8:34
Operator : CG/JU
Sample : N3395-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0164

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054039.D
Acq On : 24 Jun 2022 8:34
Operator : CG/JU
Sample : N3395-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0164

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc