

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054045.D
 Acq On : 24 Jun 2022 13:06
 Operator : CG/JU
 Sample : N3358-20
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.493	14	18	27	rVB3	5411	9708	0.59%	0.085%
2	3.911	86	89	109	rVB2	30655	59709	3.64%	0.524%
3	4.151	126	130	135	rVB3	2178	3980	0.24%	0.035%
4	4.251	142	147	151	rVB4	2095	3204	0.20%	0.028%
5	7.230	647	654	662	rBV	62739	112576	6.86%	0.989%
6	7.395	675	682	693	rBV	100874	181804	11.08%	1.597%
7	7.606	711	718	725	rBV	58578	101594	6.19%	0.892%
8	8.070	790	797	805	rBV	72074	128780	7.85%	1.131%
9	8.775	908	917	927	rBV	82036	150793	9.19%	1.325%
10	9.234	986	995	1007	rBV	137280	262721	16.02%	2.308%
11	9.956	1112	1118	1126	rBV2	49723	91391	5.57%	0.803%
12	10.497	1204	1210	1220	rBV	85945	163028	9.94%	1.432%
13	10.879	1266	1275	1283	rBV	118456	216322	13.19%	1.900%
14	11.008	1290	1297	1306	rBV	191965	364607	22.23%	3.203%
15	12.465	1541	1545	1548	rBV	1306	1765	0.11%	0.016%
16	14.099	1815	1823	1830	rBV	415620	637549	38.87%	5.600%
17	14.392	1865	1873	1883	rBV	453353	747942	45.60%	6.570%
18	14.698	1918	1925	1934	rVB	237750	365317	22.27%	3.209%
19	14.886	1950	1957	1970	rBV	57240	104439	6.37%	0.917%
20	15.426	2046	2049	2055	rVB2	2799	2958	0.18%	0.026%
21	15.685	2086	2093	2103	rVB	633036	1029485	62.77%	9.043%
22	15.797	2107	2112	2121	rBV	61796	95754	5.84%	0.841%
23	15.926	2129	2134	2139	rVB	5839	9141	0.56%	0.080%
24	16.466	2220	2226	2233	rBB3	2190	3273	0.20%	0.029%
25	17.442	2385	2392	2400	rVV	311356	502000	30.61%	4.409%
26	17.542	2401	2409	2420	rVB	781011	1238642	75.52%	10.880%
27	17.718	2435	2439	2442	rVB2	2024	2889	0.18%	0.025%
28	18.399	2550	2555	2558	rVB	1377	1907	0.12%	0.017%
29	19.387	2720	2723	2727	rBV3	7709	10650	0.65%	0.094%
30	19.463	2731	2736	2742	rVB2	6644	10249	0.62%	0.090%
31	19.716	2774	2779	2781	rBV2	3014	3610	0.22%	0.032%
32	19.745	2781	2784	2786	rVB2	1978	1937	0.12%	0.017%
33	19.827	2790	2798	2805	rBV	1053063	1609802	98.15%	14.140%
34	20.221	2860	2865	2870	rVB4	1961	2958	0.18%	0.026%
35	20.779	2958	2960	2963	rBV4	1728	1966	0.12%	0.017%
36	21.355	3052	3058	3068	rBV8	9608	20016	1.22%	0.176%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054045.D
 Acq On : 24 Jun 2022 13:06
 Operator : CG/JU
 Sample : N3358-20
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	21.437	3068	3072	3073	rBV3	2420	3291	0.20%	0.029%
38	21.713	3111	3119	3129	rVV	360016	621638	37.90%	5.460%
39	22.530	3252	3258	3262	rBV7	4598	8677	0.53%	0.076%
40	23.229	3372	3377	3384	rVB4	7483	13338	0.81%	0.117%
41	23.705	3456	3458	3461	rBV4	1822	2057	0.13%	0.018%
42	23.840	3475	3481	3486	rVB7	4015	9058	0.55%	0.080%
43	23.934	3494	3497	3499	rBV3	1437	1793	0.11%	0.016%
44	24.052	3510	3517	3524	rVB3	12674	27938	1.70%	0.245%
45	24.363	3569	3570	3574	rBV2	1881	2403	0.15%	0.021%
46	24.751	3624	3636	3650	rBV2	555791	1640108	100.00%	14.406%
47	24.968	3662	3673	3689	rBV2	198177	644249	39.28%	5.659%
48	26.167	3869	3877	3887	rVB3	16851	49419	3.01%	0.434%
49	26.384	3910	3914	3917	rBV5	1678	3000	0.18%	0.026%
50	26.901	4000	4002	4005	rVB4	1929	2056	0.13%	0.018%
51	26.937	4005	4008	4009	rBV3	1815	1741	0.11%	0.015%
52	27.553	4101	4113	4123	rBV7	15507	57710	3.52%	0.507%
53	29.210	4385	4395	4406	rVB4	10110	37449	2.28%	0.329%
54	31.214	4734	4736	4740	rBV4	2482	4301	0.26%	0.038%




Sum of corrected areas: 11384692

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054045.D
Acq On : 24 Jun 2022 13:06
Operator : CG/JU
Sample : N3358-20
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4T3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

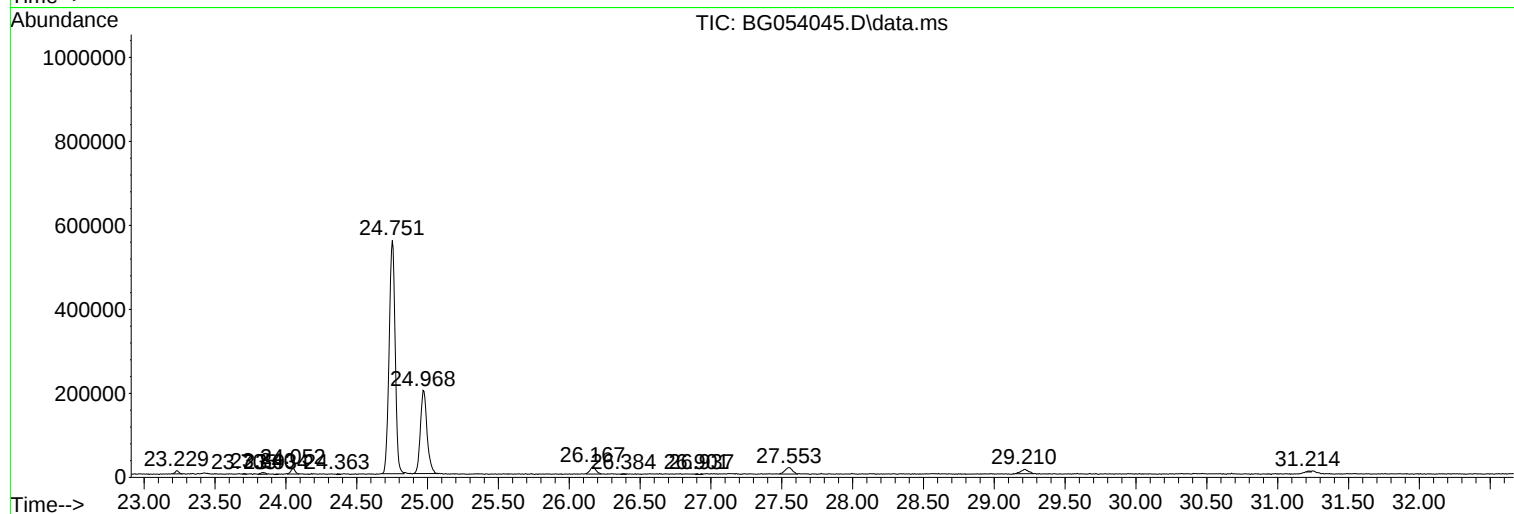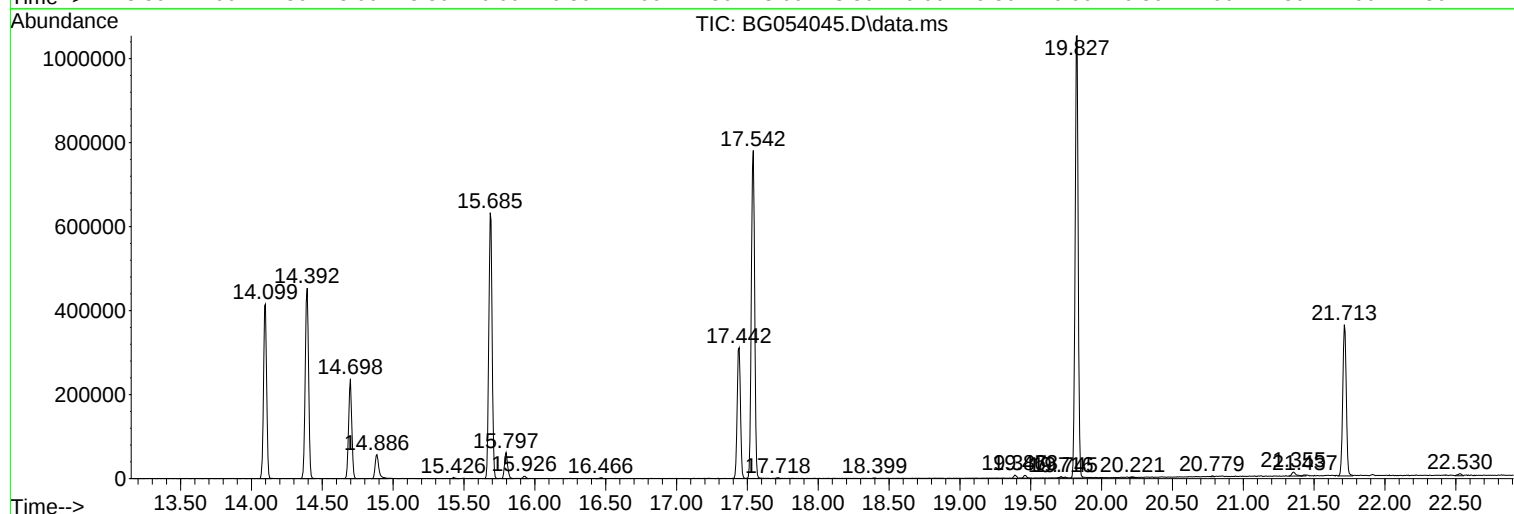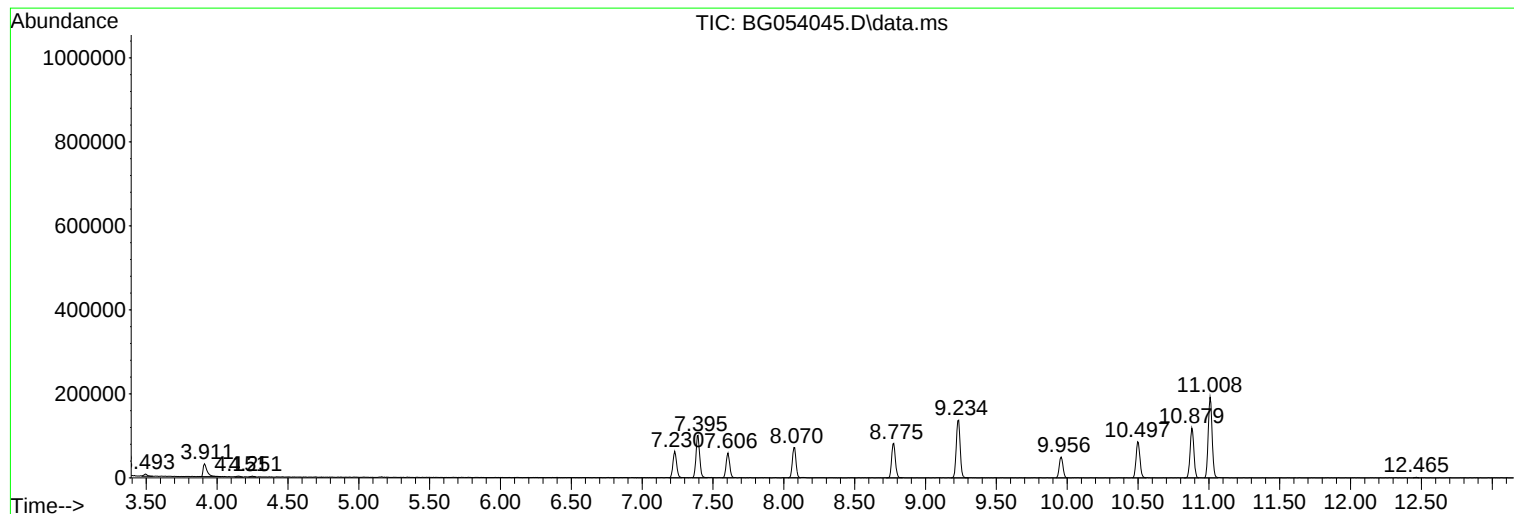

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054045.D
Acq On : 24 Jun 2022 13:06
Operator : CG/JU
Sample : N3358-20
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4T3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054045.D
Acq On : 24 Jun 2022 13:06
Operator : CG/JU
Sample : N3358-20
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4T3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc