

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054046.D
 Acq On : 24 Jun 2022 13:52
 Operator : CG/JU
 Sample : N3395-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.489	14	17	23	rVB3	3888	5318	0.49%	0.059%
2	3.918	87	90	99	rBV2	12991	25384	2.34%	0.281%
3	4.147	124	129	136	rBV4	2586	4376	0.40%	0.049%
4	4.253	142	147	150	rBV4	1899	2704	0.25%	0.030%
5	5.158	299	301	307	rBV3	1234	2122	0.20%	0.024%
6	7.232	648	654	661	rBV2	22164	38518	3.55%	0.427%
7	7.391	675	681	691	rBV	69789	121544	11.22%	1.348%
8	7.602	711	717	726	rVV	70769	126892	11.71%	1.407%
9	8.072	791	797	805	rVB2	77834	134080	12.37%	1.487%
10	8.777	910	917	926	rVB	69260	122198	11.28%	1.355%
11	9.230	986	994	1004	rBV	93263	174718	16.12%	1.938%
12	9.958	1109	1118	1127	rBV	76108	139820	12.90%	1.551%
13	10.499	1203	1210	1218	rBV	122306	229980	21.22%	2.550%
14	10.881	1267	1275	1284	rVB	127662	237560	21.92%	2.634%
15	11.010	1290	1297	1310	rBV	96610	184097	16.99%	2.042%
16	12.461	1540	1544	1552	rBB3	1946	3775	0.35%	0.042%
17	14.095	1816	1822	1830	rBV	297219	450802	41.60%	4.999%
18	14.394	1865	1873	1880	rBV	303469	512175	47.26%	5.680%
19	14.700	1917	1925	1932	rBB	253421	412738	38.09%	4.577%
20	14.888	1951	1957	1970	rBV2	19698	37258	3.44%	0.413%
21	15.428	2046	2049	2054	rVB2	4573	6001	0.55%	0.067%
22	15.687	2086	2093	2101	rBV	461246	711076	65.62%	7.885%
23	15.799	2107	2112	2120	rBV	122893	185037	17.07%	2.052%
24	15.928	2129	2134	2138	rBV3	3961	5707	0.53%	0.063%
25	16.474	2223	2227	2231	rBV3	1988	2890	0.27%	0.032%
26	17.438	2385	2391	2400	rVB	349070	561436	51.81%	6.226%
27	17.538	2400	2408	2420	rBV2	526347	850613	78.49%	9.433%
28	18.102	2499	2504	2510	rBV2	16124	19789	1.83%	0.219%
29	18.337	2540	2544	2545	rBV2	1759	1873	0.17%	0.021%
30	19.271	2697	2703	2707	rVB2	16050	20488	1.89%	0.227%
31	19.388	2719	2723	2728	rBV4	7909	12317	1.14%	0.137%
32	19.459	2731	2735	2741	rBV2	6339	9782	0.90%	0.108%
33	19.553	2749	2751	2755	rVB2	960	1260	0.12%	0.014%
34	19.606	2757	2760	2764	rVV3	1236	1665	0.15%	0.018%
35	19.741	2780	2783	2786	rBV3	2218	2777	0.26%	0.031%
36	19.823	2790	2797	2806	rVV	758832	1083692	100.00%	12.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054046.D
 Acq On : 24 Jun 2022 13:52
 Operator : CG/JU
 Sample : N3395-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.135	2848	2850	2852	rBV3	1817	1559	0.14%	0.017%
38	20.158	2852	2854	2856	rVV2	1258	1402	0.13%	0.016%
39	20.235	2865	2867	2870	rVB4	1378	1159	0.11%	0.013%
40	20.352	2885	2887	2890	rBV3	1311	1365	0.13%	0.015%
41	20.464	2902	2906	2907	rBV2	1388	1376	0.13%	0.015%
42	20.528	2914	2917	2918	rBV3	1260	1109	0.10%	0.012%
43	20.781	2957	2960	2963	rVB3	2447	2556	0.24%	0.028%
44	20.851	2970	2972	2976	rVB4	2013	2246	0.21%	0.025%
45	21.092	3010	3013	3015	rVB3	1517	1494	0.14%	0.017%
46	21.169	3023	3026	3027	rBV3	1671	1412	0.13%	0.016%
47	21.363	3053	3059	3063	rBV5	7612	13383	1.23%	0.148%
48	21.439	3068	3072	3079	rVB5	3639	7761	0.72%	0.086%
49	21.715	3112	3119	3129	rBV	410086	683080	63.03%	7.575%
50	21.921	3151	3154	3159	rVB6	1967	3168	0.29%	0.035%
51	22.297	3216	3218	3219	rBV2	1252	1090	0.10%	0.012%
52	22.532	3253	3258	3263	rBV4	3585	6891	0.64%	0.076%
53	23.237	3371	3378	3383	rBV4	5230	11802	1.09%	0.131%
54	23.960	3499	3501	3504	rBV3	1634	1579	0.15%	0.018%
55	24.054	3510	3517	3523	rBV6	7293	17412	1.61%	0.193%
56	24.312	3559	3561	3564	rBV3	1154	1347	0.12%	0.015%
57	24.753	3624	3636	3654	rBV2	363601	1079108	99.58%	11.967%
58	24.976	3662	3674	3690	rVB2	219568	683901	63.11%	7.584%
59	26.169	3869	3877	3887	rVB6	8901	25959	2.40%	0.288%
60	26.369	3909	3911	3914	rBV4	1407	1676	0.15%	0.019%
61	26.574	3944	3946	3949	rVB4	1918	1756	0.16%	0.019%
62	27.544	4105	4111	4112	rBV5	5495	8802	0.81%	0.098%
63	27.626	4123	4125	4128	rBV4	1456	1209	0.11%	0.013%
64	28.443	4262	4264	4267	rBV3	1525	2255	0.21%	0.025%
65	29.177	4386	4389	4390	rBV3	2536	2851	0.26%	0.032%
66	29.195	4390	4392	4393	rVV2	2183	1821	0.17%	0.020%
67	29.835	4500	4501	4502	rBV	2204	1148	0.11%	0.013%
68	32.121	4888	4890	4893	rBV3	1443	1435	0.13%	0.016%




Sum of corrected areas: 9017574

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054046.D
Acq On : 24 Jun 2022 13:52
Operator : CG/JU
Sample : N3395-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0166

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

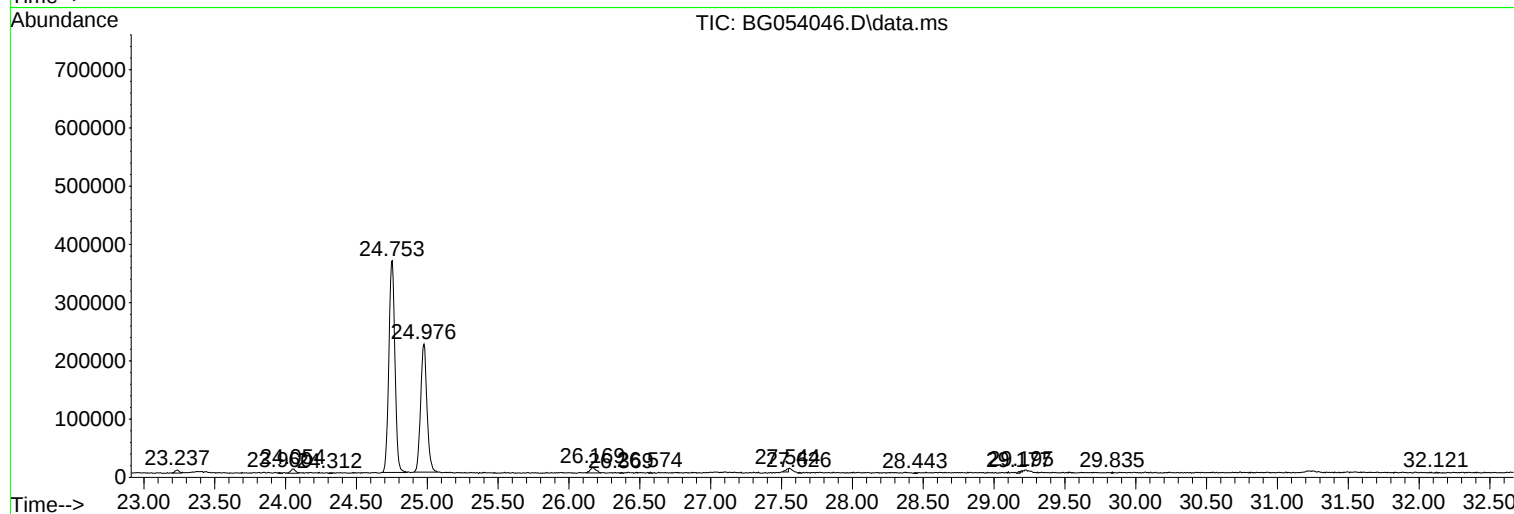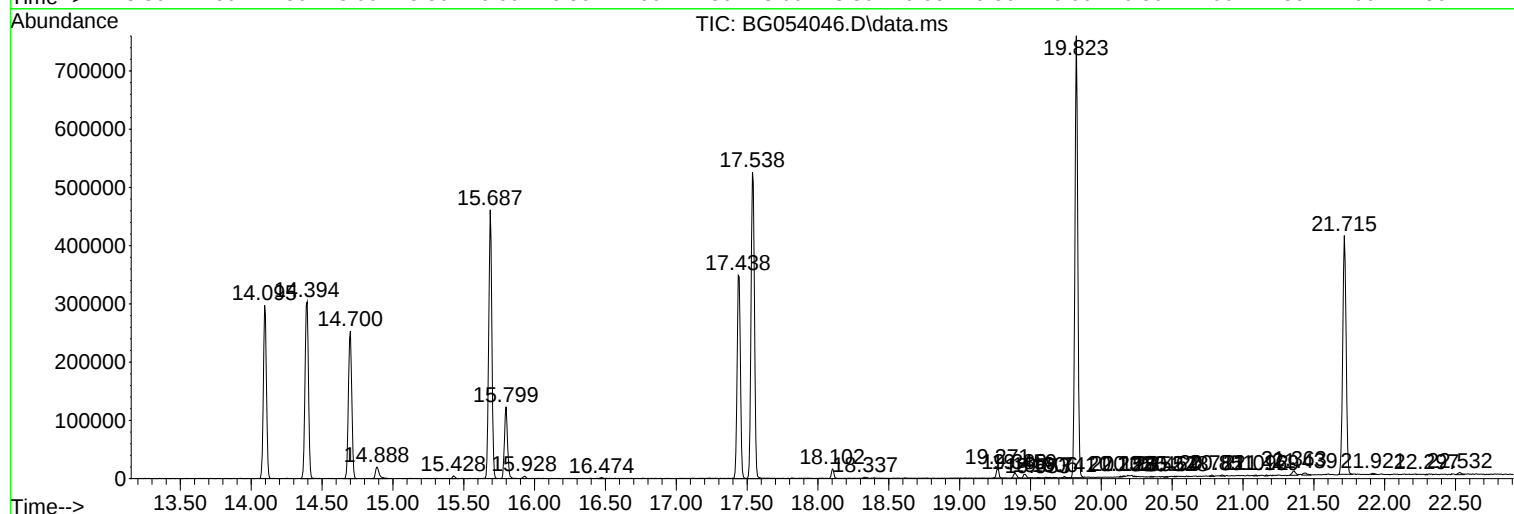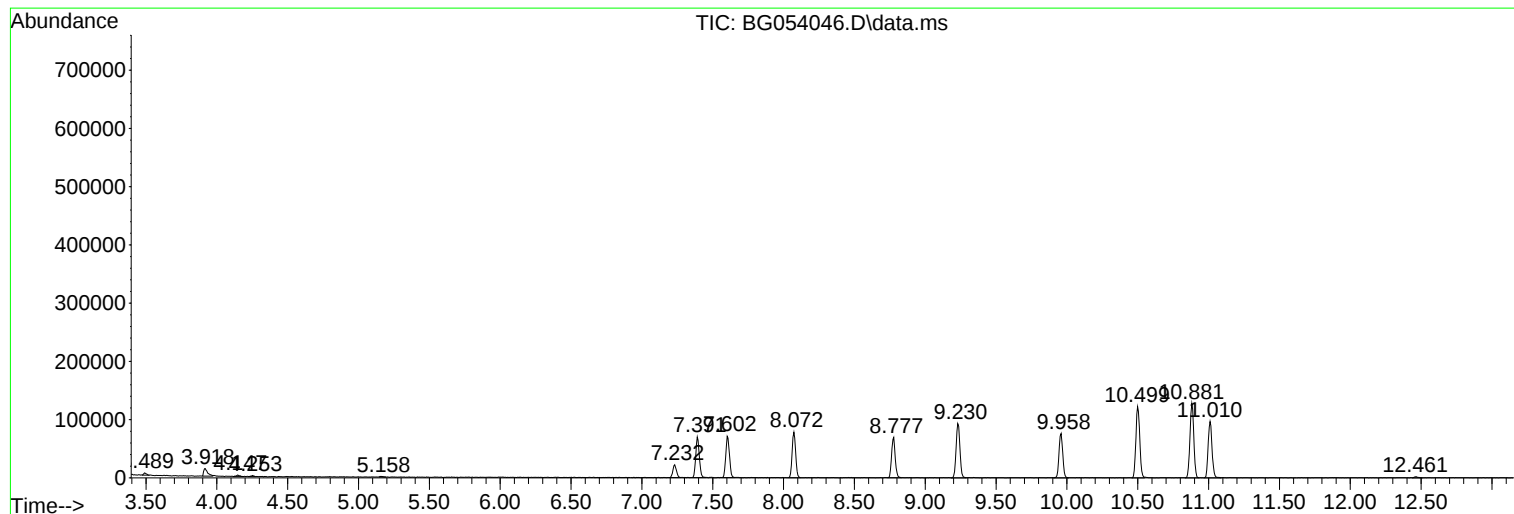

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054046.D
Acq On : 24 Jun 2022 13:52
Operator : CG/JU
Sample : N3395-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0166

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054046.D
Acq On : 24 Jun 2022 13:52
Operator : CG/JU
Sample : N3395-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0166

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc