

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054047.D
 Acq On : 24 Jun 2022 14:31
 Operator : CG/JU
 Sample : N3395-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.496	14	18	23	rVB3	3646	6418	0.59%	0.073%
2	3.590	32	34	39	rVB4	835	1130	0.10%	0.013%
3	3.919	87	90	99	rBV2	10703	20854	1.92%	0.239%
4	4.054	111	113	116	rBV3	1034	1463	0.13%	0.017%
5	4.154	124	130	134	rVB4	2229	4771	0.44%	0.055%
6	4.254	143	147	153	rBV5	1584	3430	0.32%	0.039%
7	5.159	298	301	303	rBV	1182	1600	0.15%	0.018%
8	5.540	364	366	371	rVB	856	1389	0.13%	0.016%
9	7.233	647	654	661	rBV	21600	38369	3.54%	0.439%
10	7.391	675	681	689	rBV	70964	124572	11.49%	1.426%
11	7.603	710	717	725	rBV	71061	129075	11.91%	1.478%
12	8.073	790	797	805	rVB	75955	132577	12.23%	1.518%
13	8.772	910	916	924	rBV	67005	117820	10.87%	1.349%
14	9.230	986	994	1006	rBV	96150	177449	16.37%	2.031%
15	9.953	1110	1117	1126	rBV	74278	139762	12.89%	1.600%
16	10.499	1203	1210	1218	rBV	125828	227333	20.97%	2.602%
17	10.881	1266	1275	1283	rBB	121032	222126	20.49%	2.543%
18	11.011	1290	1297	1305	rBV	97187	187797	17.32%	2.150%
19	12.462	1535	1544	1549	rBV2	2128	4015	0.37%	0.046%
20	14.095	1815	1822	1829	rBV	282075	431719	39.83%	4.942%
21	14.389	1865	1872	1880	rBV	306276	502901	46.39%	5.757%
22	14.694	1917	1924	1932	rVB	230105	375880	34.67%	4.303%
23	14.882	1951	1956	1968	rBV2	17193	32747	3.02%	0.375%
24	15.106	1987	1994	1997	rBV2	664	1319	0.12%	0.015%
25	15.429	2046	2049	2053	rBV3	1535	1942	0.18%	0.022%
26	15.494	2056	2060	2062	rVB2	1259	1564	0.14%	0.018%
27	15.687	2086	2093	2102	rBV	449274	697126	64.31%	7.981%
28	15.793	2106	2111	2120	rBV	118379	184469	17.02%	2.112%
29	15.928	2130	2134	2139	rVB	3712	5433	0.50%	0.062%
30	16.469	2220	2226	2229	rBV2	1490	1989	0.18%	0.023%
31	17.438	2384	2391	2400	rBV	328951	511745	47.21%	5.858%
32	17.538	2401	2408	2415	rBV2	541001	835286	77.06%	9.562%
33	18.102	2500	2504	2508	rBV3	5163	6394	0.59%	0.073%
34	18.337	2540	2544	2548	rVB2	1482	2011	0.19%	0.023%
35	19.271	2700	2703	2706	rVB2	1639	1733	0.16%	0.020%
36	19.389	2717	2723	2727	rBV3	7432	11206	1.03%	0.128%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054047.D
 Acq On : 24 Jun 2022 14:31
 Operator : CG/JU
 Sample : N3395-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.459	2730	2735	2739	rBV	6381	10539	0.97%	0.121%
38	19.741	2780	2783	2785	rBV	1763	1734	0.16%	0.020%
39	19.824	2790	2797	2806	rBV	722699	1084012	100.00%	12.410%
40	20.382	2890	2892	2895	rBV3	1003	1356	0.13%	0.016%
41	20.447	2898	2903	2904	rBV2	1071	1479	0.14%	0.017%
42	20.599	2926	2929	2931	rVV2	945	1088	0.10%	0.012%
43	20.658	2936	2939	2941	rBV3	1132	1287	0.12%	0.015%
44	20.687	2941	2944	2946	rBV4	1497	1660	0.15%	0.019%
45	20.781	2958	2960	2964	rVB5	1179	1210	0.11%	0.014%
46	21.105	3013	3015	3017	rBV3	1114	1090	0.10%	0.012%
47	21.357	3054	3058	3061	rBV4	6865	10141	0.94%	0.116%
48	21.716	3112	3119	3127	rBV2	358247	624988	57.66%	7.155%
49	21.986	3163	3165	3169	rBV4	1749	2416	0.22%	0.028%
50	22.021	3169	3171	3172	rBV2	1544	1433	0.13%	0.016%
51	22.156	3192	3194	3197	rBV4	1557	1736	0.16%	0.020%
52	22.186	3197	3199	3200	rVV2	1935	1492	0.14%	0.017%
53	22.233	3203	3207	3210	rBV4	1916	3254	0.30%	0.037%
54	22.526	3253	3257	3259	rBV4	3108	3526	0.33%	0.040%
55	23.096	3352	3354	3355	rBV2	1788	1142	0.11%	0.013%
56	23.226	3373	3376	3380	rVB5	3278	5498	0.51%	0.063%
57	23.314	3389	3391	3393	rBV2	1577	1513	0.14%	0.017%
58	23.884	3486	3488	3490	rBV3	1465	1632	0.15%	0.019%
59	24.048	3509	3516	3523	rBV8	7679	20824	1.92%	0.238%
60	24.747	3623	3635	3651	rBV2	374993	1082797	99.89%	12.396%
61	24.971	3661	3673	3691	rVB2	203649	636490	58.72%	7.287%
62	25.505	3762	3764	3765	rBV2	1456	1154	0.11%	0.013%
63	25.999	3845	3848	3851	rBV5	1383	2292	0.21%	0.026%
64	26.169	3870	3877	3886	rVB4	9999	27146	2.50%	0.311%
65	26.281	3895	3896	3900	rBV3	1810	1945	0.18%	0.022%
66	27.550	4107	4112	4123	rVB8	7895	24133	2.23%	0.276%
67	28.378	4251	4253	4258	rBV2	1692	1886	0.17%	0.022%
68	29.219	4386	4396	4397	rBV6	5166	12179	1.12%	0.139%
69	29.407	4426	4428	4431	rBV4	1459	1597	0.15%	0.018%
70	29.430	4431	4432	4436	rVB3	2368	2313	0.21%	0.026%
71	29.471	4436	4439	4440	rBV3	1845	2094	0.19%	0.024%
72	30.094	4543	4545	4548	rBV4	1482	1496	0.14%	0.017%
73	31.199	4730	4733	4734	rBV2	2293	2311	0.21%	0.026%
74	31.616	4802	4804	4807	rBV4	1417	1435	0.13%	0.016%
75	31.686	4814	4816	4817	rBV	1596	1459	0.13%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054047.D
Acq On : 24 Jun 2022 14:31
Operator : CG/JU
Sample : N3395-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0169

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 8735191

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054047.D
Acq On : 24 Jun 2022 14:31
Operator : CG/JU
Sample : N3395-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

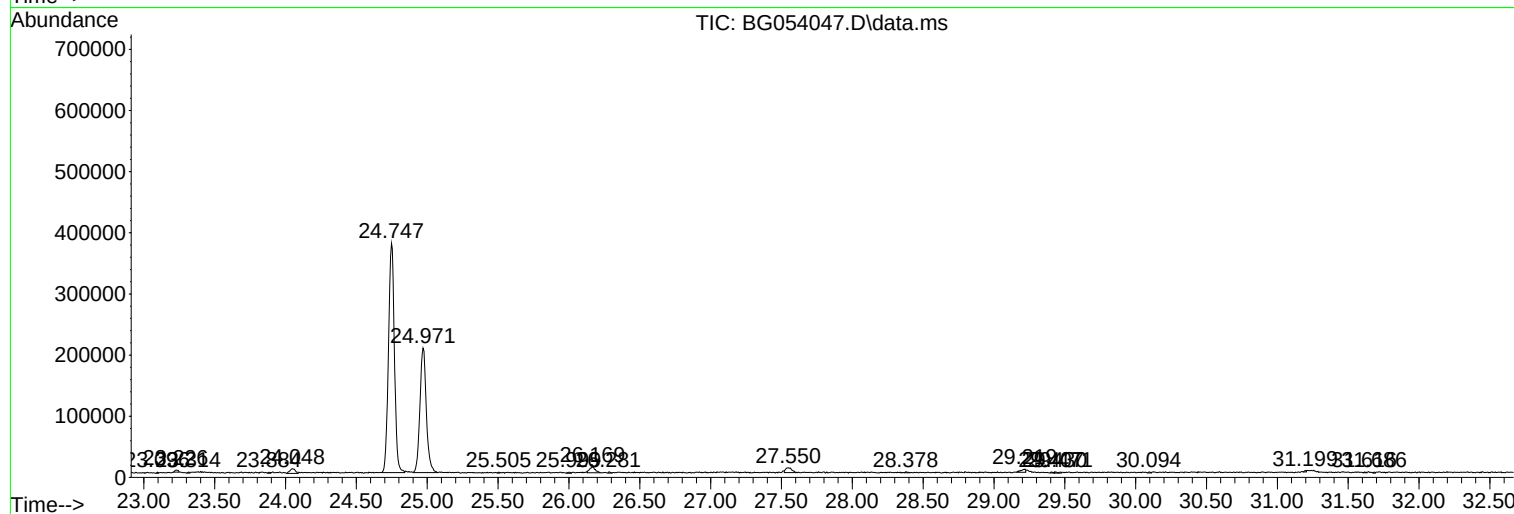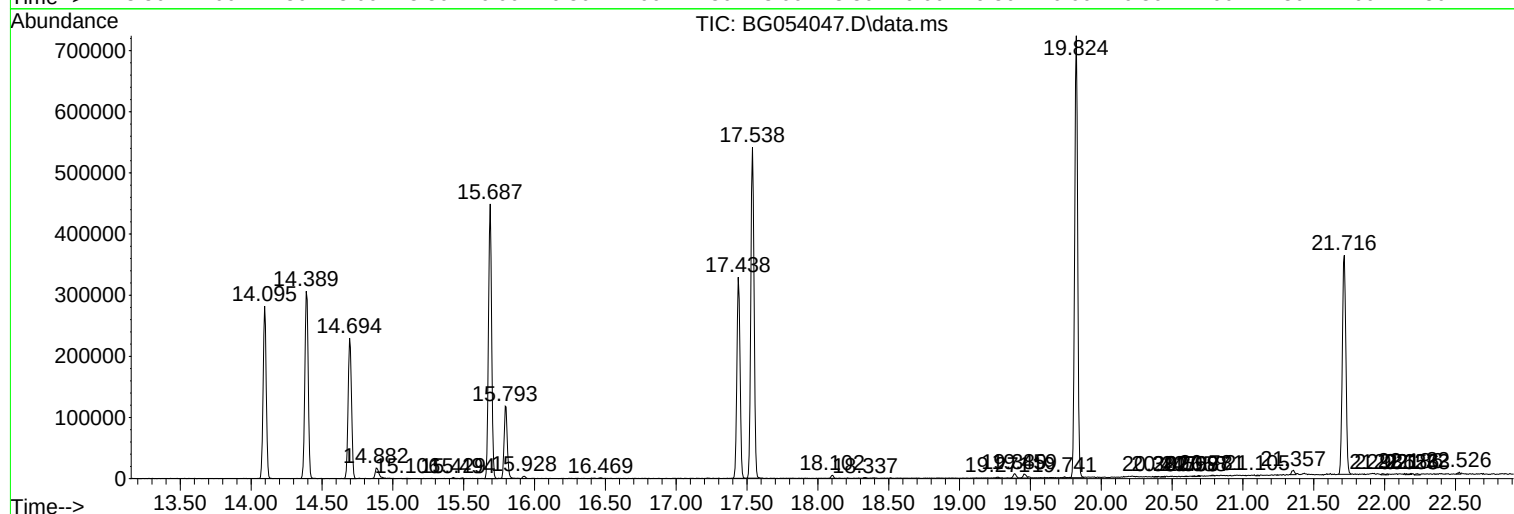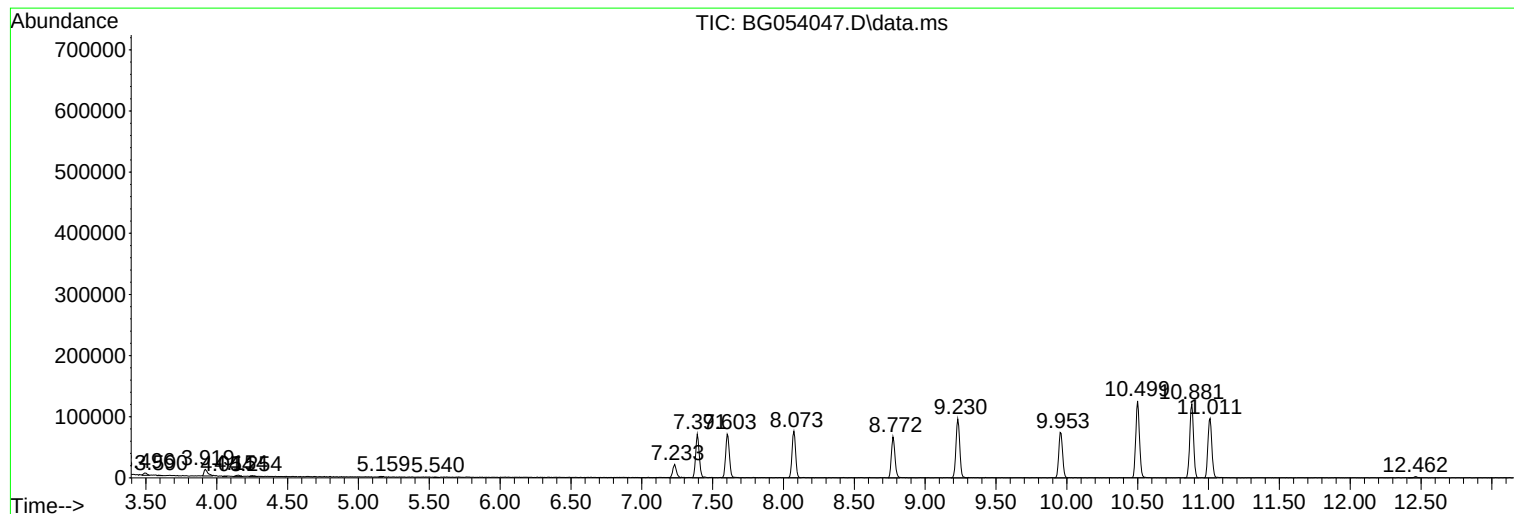

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054047.D
Acq On : 24 Jun 2022 14:31
Operator : CG/JU
Sample : N3395-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054047.D
Acq On : 24 Jun 2022 14:31
Operator : CG/JU
Sample : N3395-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------