

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054048.D
 Acq On : 24 Jun 2022 15:10
 Operator : CG/JU
 Sample : N3395-18
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.495	14	18	23	rVB3	4533	7336	0.57%	0.077%
2	3.918	86	90	99	rBV	16750	32503	2.54%	0.342%
3	4.147	126	129	135	rVB2	2926	4495	0.35%	0.047%
4	4.611	206	208	214	rVB2	817	1330	0.10%	0.014%
5	5.163	298	302	308	rVB4	1262	2454	0.19%	0.026%
6	7.226	649	653	662	rVB	21583	38314	3.00%	0.404%
7	7.390	674	681	689	rBV	75734	133843	10.47%	1.410%
8	7.608	711	718	729	rVB	75372	140135	10.96%	1.476%
9	8.072	791	797	805	rBV	67308	117879	9.22%	1.241%
10	8.771	910	916	929	rVB	70760	128487	10.05%	1.353%
11	9.229	987	994	1005	rVB	104661	193759	15.15%	2.041%
12	9.958	1111	1118	1126	rBV	85383	154344	12.07%	1.626%
13	10.498	1203	1210	1219	rBV	137366	251973	19.71%	2.654%
14	10.880	1268	1275	1284	rBV	108441	202864	15.87%	2.137%
15	11.009	1290	1297	1305	rBV	118732	227221	17.77%	2.393%
16	12.461	1540	1544	1550	rVB2	1910	3326	0.26%	0.035%
17	14.094	1816	1822	1830	rVB	331882	497683	38.93%	5.241%
18	14.388	1864	1872	1880	rBV	332761	552612	43.22%	5.820%
19	14.693	1918	1924	1932	rVB	215343	352088	27.54%	3.708%
20	14.887	1951	1957	1967	rBV	21977	39090	3.06%	0.412%
21	15.428	2044	2049	2053	rBV	9127	13079	1.02%	0.138%
22	15.487	2055	2059	2066	rVB3	1312	2144	0.17%	0.023%
23	15.686	2084	2093	2101	rBV	498765	786884	61.55%	8.287%
24	15.798	2106	2112	2122	rBV	152540	227673	17.81%	2.398%
25	15.927	2130	2134	2138	rBV2	3852	6422	0.50%	0.068%
26	16.474	2218	2227	2231	rVB3	1618	2822	0.22%	0.030%
27	17.437	2385	2391	2399	rBV	300207	483601	37.83%	5.093%
28	17.537	2401	2408	2419	rVB	621869	968762	75.77%	10.203%
29	18.101	2500	2504	2508	rVB2	4270	5147	0.40%	0.054%
30	18.336	2540	2544	2546	rBV2	2329	2836	0.22%	0.030%
31	18.389	2550	2553	2558	rBV2	1155	1947	0.15%	0.021%
32	19.112	2671	2676	2677	rBV2	1113	1547	0.12%	0.016%
33	19.388	2718	2723	2729	rVB2	8741	13015	1.02%	0.137%
34	19.458	2729	2735	2740	rBV	8358	12974	1.01%	0.137%
35	19.740	2778	2783	2787	rBV4	2084	3389	0.27%	0.036%
36	19.823	2790	2797	2808	rVV	846582	1266163	99.03%	13.335%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054048.D
 Acq On : 24 Jun 2022 15:10
 Operator : CG/JU
 Sample : N3395-18
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.346	2885	2886	2890	rVB3	1407	1366	0.11%	0.014%
38	20.786	2956	2961	2964	rBV5	2055	3370	0.26%	0.035%
39	20.827	2966	2968	2970	rBV3	1444	1494	0.12%	0.016%
40	20.851	2970	2972	2975	rVB3	1608	1501	0.12%	0.016%
41	20.980	2991	2994	2997	rBV3	1282	1421	0.11%	0.015%
42	21.356	3054	3058	3067	rVB5	8751	15262	1.19%	0.161%
43	21.427	3067	3070	3075	rBV5	2837	4959	0.39%	0.052%
44	21.715	3109	3119	3128	rBV2	345393	596265	46.64%	6.280%
45	22.044	3173	3175	3177	rBV3	1697	1505	0.12%	0.016%
46	22.331	3222	3224	3228	rVB5	1485	1891	0.15%	0.020%
47	22.484	3247	3250	3251	rBV3	1504	1537	0.12%	0.016%
48	22.531	3255	3258	3262	rVB5	2603	3961	0.31%	0.042%
49	22.913	3321	3323	3325	rBV2	1782	1784	0.14%	0.019%
50	23.160	3364	3365	3370	rVB5	1532	1348	0.11%	0.014%
51	23.230	3373	3377	3382	rVB6	5185	8261	0.65%	0.087%
52	23.595	3437	3439	3441	rBV3	1321	1295	0.10%	0.014%
53	24.006	3505	3509	3510	rBV3	2008	2164	0.17%	0.023%
54	24.041	3510	3515	3526	rBV6	6547	16600	1.30%	0.175%
55	24.746	3623	3635	3653	rBV2	424452	1278517	100.00%	13.465%
56	24.970	3662	3673	3688	rVB2	192386	590586	46.19%	6.220%
57	26.162	3871	3876	3884	rVB6	8885	23054	1.80%	0.243%
58	27.332	4072	4075	4076	rBV2	1480	1629	0.13%	0.017%
59	27.543	4107	4111	4125	rVB2	7000	22432	1.75%	0.236%
60	27.807	4154	4156	4160	rBV4	1199	1891	0.15%	0.020%
61	27.925	4174	4176	4180	rBV4	1479	1978	0.15%	0.021%
62	28.718	4309	4311	4314	rBV4	1472	1990	0.16%	0.021%
63	29.223	4388	4397	4404	rBV10	4663	16111	1.26%	0.170%
64	29.552	4452	4453	4458	rBV4	1603	1761	0.14%	0.019%
65	30.346	4586	4588	4593	rVB4	1480	1784	0.14%	0.019%
66	30.393	4593	4596	4599	rBV4	1565	1919	0.15%	0.020%
67	31.027	4702	4704	4707	rBV3	1308	1386	0.11%	0.015%
68	31.198	4731	4733	4736	rBV4	1839	2380	0.19%	0.025%
69	31.450	4774	4776	4778	rBV3	1704	1524	0.12%	0.016%




Sum of corrected areas: 9495067

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054048.D
Acq On : 24 Jun 2022 15:10
Operator : CG/JU
Sample : N3395-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

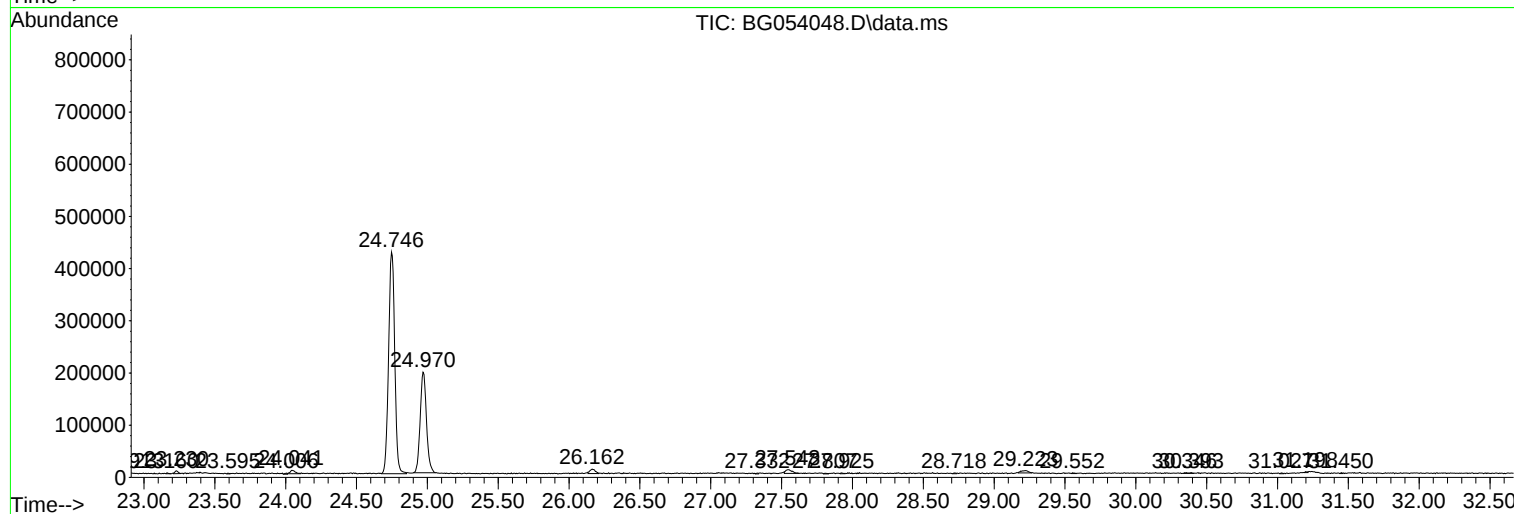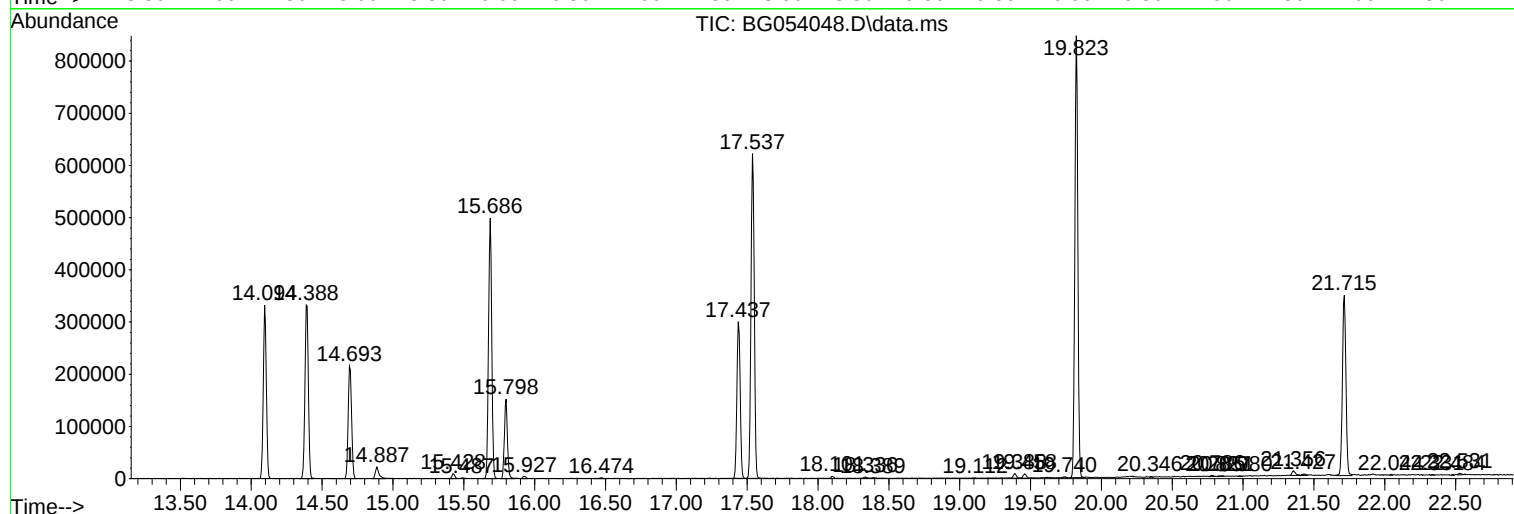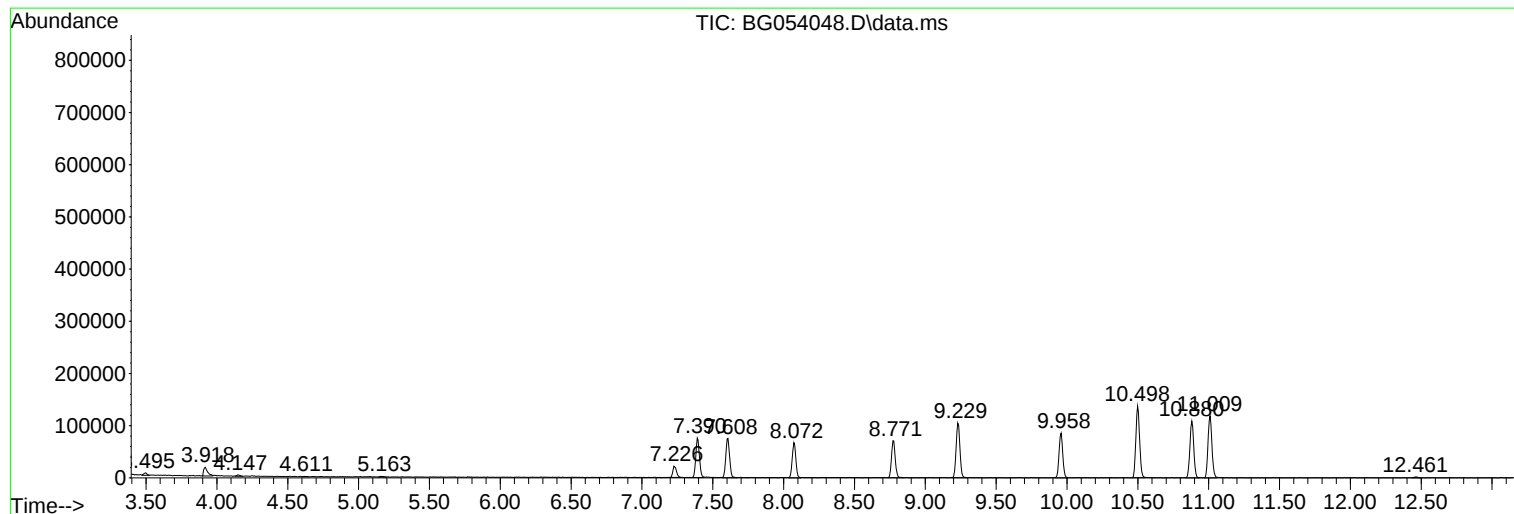

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054048.D
Acq On : 24 Jun 2022 15:10
Operator : CG/JU
Sample : N3395-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054048.D
Acq On : 24 Jun 2022 15:10
Operator : CG/JU
Sample : N3395-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc