

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054049.D
 Acq On : 24 Jun 2022 15:49
 Operator : CG/JU
 Sample : N3395-22
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.499	15	19	24	rVB3	4056	6660	0.67%	0.085%
2	3.916	86	90	101	rBV2	14993	27785	2.80%	0.354%
3	4.004	103	105	109	rVB4	1304	1611	0.16%	0.021%
4	4.151	125	130	135	rVB2	2070	3643	0.37%	0.046%
5	4.562	197	200	205	rBV3	649	1273	0.13%	0.016%
6	4.645	213	214	219	rVB3	826	1159	0.12%	0.015%
7	5.156	299	301	304	rBV	1359	1141	0.11%	0.015%
8	5.532	360	365	368	rVB3	698	1232	0.12%	0.016%
9	6.108	460	463	466	rBV3	758	1115	0.11%	0.014%
10	7.230	649	654	661	rBV3	19208	33649	3.39%	0.428%
11	7.394	675	682	689	rBV	61523	110944	11.17%	1.412%
12	7.482	695	697	702	rVB3	868	1053	0.11%	0.013%
13	7.606	712	718	726	rBV2	64808	112827	11.36%	1.436%
14	8.076	791	798	805	rBV	62163	113392	11.42%	1.443%
15	8.775	910	917	931	rBB	60693	109723	11.05%	1.397%
16	9.233	985	995	1006	rBV	84702	161502	16.26%	2.056%
17	9.956	1111	1118	1127	rBV	68049	123442	12.43%	1.571%
18	10.497	1203	1210	1220	rBV	107815	203057	20.45%	2.585%
19	10.879	1268	1275	1286	rVB	98211	191580	19.29%	2.439%
20	11.008	1288	1297	1307	rBV	91689	173244	17.45%	2.205%
21	12.465	1541	1545	1549	rBB2	1817	3114	0.31%	0.040%
22	14.092	1816	1822	1831	rBV	266588	409170	41.20%	5.208%
23	14.392	1866	1873	1881	rVB	273621	459133	46.24%	5.844%
24	14.698	1918	1925	1933	rVB	202949	321219	32.35%	4.089%
25	14.886	1952	1957	1966	rBV2	13653	26565	2.68%	0.338%
26	14.944	1966	1967	1973	rVB2	810	1015	0.10%	0.013%
27	15.485	2057	2059	2064	rBV3	688	1081	0.11%	0.014%
28	15.685	2085	2093	2103	rVB	418146	656993	66.16%	8.363%
29	15.796	2106	2112	2121	rBV	97119	144156	14.52%	1.835%
30	15.926	2130	2134	2139	rVB2	3435	5044	0.51%	0.064%
31	16.466	2223	2226	2231	rBV3	1407	1903	0.19%	0.024%
32	16.936	2301	2306	2309	rVB3	995	1358	0.14%	0.017%
33	17.441	2385	2392	2398	rBV	285481	437585	44.07%	5.570%
34	17.535	2401	2408	2419	rBV	467698	759732	76.51%	9.671%
35	18.082	2498	2501	2504	rBV3	511	1006	0.10%	0.013%
36	18.329	2540	2543	2546	rBV3	2781	3706	0.37%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054049.D
 Acq On : 24 Jun 2022 15:49
 Operator : CG/JU
 Sample : N3395-22
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	18.399	2551	2555	2558	rVB3	1226	1451	0.15%	0.018%
38	19.386	2718	2723	2729	rVB3	6780	9917	1.00%	0.126%
39	19.457	2731	2735	2742	rVB2	6401	9728	0.98%	0.124%
40	19.598	2756	2759	2760	rBV2	1886	1424	0.14%	0.018%

41	19.739	2779	2783	2788	rBV3	1680	1955	0.20%	0.025%
42	19.821	2790	2797	2807	rBV	652307	993033	100.00%	12.641%
43	20.203	2860	2862	2867	rVB4	1653	2068	0.21%	0.026%
44	20.320	2880	2882	2885	rVV2	1053	1243	0.13%	0.016%
45	20.350	2885	2887	2888	rVV2	1431	1079	0.11%	0.014%

46	20.391	2892	2894	2897	rVB4	1029	1119	0.11%	0.014%
47	20.426	2897	2900	2902	rBV3	1229	1324	0.13%	0.017%
48	20.473	2906	2908	2913	rVB5	951	1227	0.12%	0.016%
49	20.785	2958	2961	2963	rVB3	1914	2383	0.24%	0.030%
50	20.949	2988	2989	2990	rBV	1744	1040	0.10%	0.013%

51	21.290	3044	3047	3049	rBV3	1350	1535	0.15%	0.020%
52	21.354	3053	3058	3068	rVV4	14792	29214	2.94%	0.372%
53	21.437	3068	3072	3075	rVB5	2892	4647	0.47%	0.059%
54	21.525	3085	3087	3089	rBV3	1439	1673	0.17%	0.021%
55	21.560	3091	3093	3094	rVV2	1719	1001	0.10%	0.013%

56	21.595	3097	3099	3101	rVB3	1680	1360	0.14%	0.017%
57	21.713	3112	3119	3127	rBV2	307445	530398	53.41%	6.752%
58	21.848	3140	3142	3145	rBV3	1254	1000	0.10%	0.013%
59	22.042	3173	3175	3179	rBV2	1238	1426	0.14%	0.018%
60	22.154	3192	3194	3198	rBV6	1044	1076	0.11%	0.014%

61	22.524	3253	3257	3259	rBV3	3363	4712	0.47%	0.060%
62	22.641	3274	3277	3278	rVB3	1838	1666	0.17%	0.021%
63	22.653	3278	3279	3282	rBV3	2375	1982	0.20%	0.025%
64	22.723	3289	3291	3292	rBV2	1312	1174	0.12%	0.015%
65	22.859	3312	3314	3318	rVB4	1812	1642	0.17%	0.021%

66	22.947	3327	3329	3331	rBV2	1330	1600	0.16%	0.020%
67	23.235	3374	3378	3383	rVB5	4987	8248	0.83%	0.105%
68	23.323	3390	3393	3395	rBV4	1526	2160	0.22%	0.027%
69	24.045	3510	3516	3523	rBV5	6613	15884	1.60%	0.202%
70	24.128	3528	3530	3532	rBV2	1217	1367	0.14%	0.017%

71	24.745	3623	3635	3650	rBV2	329359	984486	99.14%	12.532%
72	24.891	3658	3660	3661	rBV2	1794	1219	0.12%	0.016%
73	24.968	3663	3673	3690	rVV	177843	539614	54.34%	6.869%
74	25.244	3716	3720	3722	rBV4	2021	2592	0.26%	0.033%
75	25.297	3727	3729	3731	rVB3	1501	1053	0.11%	0.013%

76	25.391	3743	3745	3747	rBV3	1624	1655	0.17%	0.021%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054049.D
 Acq On : 24 Jun 2022 15:49
 Operator : CG/JU
 Sample : N3395-22
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	25.520	3765	3767	3769	rBV2	1505	1405	0.14%	0.018%
78	25.673	3789	3793	3794	rBV3	1208	1431	0.14%	0.018%
79	26.166	3870	3877	3884	rBV7	8752	21914	2.21%	0.279%
80	26.372	3910	3912	3914	rBV3	1607	1059	0.11%	0.013%
81	26.537	3938	3940	3943	rBV4	1204	1073	0.11%	0.014%
82	26.795	3982	3984	3987	rBV3	1351	1138	0.11%	0.014%
83	26.919	4003	4005	4009	rVB5	1630	1274	0.13%	0.016%
84	27.541	4107	4111	4123	rVB6	7742	21621	2.18%	0.275%
85	27.976	4182	4185	4187	rBV4	2020	2699	0.27%	0.034%
86	28.035	4193	4195	4197	rBV3	1470	1440	0.15%	0.018%
87	28.264	4232	4234	4237	rVB3	1309	999	0.10%	0.013%
88	28.611	4291	4293	4294	rBV2	1420	1210	0.12%	0.015%
89	29.122	4378	4380	4382	rBV3	1214	1123	0.11%	0.014%
90	29.333	4414	4416	4418	rBV3	1478	1643	0.17%	0.021%
91	30.144	4552	4554	4555	rBV	1747	1242	0.13%	0.016%
92	31.108	4717	4718	4719	rBV	1956	1089	0.11%	0.014%
93	31.537	4787	4791	4792	rBV4	2008	2025	0.20%	0.026%
94	31.778	4830	4832	4833	rBV	1420	1028	0.10%	0.013%
95	31.866	4845	4847	4850	rBV4	1202	1535	0.15%	0.020%
96	32.165	4897	4898	4901	rBV3	1649	1648	0.17%	0.021%
97	32.506	4954	4956	4957	rBV2	1347	1044	0.11%	0.013%




Sum of corrected areas: 7855827

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054049.D
Acq On : 24 Jun 2022 15:49
Operator : CG/JU
Sample : N3395-22
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

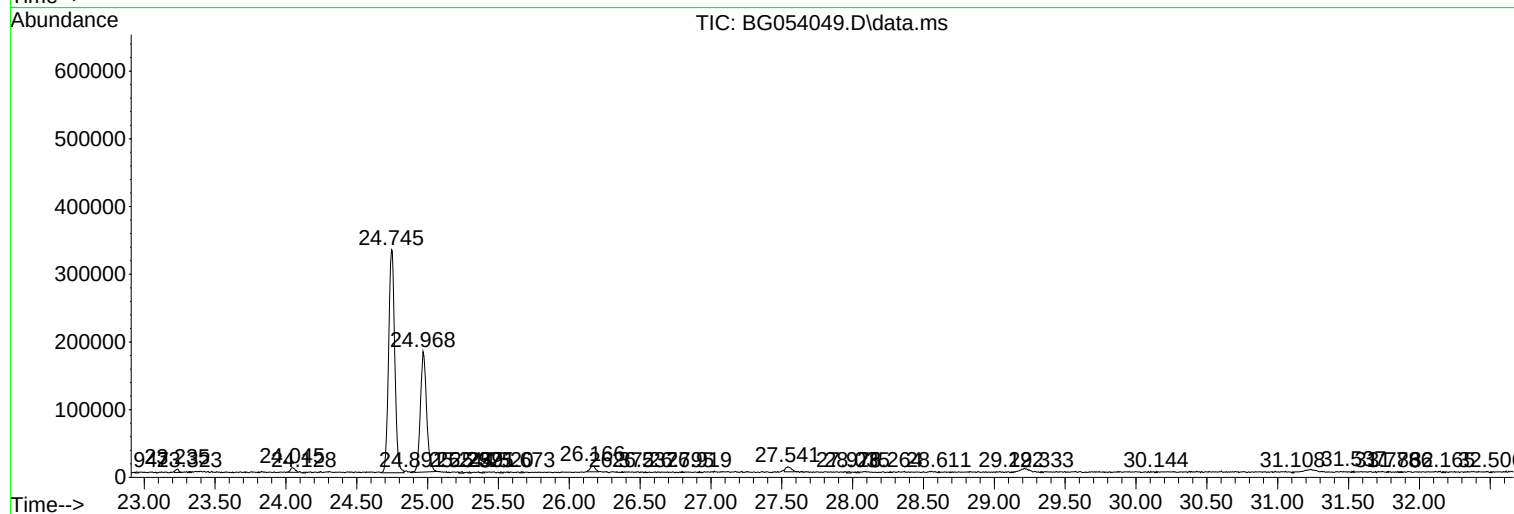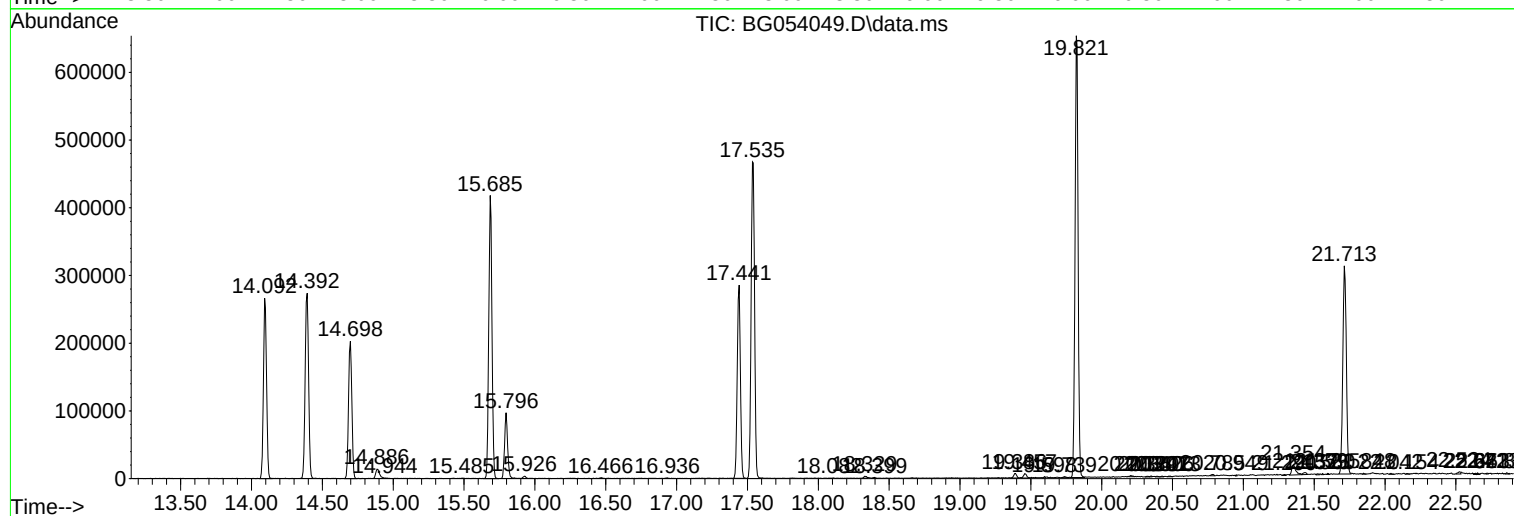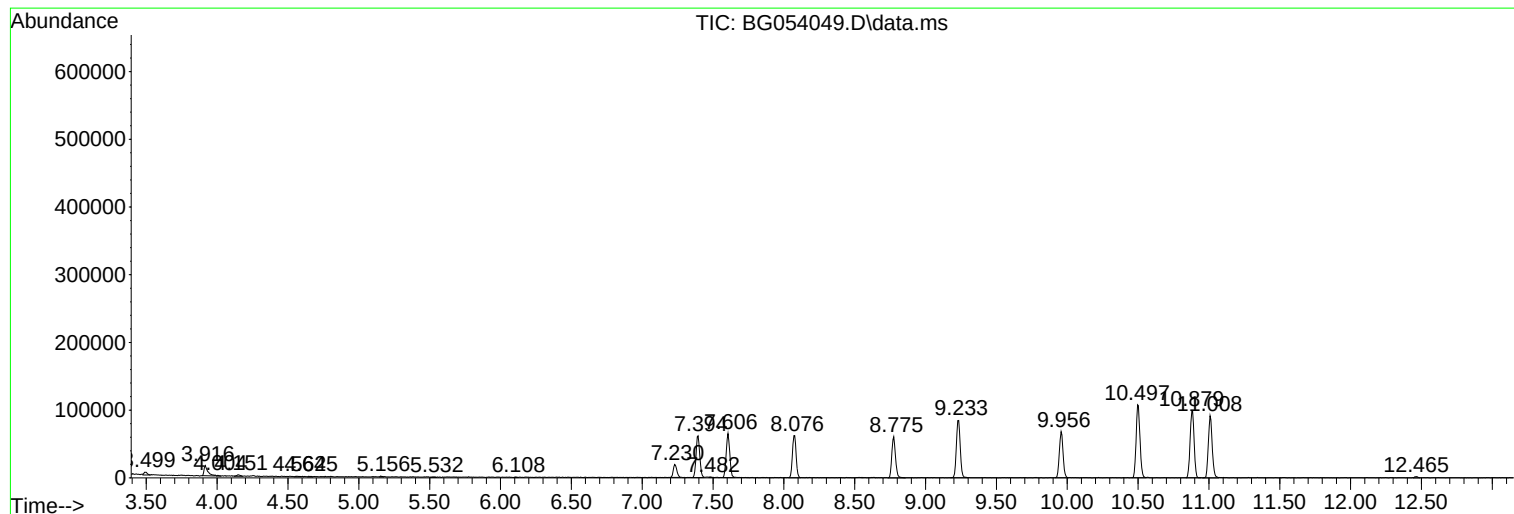

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054049.D
Acq On : 24 Jun 2022 15:49
Operator : CG/JU
Sample : N3395-22
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054049.D
Acq On : 24 Jun 2022 15:49
Operator : CG/JU
Sample : N3395-22
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------