

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054052.D
 Acq On : 24 Jun 2022 17:47
 Operator : CG/JU
 Sample : PB145691BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK691

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.496	14	18	23	rVV2	5449	7919	0.81%	0.088%
2	3.749	60	61	66	rVB3	918	1063	0.11%	0.012%
3	3.908	85	88	101	rBV	69668	127023	12.97%	1.411%
4	4.043	109	111	116	rVB3	884	1131	0.12%	0.013%
5	4.248	145	146	149	rVB	1095	1016	0.10%	0.011%
6	7.122	633	635	640	rVB	788	1007	0.10%	0.011%
7	7.227	647	653	662	rBV	92456	167171	17.06%	1.858%
8	7.392	675	681	690	rVV	70694	121713	12.42%	1.352%
9	7.603	708	717	728	rVB	91806	162245	16.56%	1.803%
10	8.073	788	797	807	rVB	78431	138148	14.10%	1.535%
11	8.773	910	916	927	rBV	127184	226501	23.12%	2.517%
12	8.861	927	931	934	rVB	755	1256	0.13%	0.014%
13	9.231	986	994	1005	rBV	94256	170152	17.37%	1.891%
14	9.954	1111	1117	1127	rBV	77769	143413	14.64%	1.594%
15	10.500	1203	1210	1226	rVB	130997	244417	24.95%	2.716%
16	10.882	1267	1275	1284	rVB	126140	232497	23.73%	2.583%
17	11.011	1290	1297	1313	rVB	129382	244002	24.91%	2.711%
18	12.462	1540	1544	1549	rBV2	1478	2628	0.27%	0.029%
19	14.096	1815	1822	1828	rBV	285361	424828	43.36%	4.721%
20	14.390	1865	1872	1879	rBV	295581	482530	49.25%	5.362%
21	14.695	1917	1924	1934	rBV	241858	392480	40.06%	4.361%
22	14.883	1950	1956	1970	rBV2	101250	176405	18.01%	1.960%
23	15.688	2086	2093	2102	rVB	424322	664525	67.83%	7.384%
24	15.794	2105	2111	2124	rBV	111603	176042	17.97%	1.956%
25	15.923	2128	2133	2137	rBV3	3591	4895	0.50%	0.054%
26	16.475	2223	2227	2230	rVV2	1032	1567	0.16%	0.017%
27	17.222	2351	2354	2359	rBV	854	1508	0.15%	0.017%
28	17.439	2384	2391	2399	rBV	336730	532278	54.33%	5.914%
29	17.539	2401	2408	2418	rVB	493439	760689	77.65%	8.452%
30	19.390	2716	2723	2730	rBV2	6275	9465	0.97%	0.105%
31	19.460	2730	2735	2739	rBV	5649	8925	0.91%	0.099%
32	19.625	2760	2763	2765	rBV2	913	1046	0.11%	0.012%
33	19.824	2790	2797	2805	rVV	663690	974060	99.42%	10.823%
34	19.924	2812	2814	2817	rBV3	951	1049	0.11%	0.012%
35	20.148	2850	2852	2854	rBV3	1321	1297	0.13%	0.014%
36	20.177	2854	2857	2859	rVV2	1178	1583	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054052.D
 Acq On : 24 Jun 2022 17:47
 Operator : CG/JU
 Sample : PB145691BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK691

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.482	2907	2909	2912	rVB2	1165	1283	0.13%	0.014%
38	20.518	2914	2915	2919	rBV3	1216	1273	0.13%	0.014%
39	20.923	2982	2984	2987	rVV2	1043	1142	0.12%	0.013%
40	21.123	3014	3018	3020	rBV4	1311	1794	0.18%	0.020%
41	21.205	3030	3032	3035	rVB3	1162	1005	0.10%	0.011%
42	21.434	3069	3071	3076	rVB4	1838	2490	0.25%	0.028%
43	21.710	3112	3118	3126	rBV	363917	640545	65.38%	7.117%
44	22.128	3187	3189	3191	rBV3	1474	1567	0.16%	0.017%
45	22.504	3250	3253	3254	rBV3	1338	1638	0.17%	0.018%
46	22.680	3281	3283	3286	rBV4	1119	1412	0.14%	0.016%
47	23.203	3370	3372	3373	rBV	1503	1353	0.14%	0.015%
48	23.232	3373	3377	3379	rVV4	3513	4789	0.49%	0.053%
49	23.461	3414	3416	3421	rBV3	1393	1823	0.19%	0.020%
50	23.708	3457	3458	3459	rBV	1839	1005	0.10%	0.011%
51	24.043	3512	3515	3521	rVB7	6521	11585	1.18%	0.129%
52	24.166	3534	3536	3537	rBV3	1697	1196	0.12%	0.013%
53	24.366	3568	3570	3572	rVB2	1552	1047	0.11%	0.012%
54	24.748	3622	3635	3650	rBV	336111	979697	100.00%	10.886%
55	24.971	3661	3673	3694	rVB2	208864	654414	66.80%	7.272%
56	25.547	3769	3771	3773	rBV3	1749	1307	0.13%	0.015%
57	25.853	3819	3823	3824	rBV4	1295	1519	0.16%	0.017%
58	26.164	3871	3876	3885	rVB4	9454	24817	2.53%	0.276%
59	27.345	4074	4077	4078	rBV3	1458	1273	0.13%	0.014%
60	27.545	4101	4111	4122	rBV6	10061	36053	3.68%	0.401%
61	27.674	4131	4133	4136	rVB3	1432	1133	0.12%	0.013%
62	28.573	4284	4286	4288	rVB3	1378	983	0.10%	0.011%
63	28.808	4324	4326	4327	rBV2	1384	1318	0.13%	0.015%
64	29.031	4362	4364	4368	rBV3	1248	1238	0.13%	0.014%
65	29.196	4390	4392	4393	rBV2	2422	1377	0.14%	0.015%
66	30.359	4589	4590	4592	rBV2	1733	1421	0.15%	0.016%
67	30.500	4612	4614	4615	rBV2	1443	1301	0.13%	0.014%
68	30.994	4697	4698	4700	rBV2	1551	1099	0.11%	0.012%
69	31.146	4721	4724	4725	rBV2	1958	1872	0.19%	0.021%
70	31.205	4732	4734	4736	rBV2	2193	1676	0.17%	0.019%
71	31.934	4855	4858	4859	rBV3	1698	1684	0.17%	0.019%




Sum of corrected areas: 8999603

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054052.D
Acq On : 24 Jun 2022 17:47
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

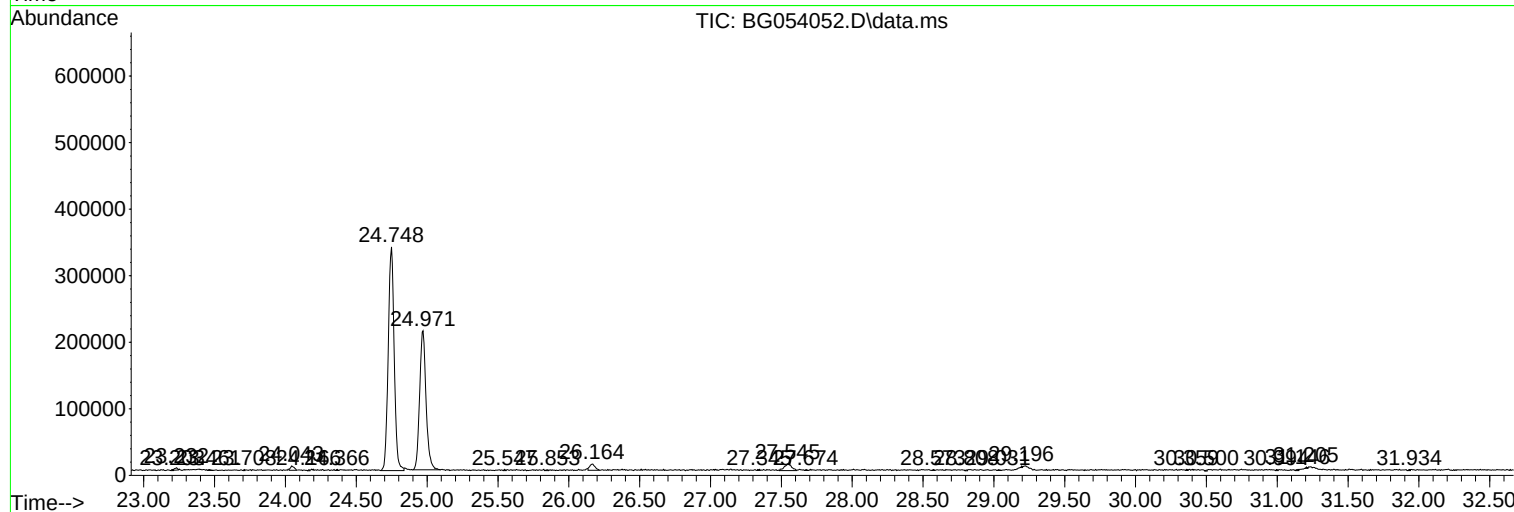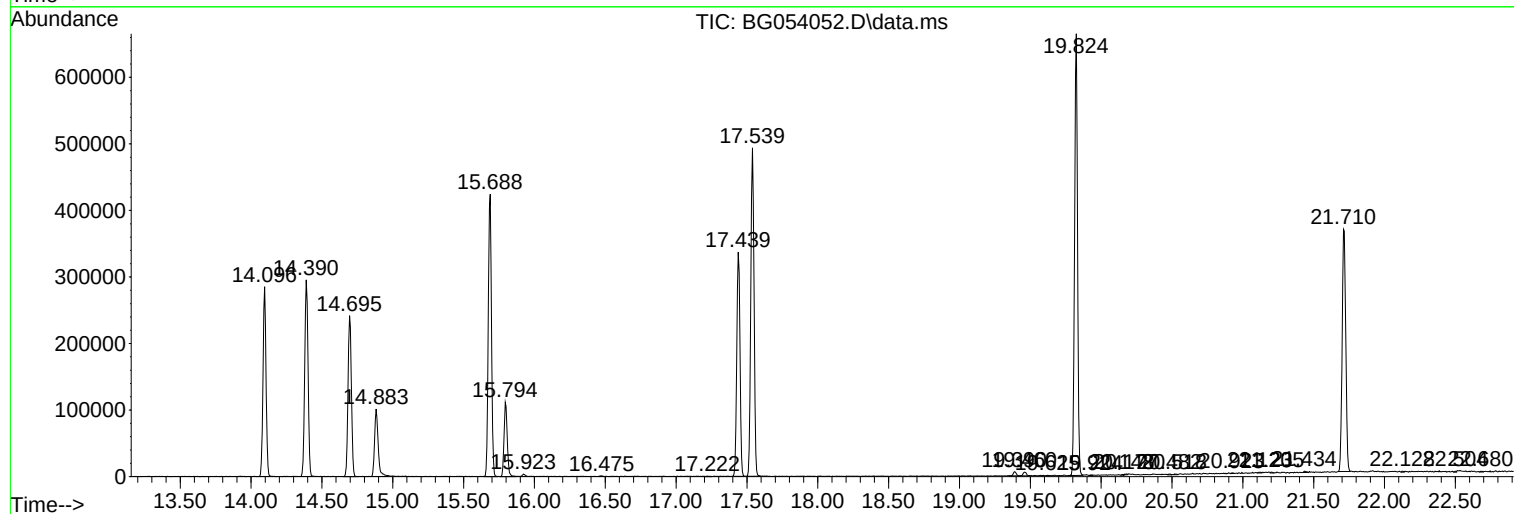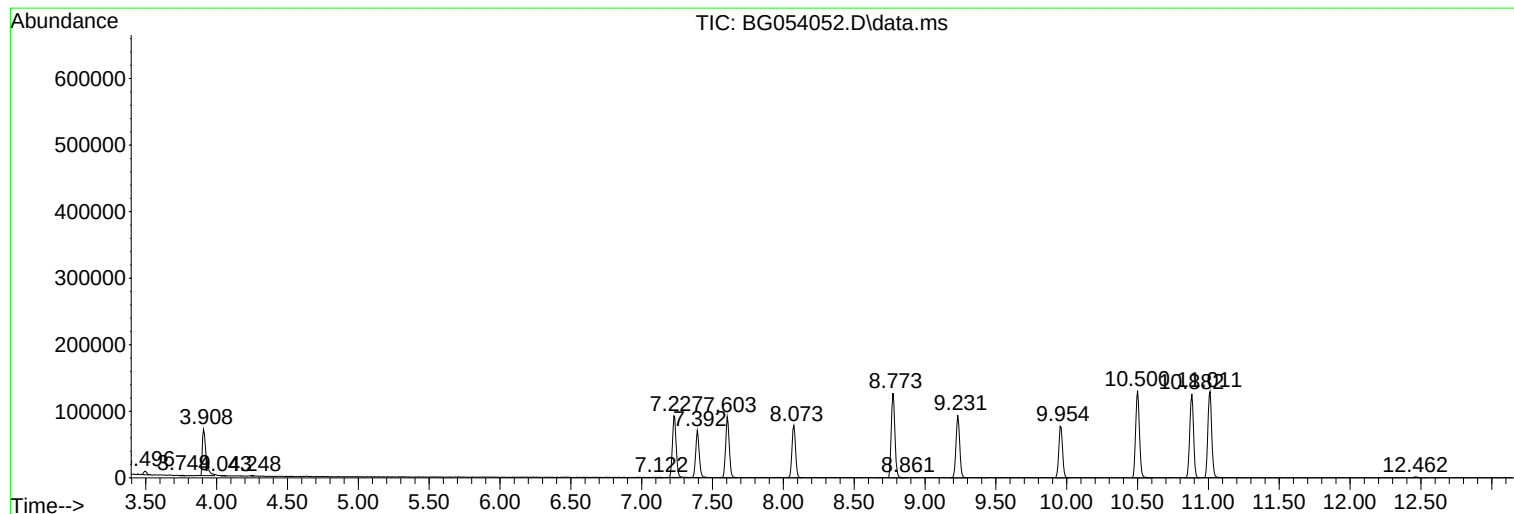

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054052.D
Acq On : 24 Jun 2022 17:47
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054052.D
Acq On : 24 Jun 2022 17:47
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------