
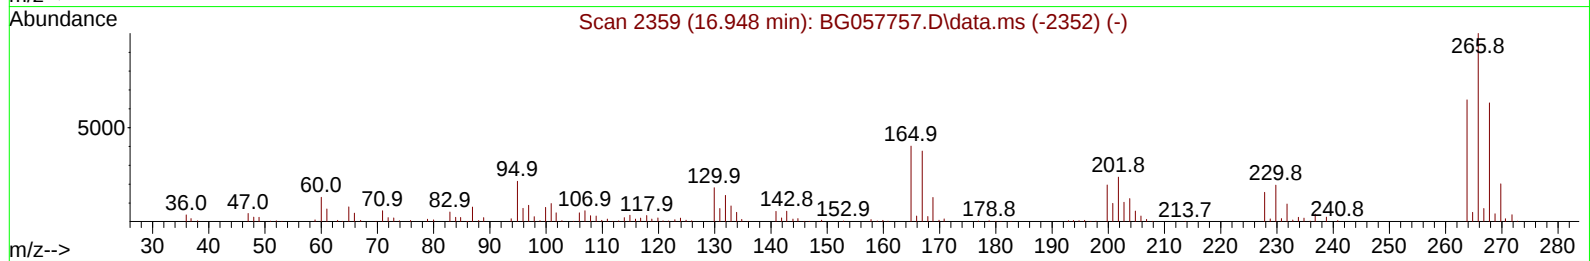
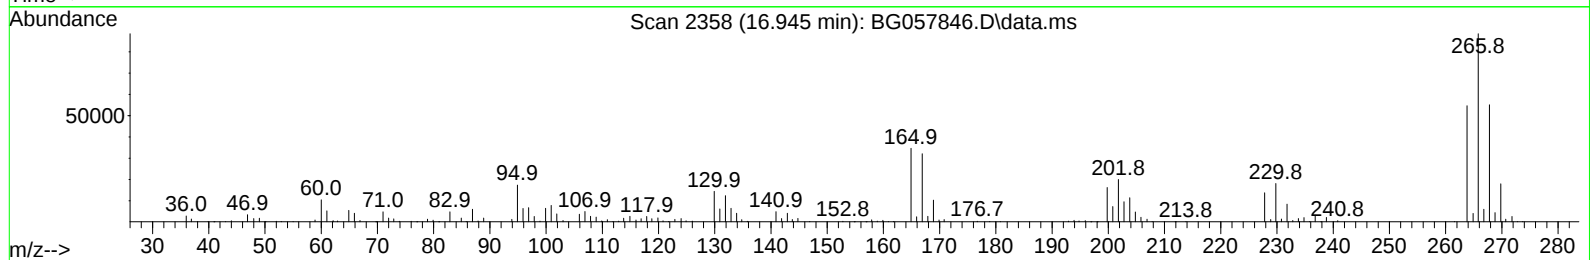


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
Data File : BG057846.D
Acq On : 23 Jun 2023 17:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 18:26:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

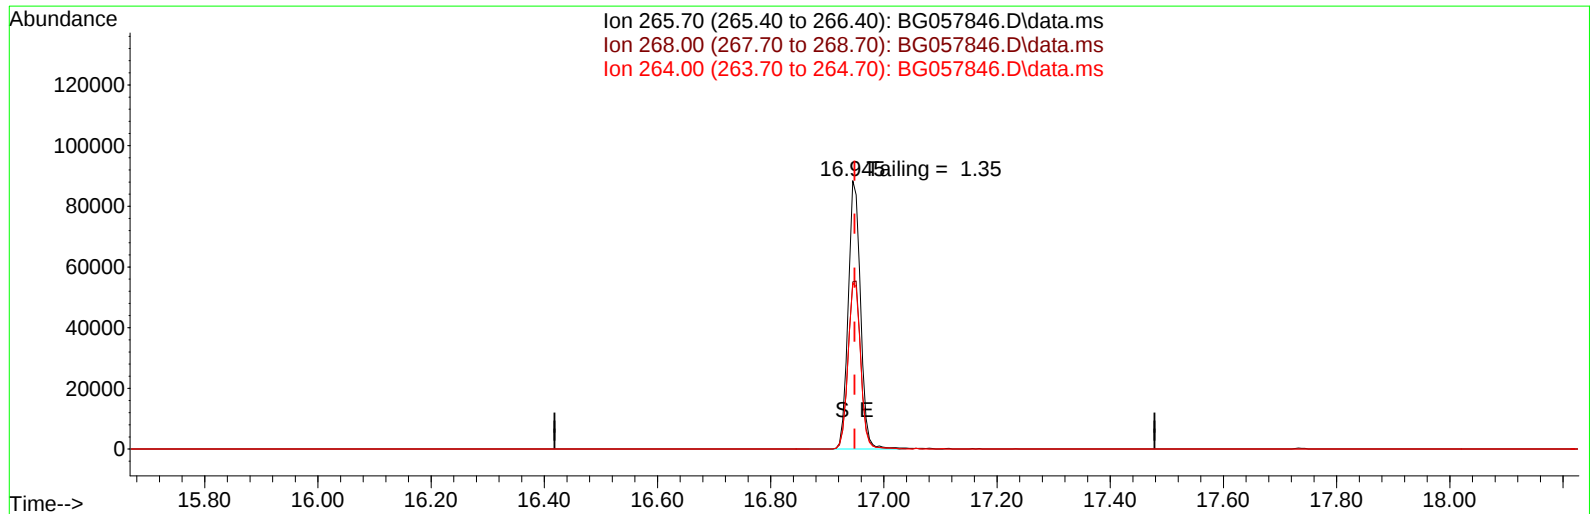

TIC: BG057846.D\data.ms

(70) Pentachlorophenol (C)




16.945min (-0.003) 36630.25 ng

response 133706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.29
264.00	64.70	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
Data File : BG057846.D
Acq On : 23 Jun 2023 17:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 18:26:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

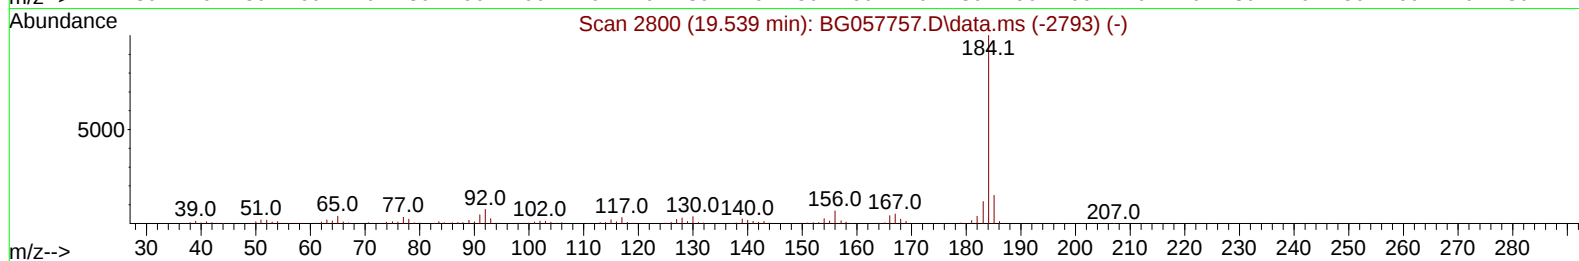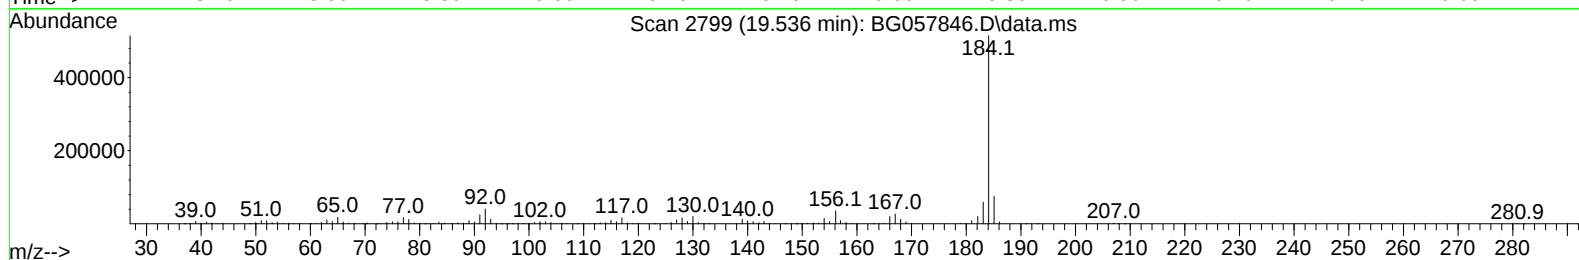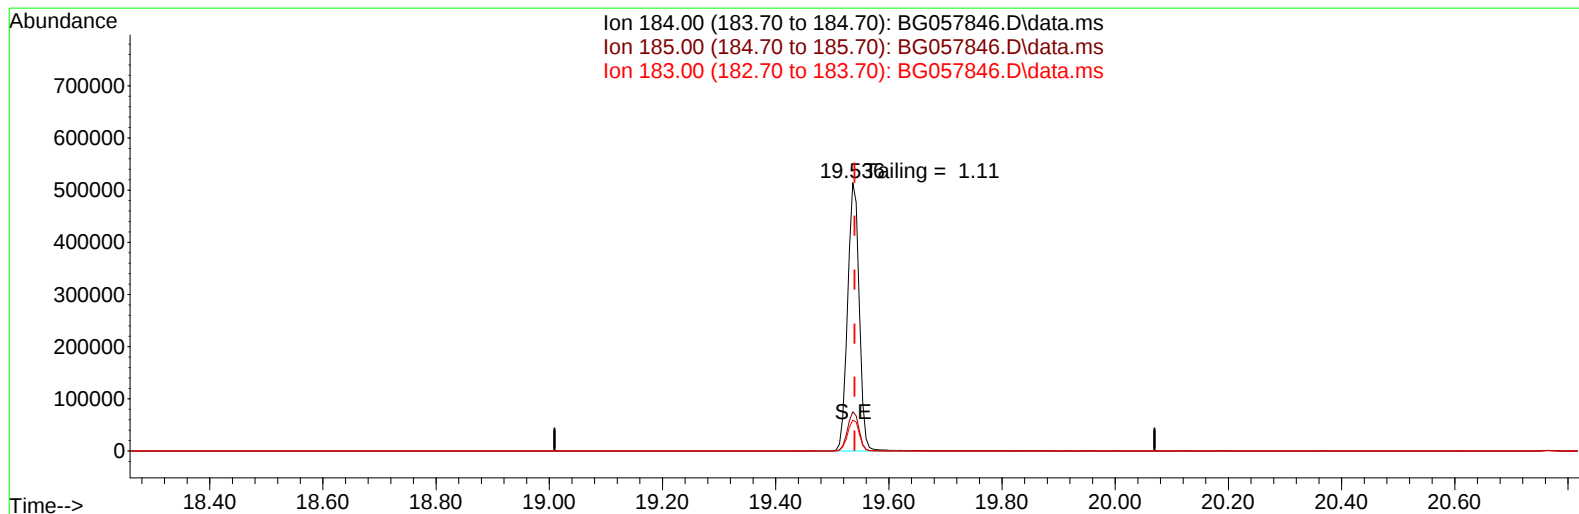

TIC: BG057846.D\data.ms

(77) Benzidine

19.536min (-0.003) 0.00 ng

response 729398

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.63
183.00	11.70	11.50
0.00	0.00	0.00