

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
 Data File : BG057837.D
 Acq On : 23 Jun 2023 11:19
 Operator : CG/JU
 Sample : 03238-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PMW-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.492	401	409	416	rBV	268802	411958	17.01%	4.126%
2	7.078	673	679	688	rBV	179364	294255	12.15%	2.947%
3	7.918	816	822	829	rBV	118753	192698	7.95%	1.930%
4	9.082	1012	1020	1031	rVB	344902	595638	24.59%	5.965%
5	10.727	1290	1300	1307	rBV	166486	299549	12.37%	3.000%
6	13.183	1711	1718	1727	rBV	944762	1428247	58.96%	14.304%
7	14.558	1946	1952	1961	rVB	315280	476954	19.69%	4.777%
8	15.909	2176	2182	2188	rBV	87292	128926	5.32%	1.291%
9	16.044	2197	2205	2214	rBV	933280	1399656	57.78%	14.018%
10	17.301	2408	2419	2426	rBV	437374	659556	27.23%	6.606%
11	18.183	2565	2569	2578	rBV	51533	86390	3.57%	0.865%
12	19.464	2783	2787	2794	rBV4	29655	46190	1.91%	0.463%
13	19.916	2857	2864	2869	rBV	1876711	2422363	100.00%	24.260%
14	21.203	3079	3083	3090	rBV5	30615	57318	2.37%	0.574%
15	21.285	3093	3097	3102	rVV	19751	30720	1.27%	0.308%
16	21.549	3136	3142	3150	rVB	441336	675495	27.89%	6.765%
17	24.699	3669	3678	3693	rVB	272409	779034	32.16%	7.802%




Sum of corrected areas: 9984947

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
Data File : BG057837.D
Acq On : 23 Jun 2023 11:19
Operator : CG/JU
Sample : 03238-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PMW-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

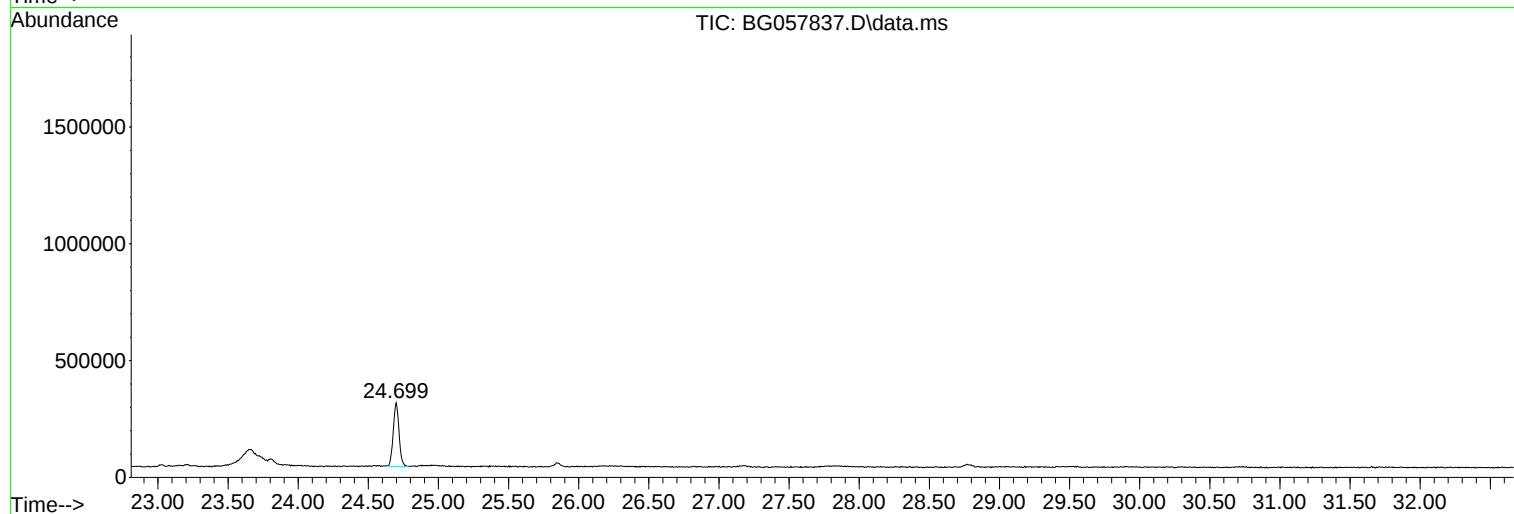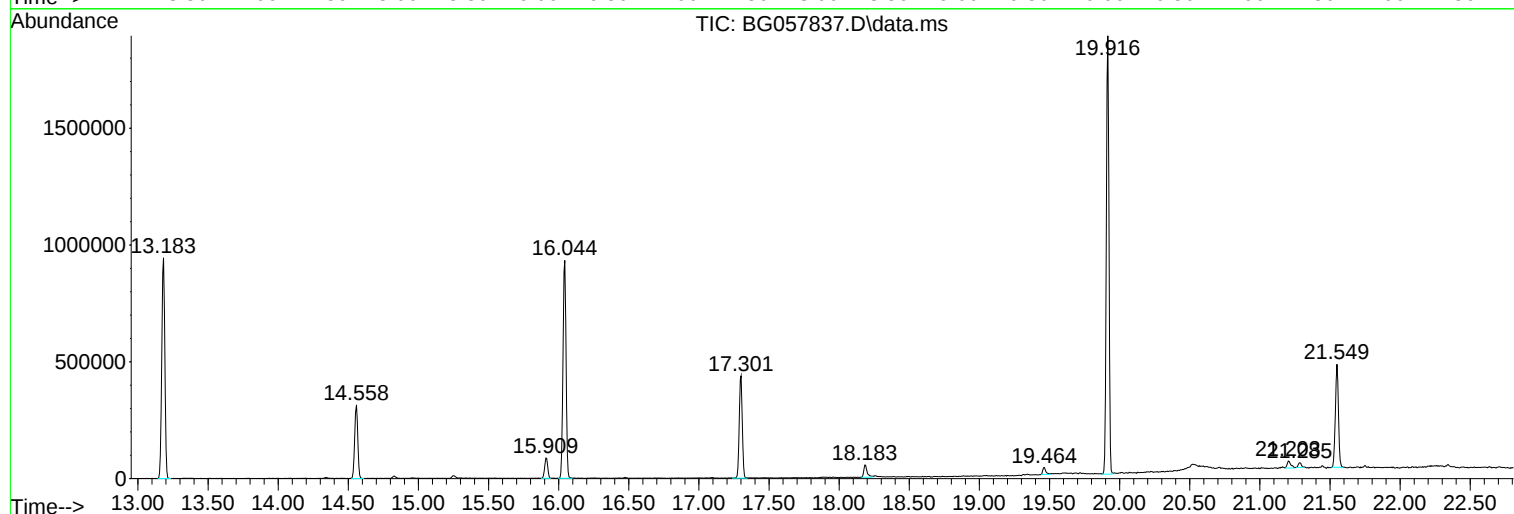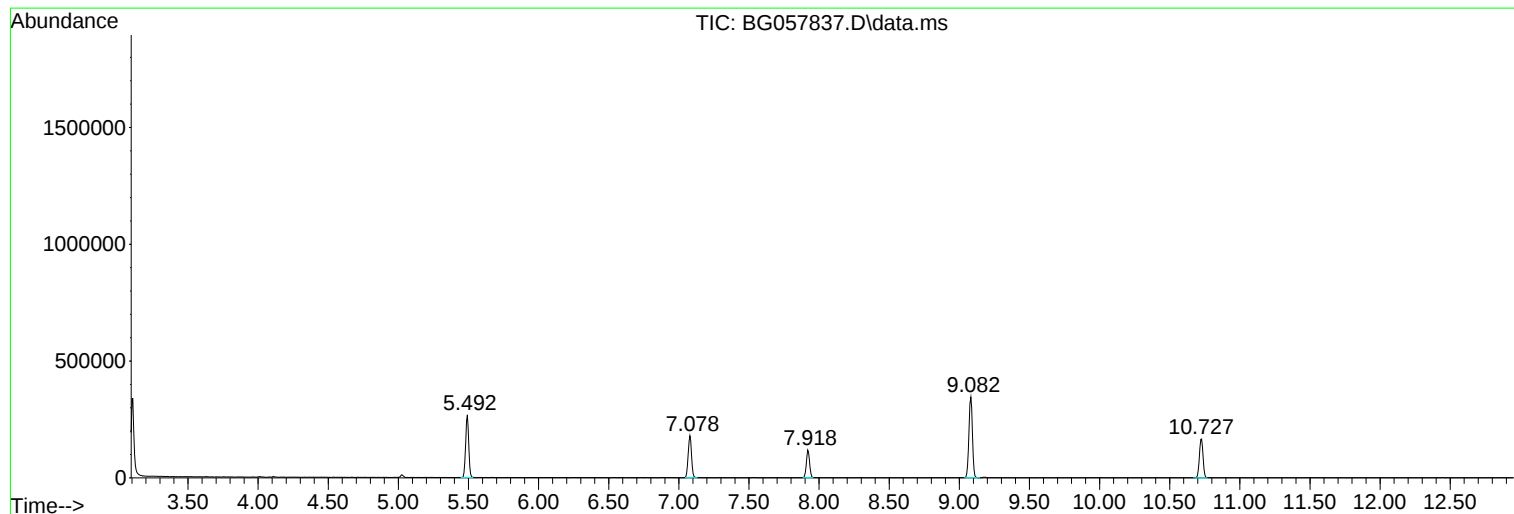

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
Data File : BG057837.D
Acq On : 23 Jun 2023 11:19
Operator : CG/JU
Sample : 03238-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PMW-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
Data File : BG057837.D
Acq On : 23 Jun 2023 11:19
Operator : CG/JU
Sample : 03238-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PMW-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc