


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
 Data File : BG057832.D
 Acq On : 23 Jun 2023 7:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 03:40:38 2023

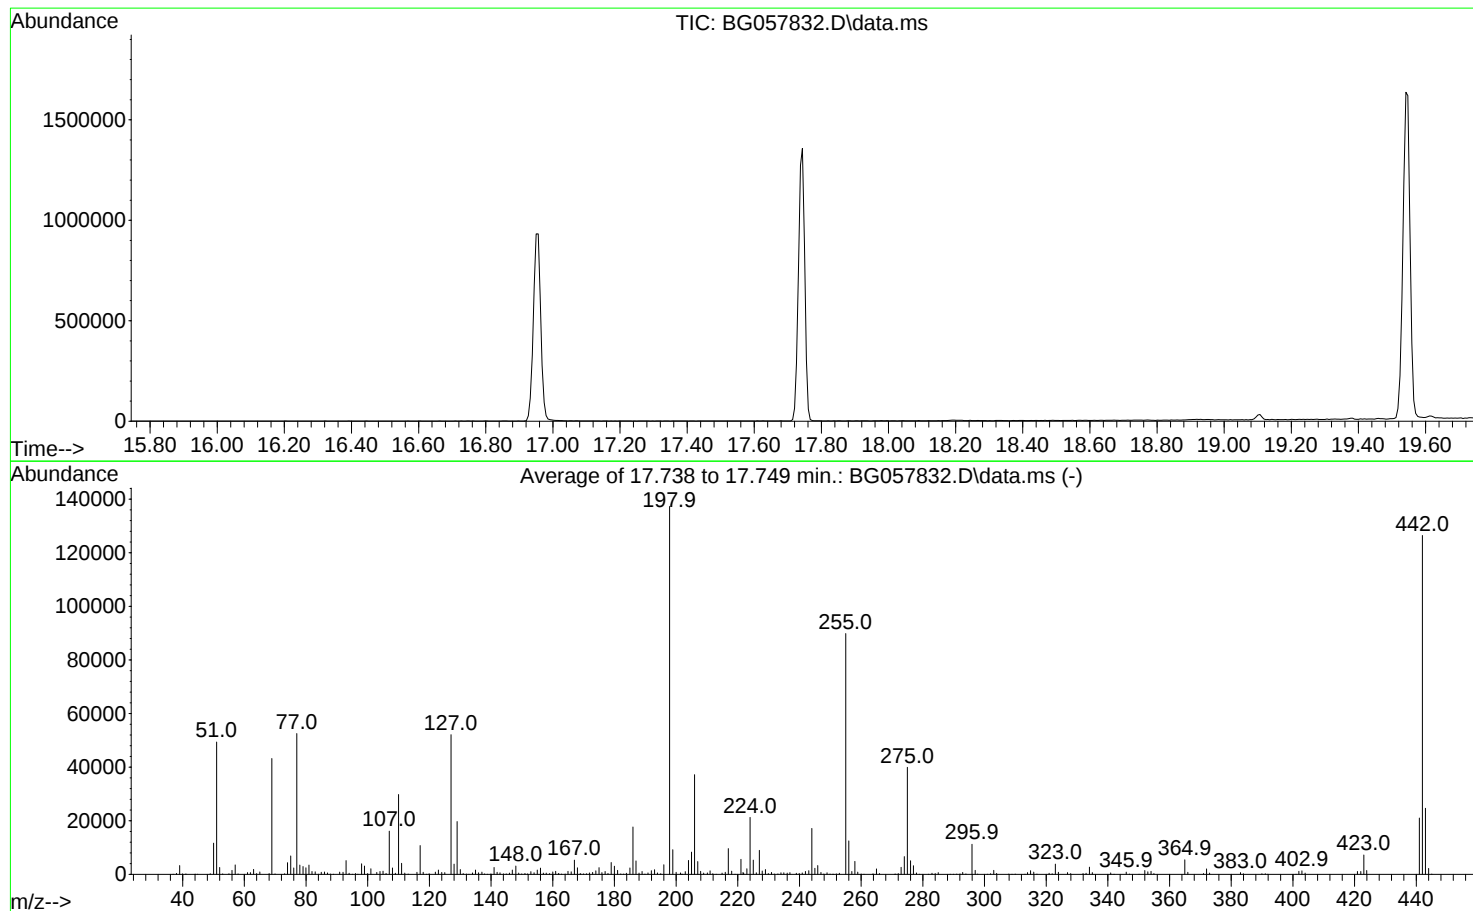

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	49355	PASS
68	69	0.00	2	0.8	325	PASS
69	198	0.00	100	31.5	43205	PASS
70	69	0.00	2	0.4	180	PASS
127	198	10	80	38.0	52117	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137245	PASS
199	198	5	9	6.7	9205	PASS
275	198	10	60	29.1	39920	PASS
365	198	1	100	4.0	5451	PASS
441	198	0.01	100	15.3	20997	PASS
442	442	50	100	100.0	126443	PASS
443	442	15	24	19.5	24669	PASS