
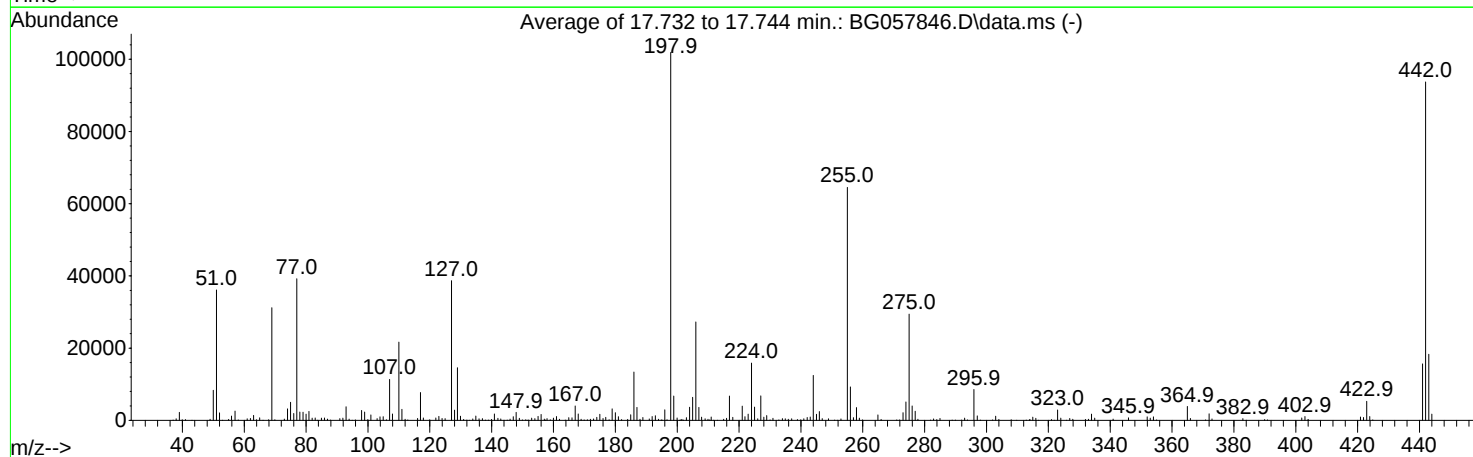


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062323\
 Data File : BG057846.D
 Acq On : 23 Jun 2023 17:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 03:40:38 2023

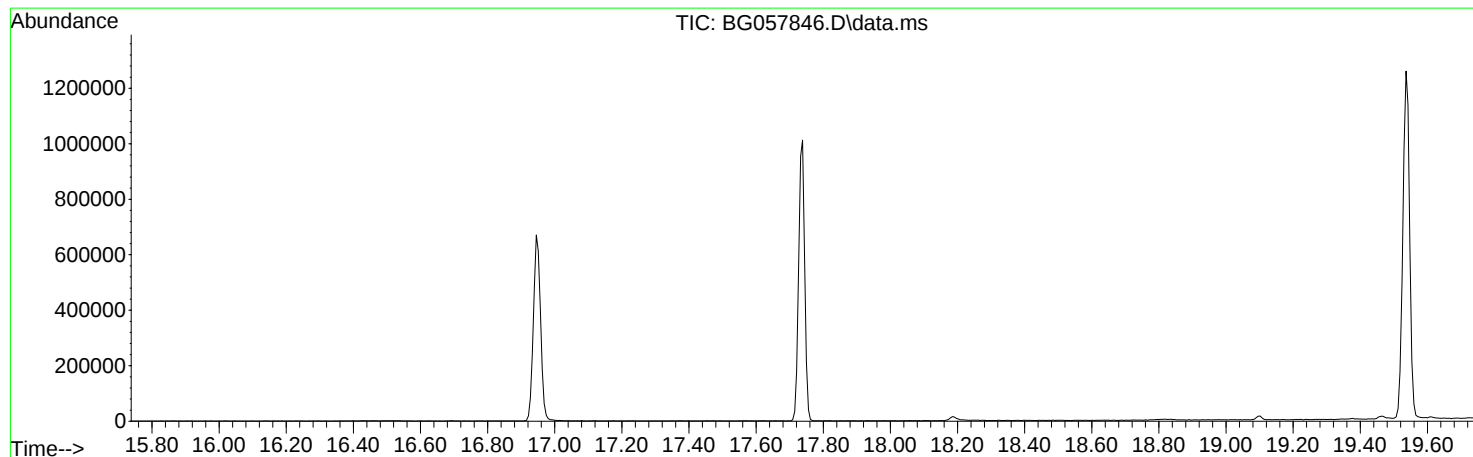

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	36107	PASS
68	69	0.00	2	0.6	202	PASS
69	198	0.00	100	30.6	31216	PASS
70	69	0.00	2	0.5	160	PASS
127	198	10	80	38.0	38688	PASS
197	198	0.00	2	0.2	174	PASS
198	198	100	100	100.0	101872	PASS
199	198	5	9	6.6	6745	PASS
275	198	10	60	28.9	29421	PASS
365	198	1	100	3.8	3837	PASS
441	198	0.01	100	15.3	15630	PASS
442	442	50	100	100.0	93728	PASS
443	442	15	24	19.5	18300	PASS