


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062419\
 Data File : BG041425.D
 Acq On : 24 Jun 2019 17:21
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

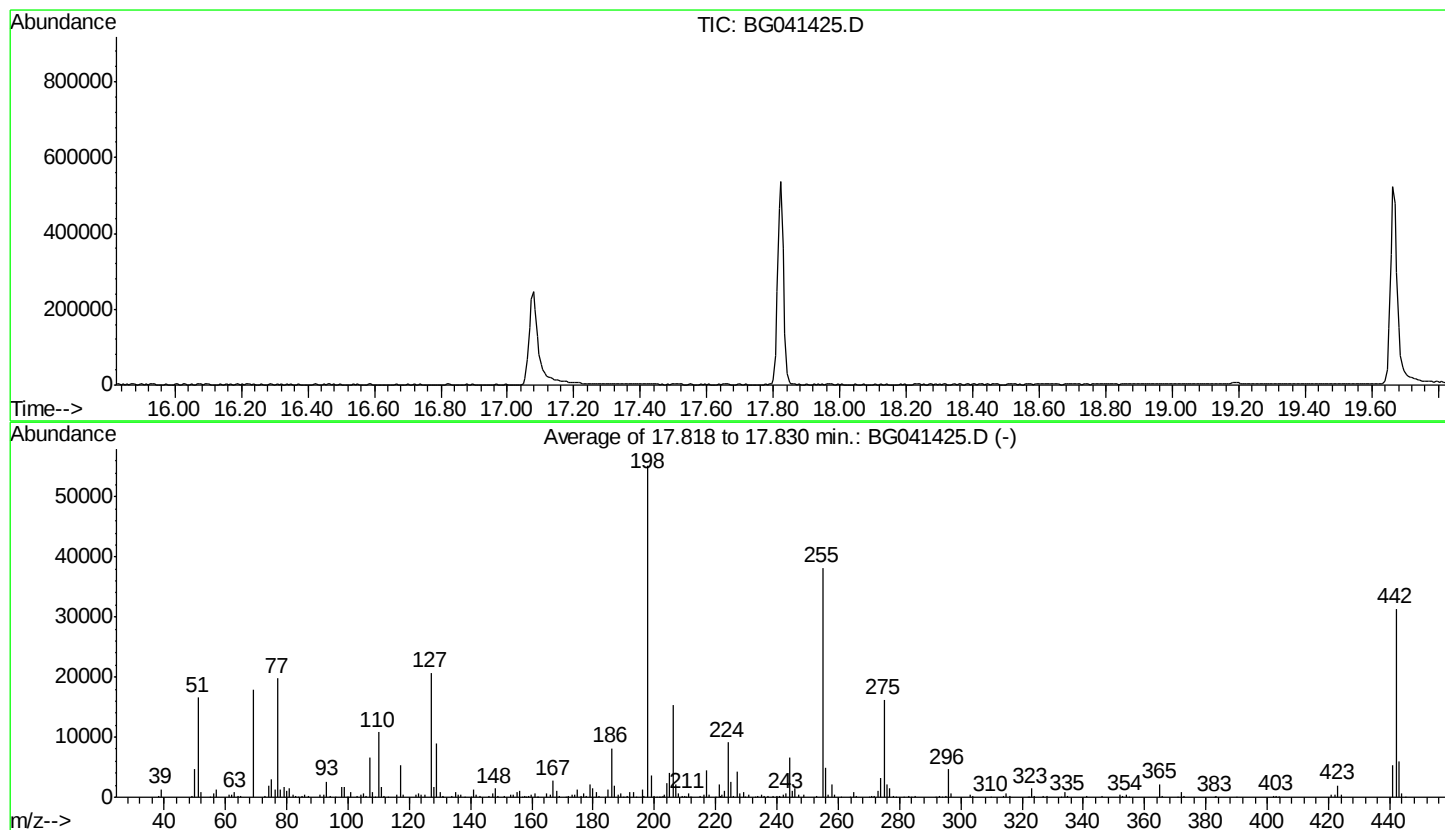

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	16562	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.3	17839	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.6	20761	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55202	PASS
199	198	5	9	6.7	3688	PASS
275	198	10	60	29.5	16286	PASS
365	198	1	100	3.9	2132	PASS
441	198	0.01	100	9.6	5288	PASS
442	198	50	100	56.8	31328	PASS
443	442	15	24	19.0	5958	PASS