
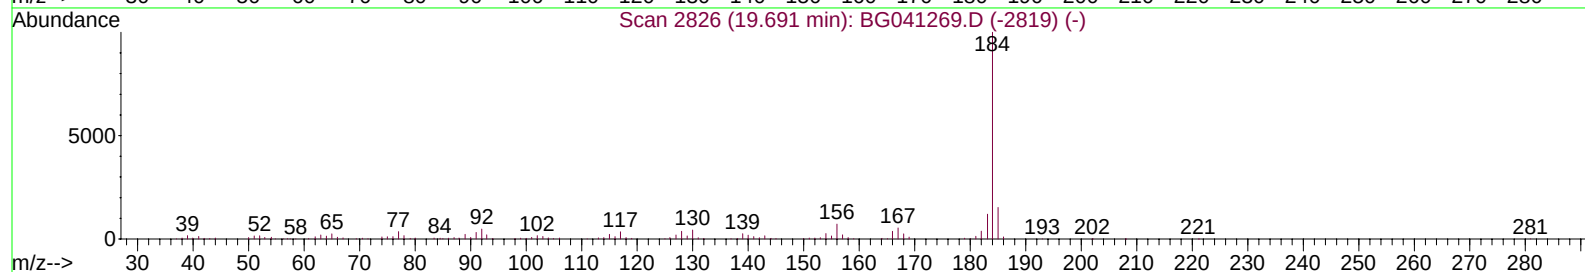
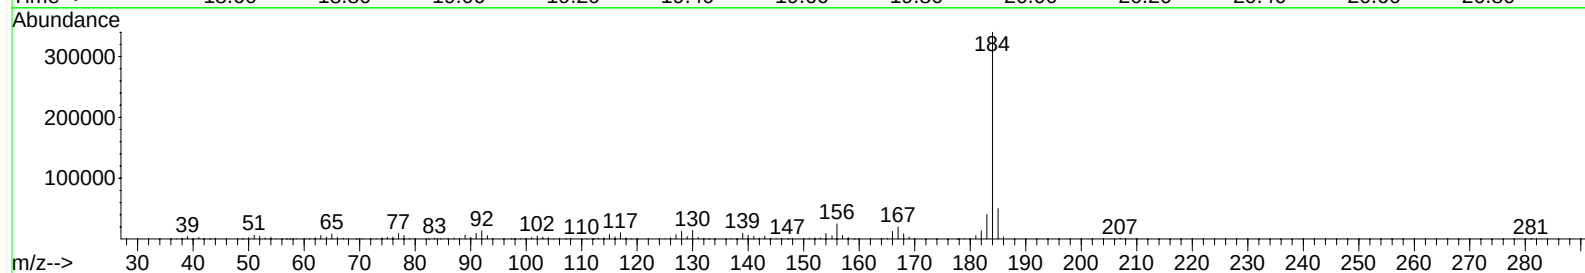


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062519\
Data File : BG041443.D
Acq On : 25 Jun 2019 11:15
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 12:07:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

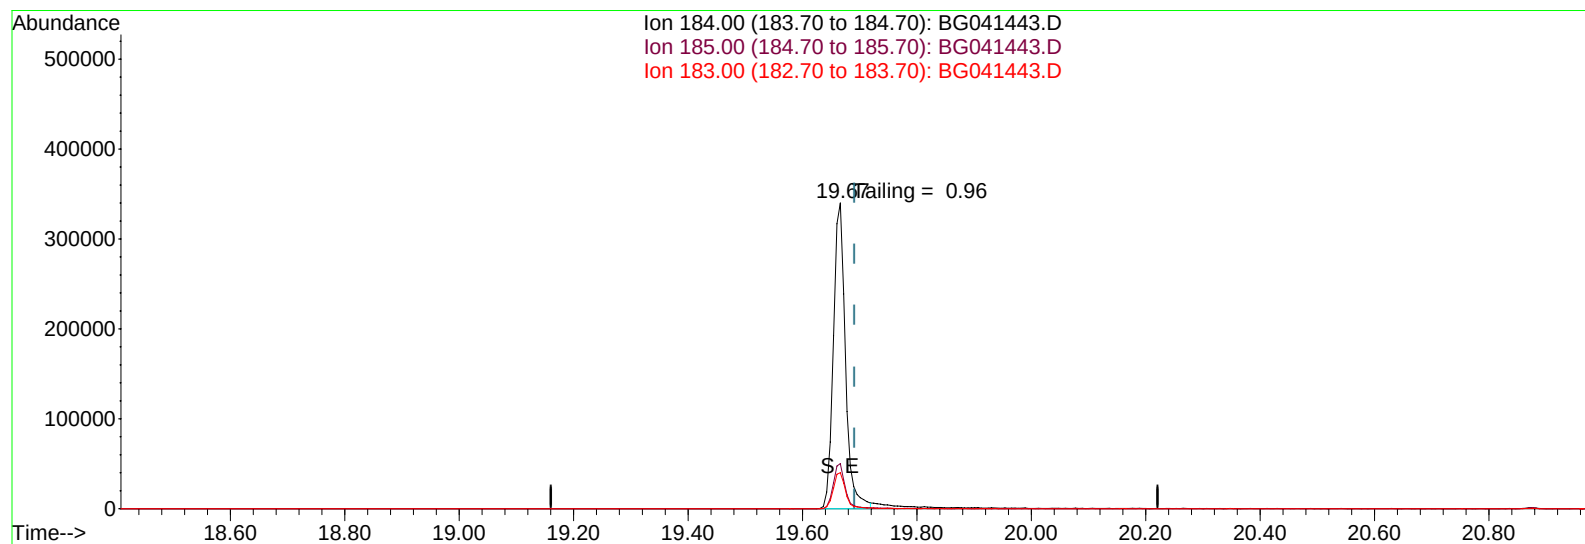

TIC: BG041443.D

(77) Benzidine




19.666min (-0.025) 0.00ng

response 517248

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.74
183.00	12.00	11.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062519\
Data File : BG041443.D
Acq On : 25 Jun 2019 11:15
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 12:07:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

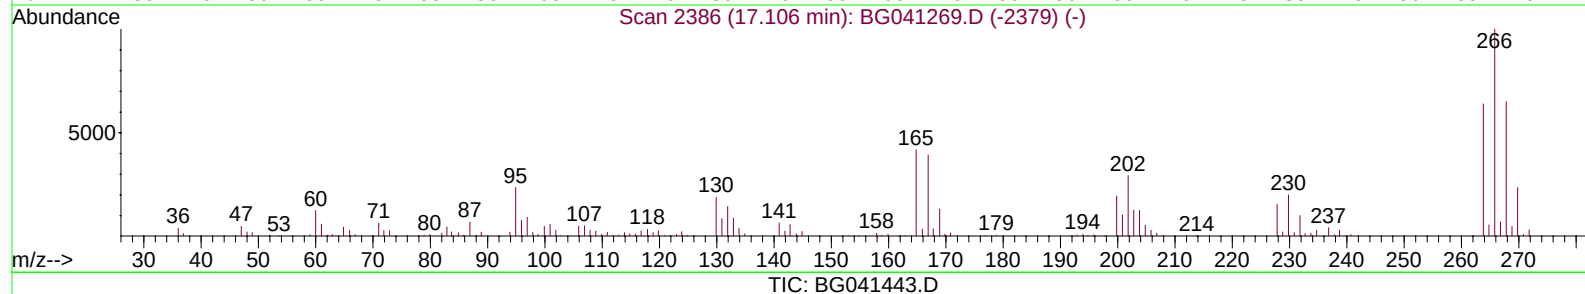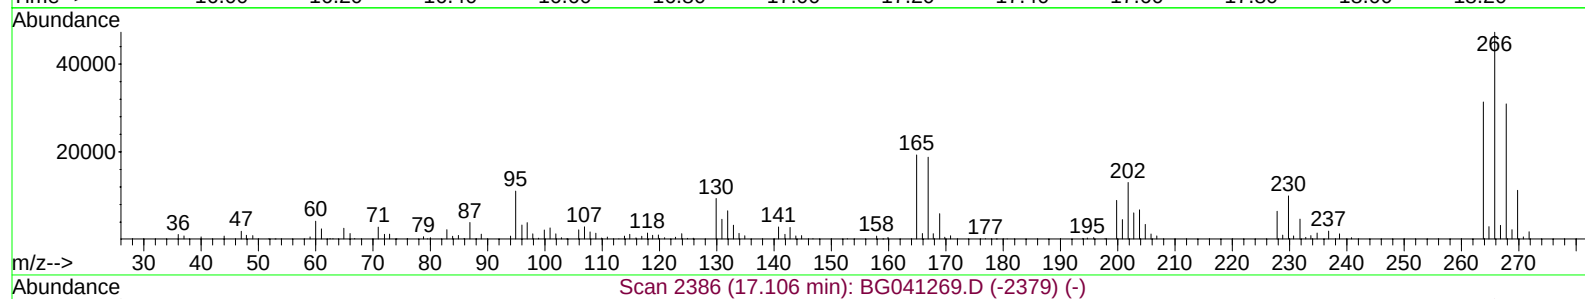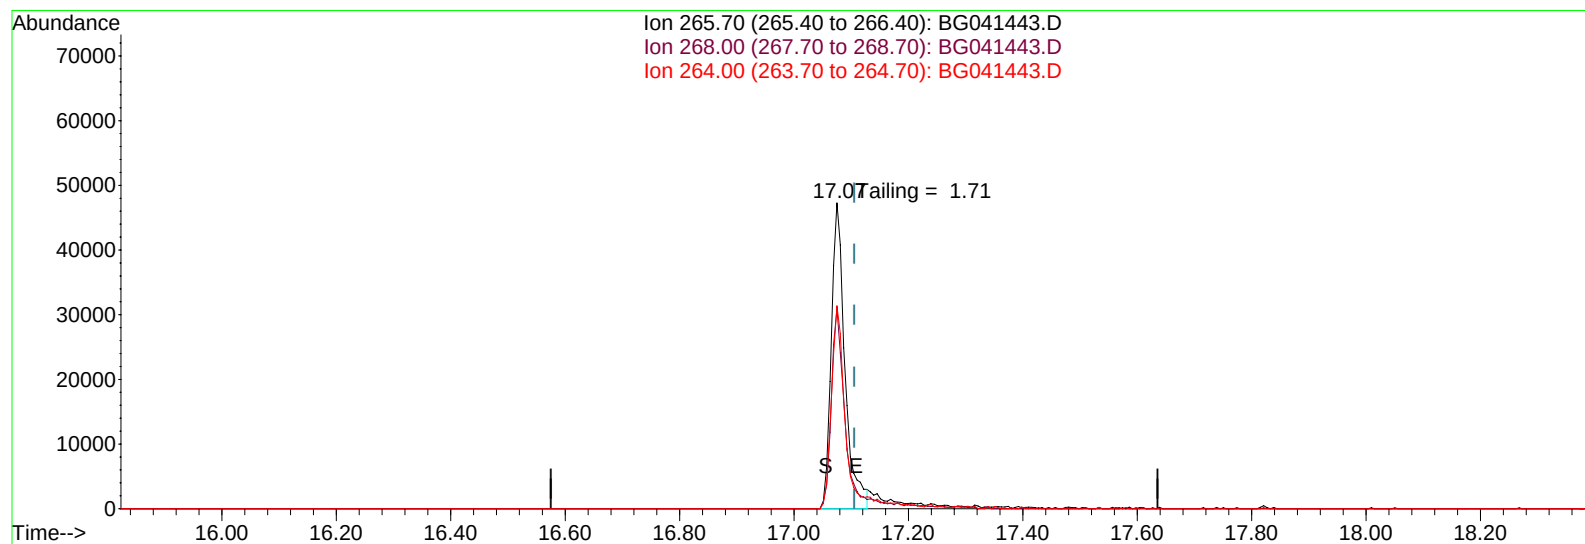

(70) Pentachlorophenol (C)

17.075min (-0.031) 24592.01ng

response 82123

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.48
264.00	64.00	66.36
0.00	0.00	0.00