
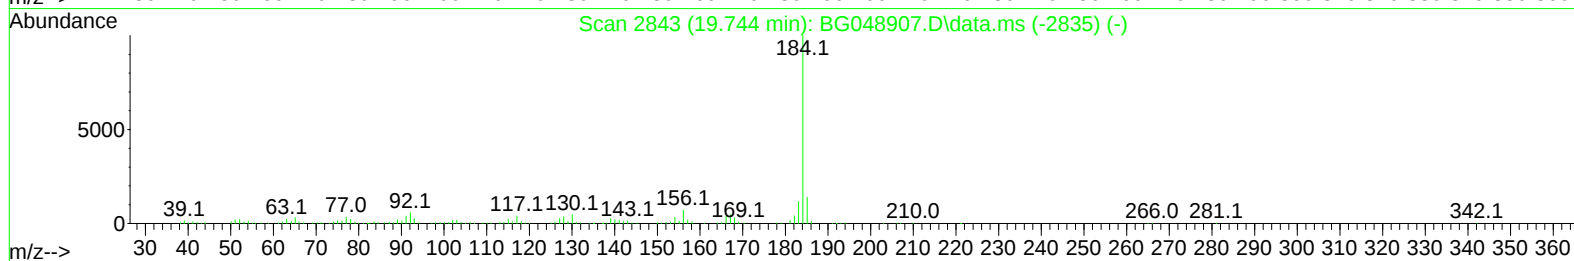
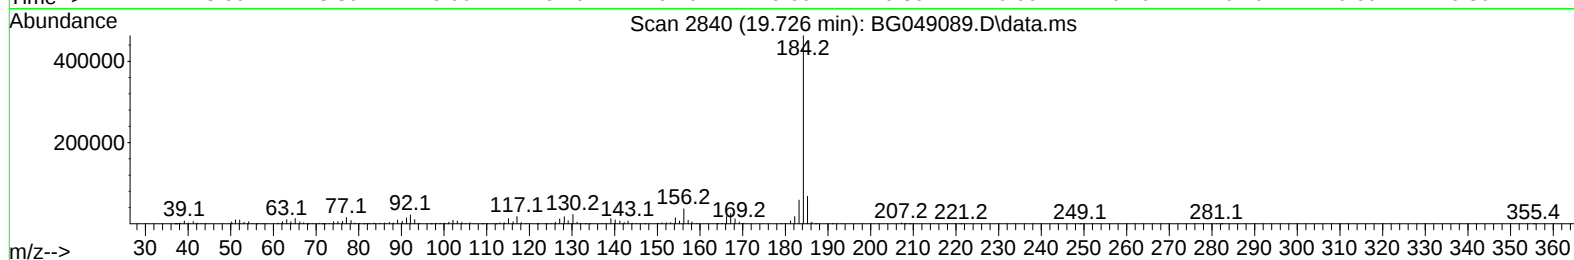


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062521\
Data File : BG049089.D
Acq On : 25 Jun 2021 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 14:30:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

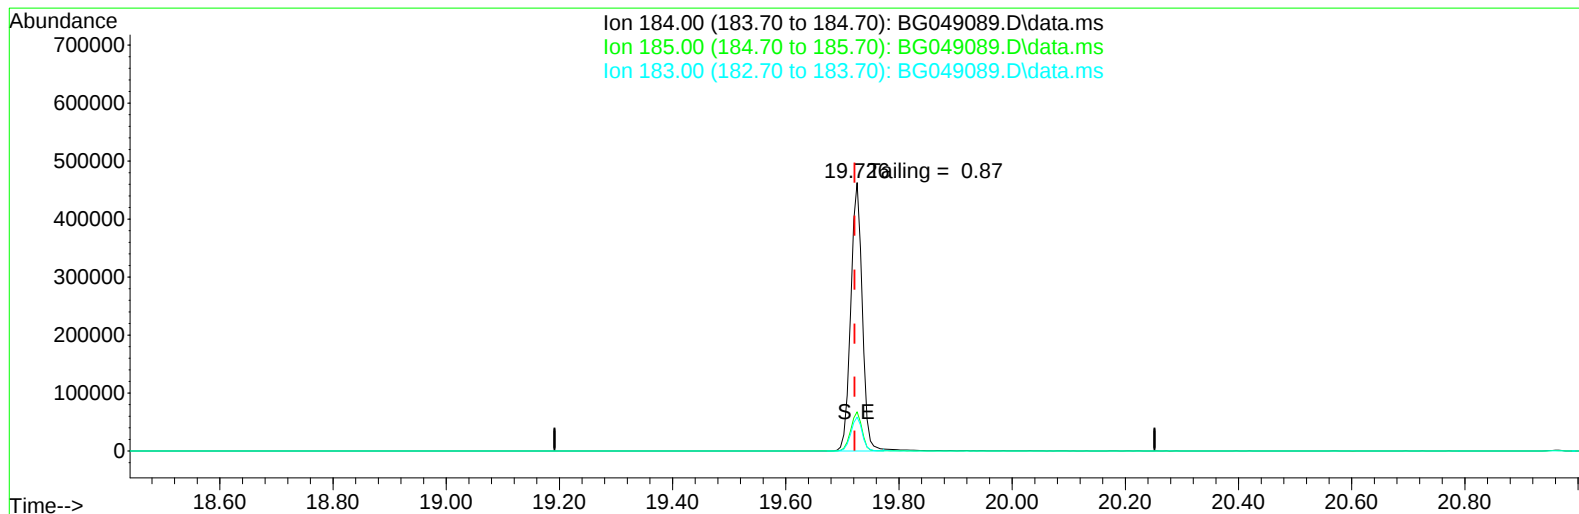

TIC: BG049089.D\data.ms

(77) Benzidine




19.726min (+ 0.005) 0.00 ng

response 659292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.62
183.00	11.70	12.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062521\
Data File : BG049089.D
Acq On : 25 Jun 2021 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 14:30:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

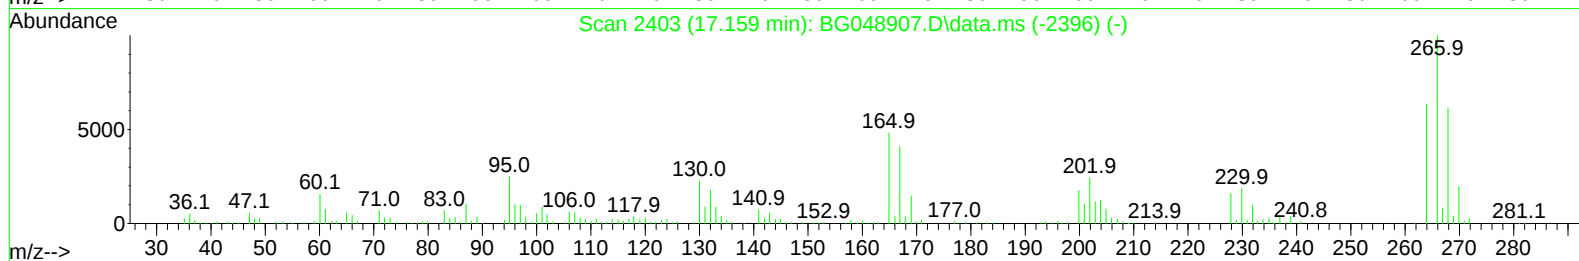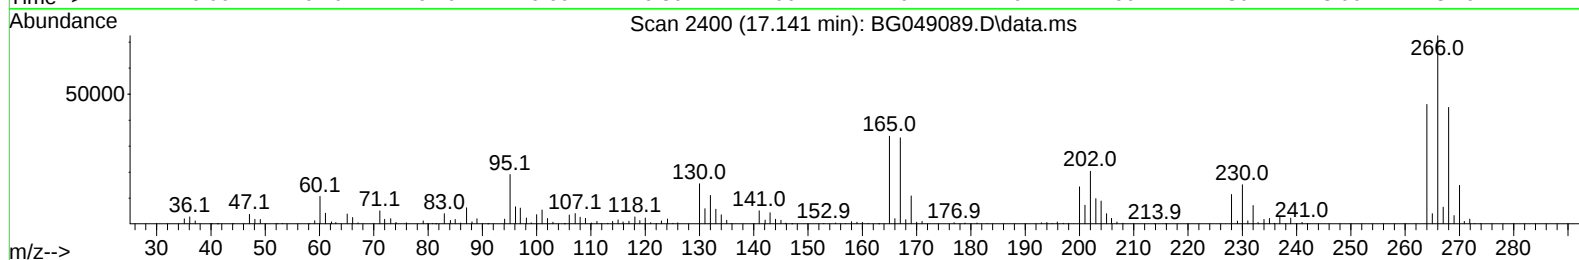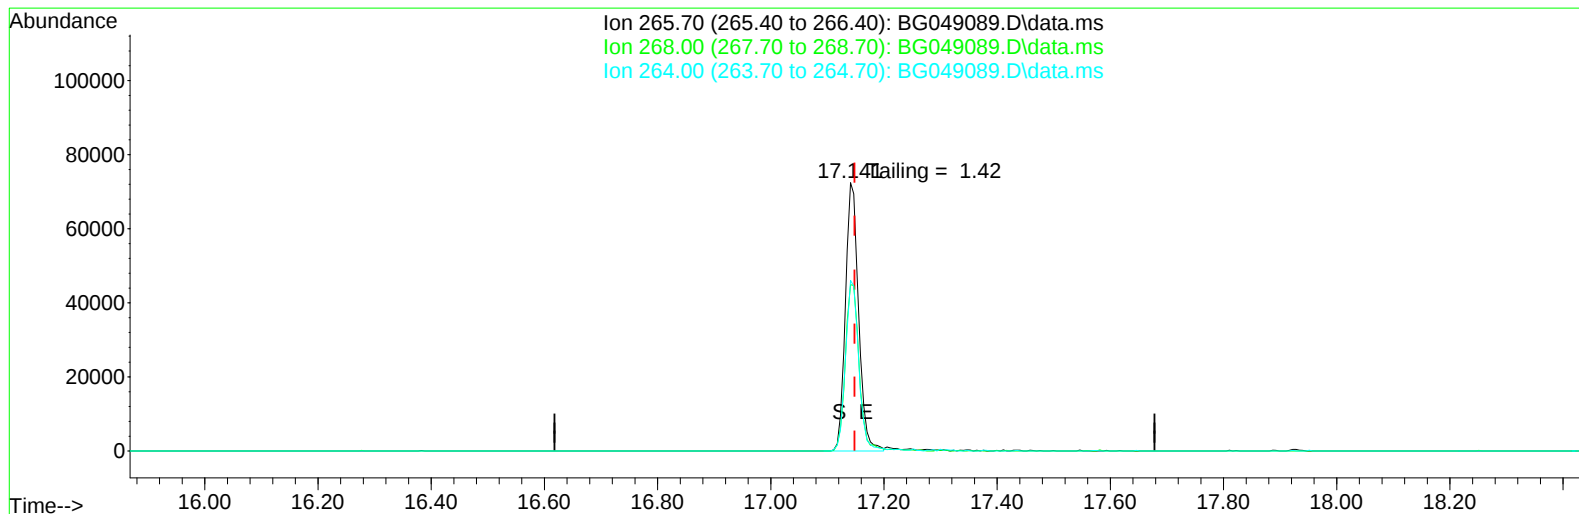

TIC: BG049089.D\data.ms

(70) Pentachlorophenol (C)

17.141min (-0.007) 25002.86 ng

response 117334

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.93
264.00	61.30	63.59
0.00	0.00	0.00