
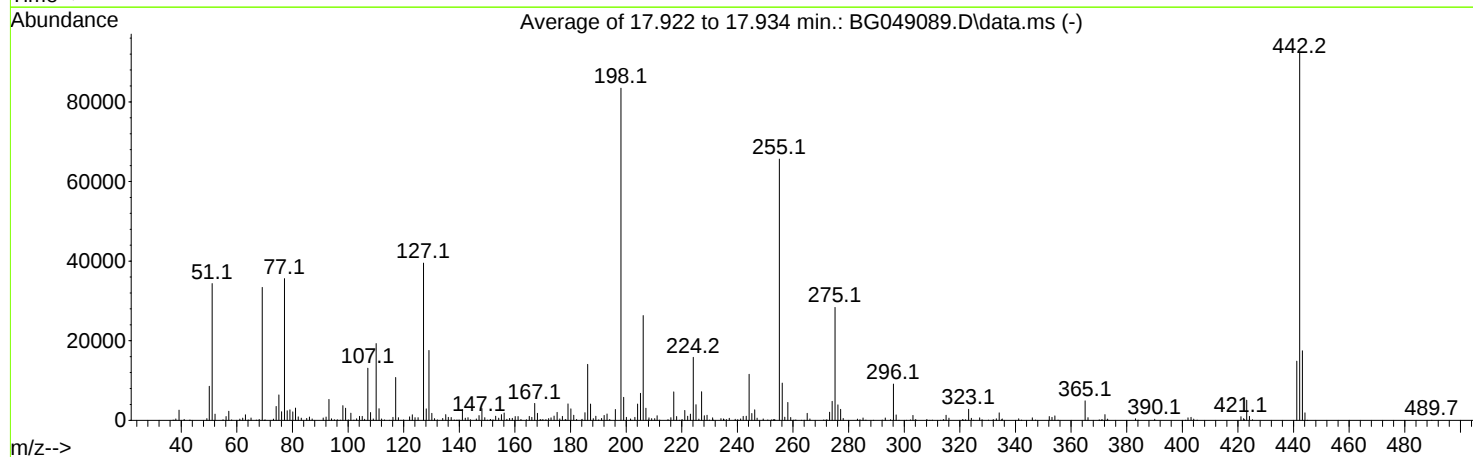


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062521\
 Data File : BG049089.D
 Acq On : 25 Jun 2021 12:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 24 11:02:36 2021

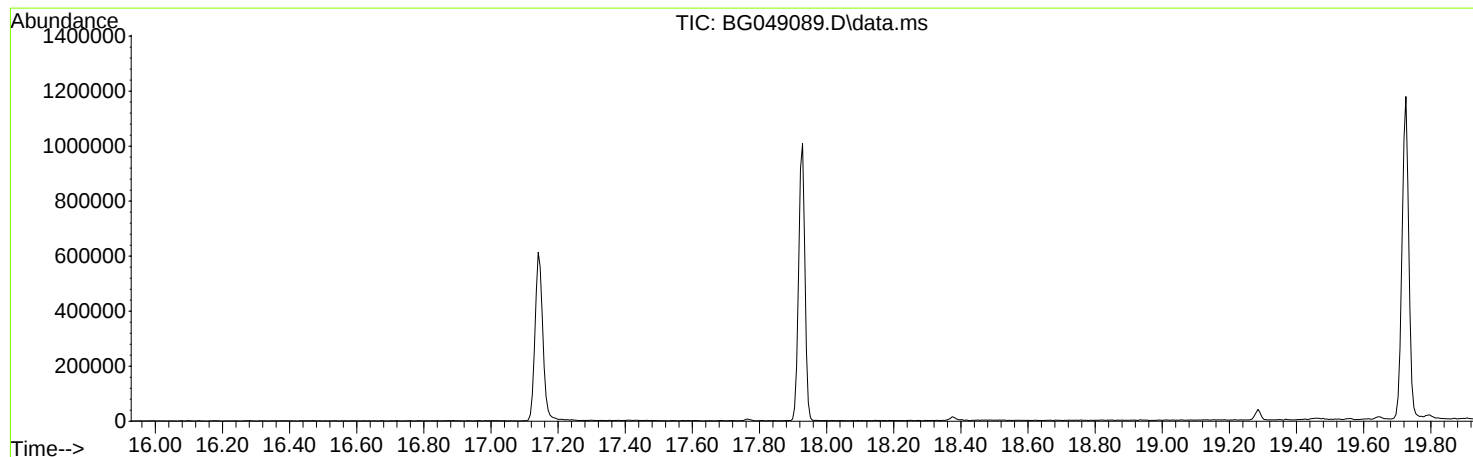

AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	34373	PASS
68	69	0.00	2	0.7	249	PASS
69	198	0.00	100	40.0	33392	PASS
70	69	0.00	2	0.4	143	PASS
127	198	10	80	47.3	39504	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83432	PASS
199	198	5	9	7.0	5804	PASS
275	198	10	60	34.0	28392	PASS
365	198	1	100	5.9	4892	PASS
441	198	0.01	100	17.8	14865	PASS
442	442	100	100	100.0	92400	PASS
443	442	15	24	18.9	17476	PASS

Instrument :
BNA_G
ClientSampleId :
DFTPP

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/25/2021	BNA_G	<u>BG049089.D</u>
Compound Name	Response	Retention Time
DDT	212177	20.96
DDD	1753	20.51
DDE	145	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1898	214075	0.89

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062521\
Data File : BG049089.D
Acq On : 25 Jun 2021 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 25 14:30:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

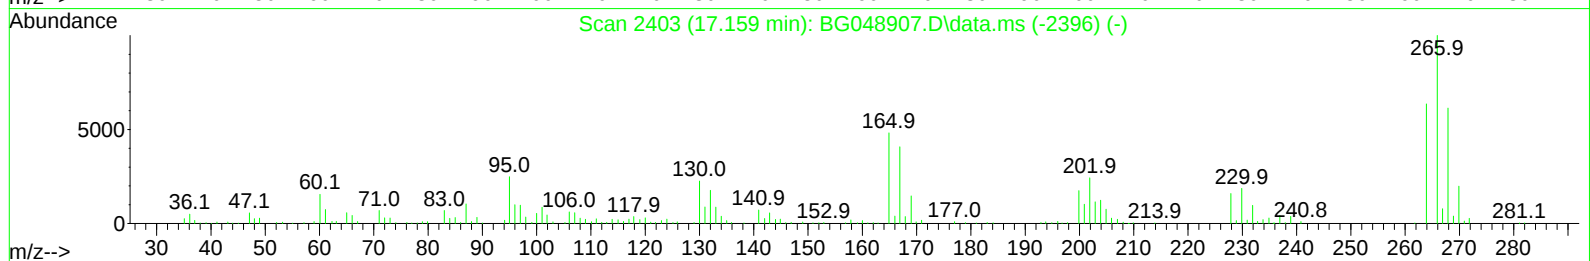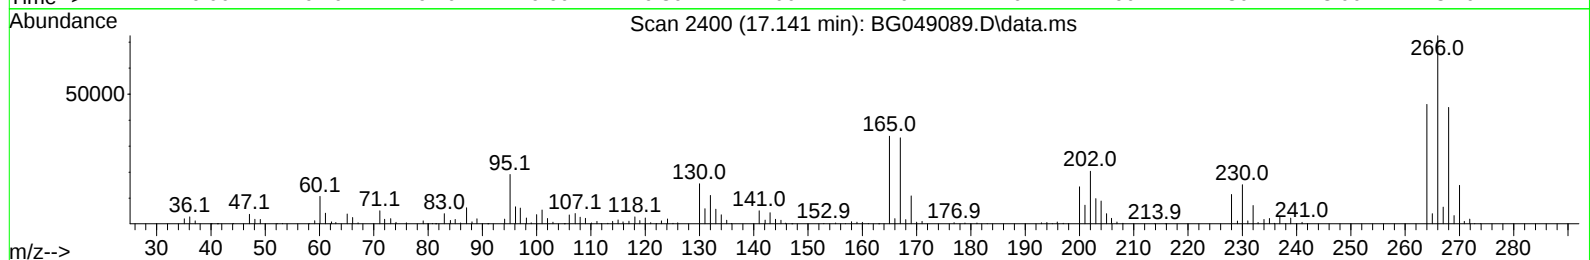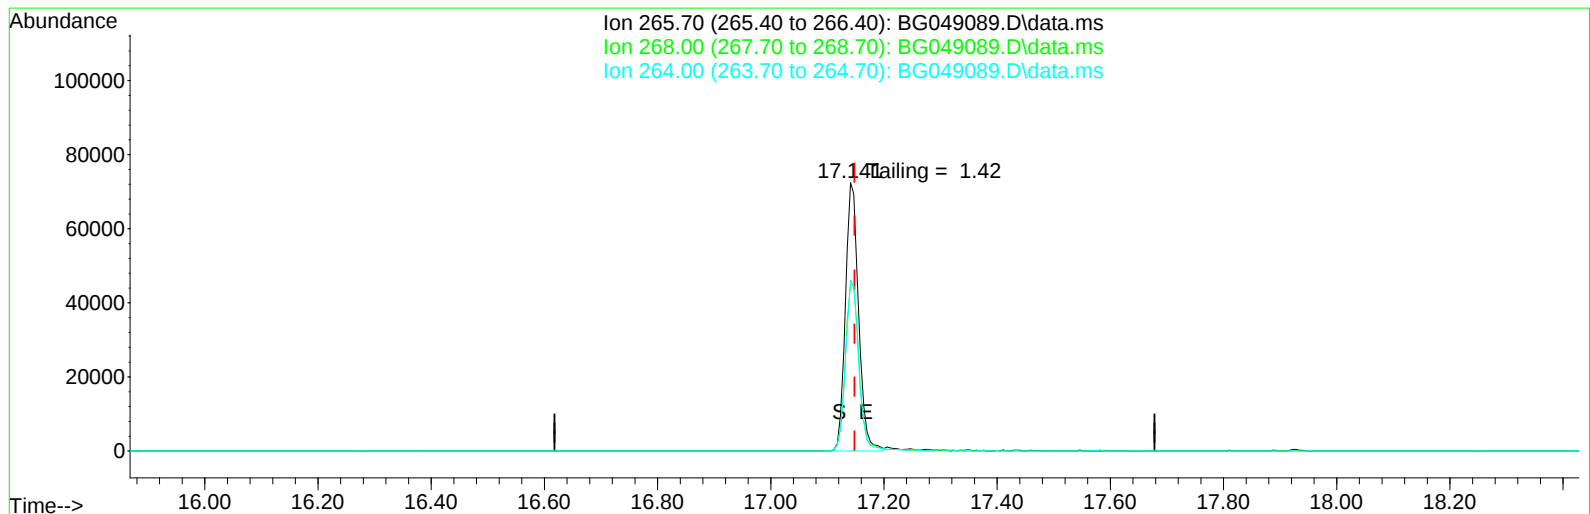

TIC: BG049089.D\data.ms

(70) Pentachlorophenol (C)

17.141min (-0.007) 25002.86 ng




response 117334

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.93
264.00	61.30	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062521\
Data File : BG049089.D
Acq On : 25 Jun 2021 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 25 14:30:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

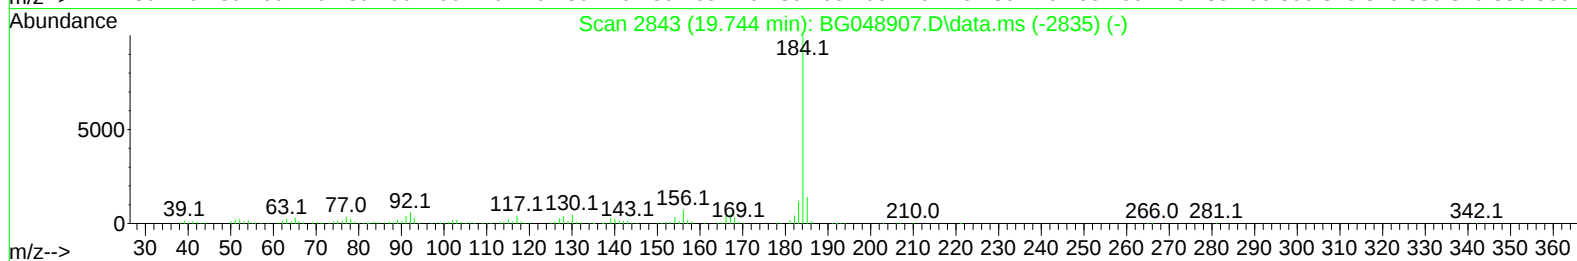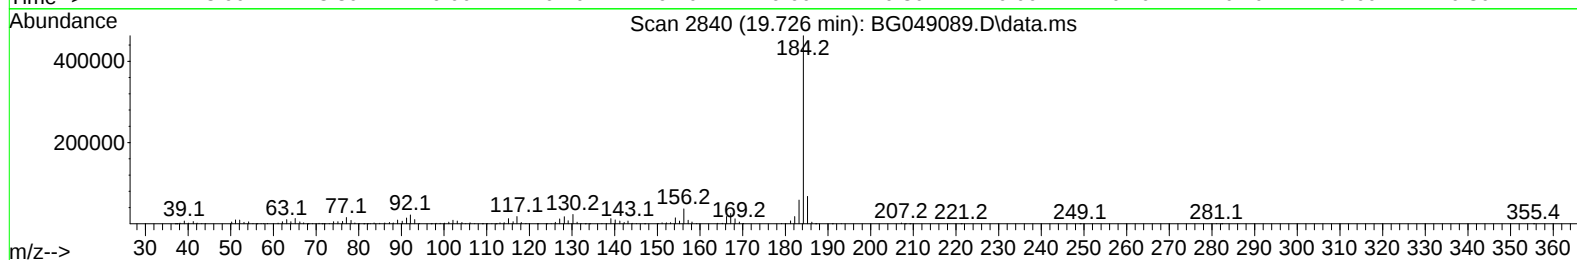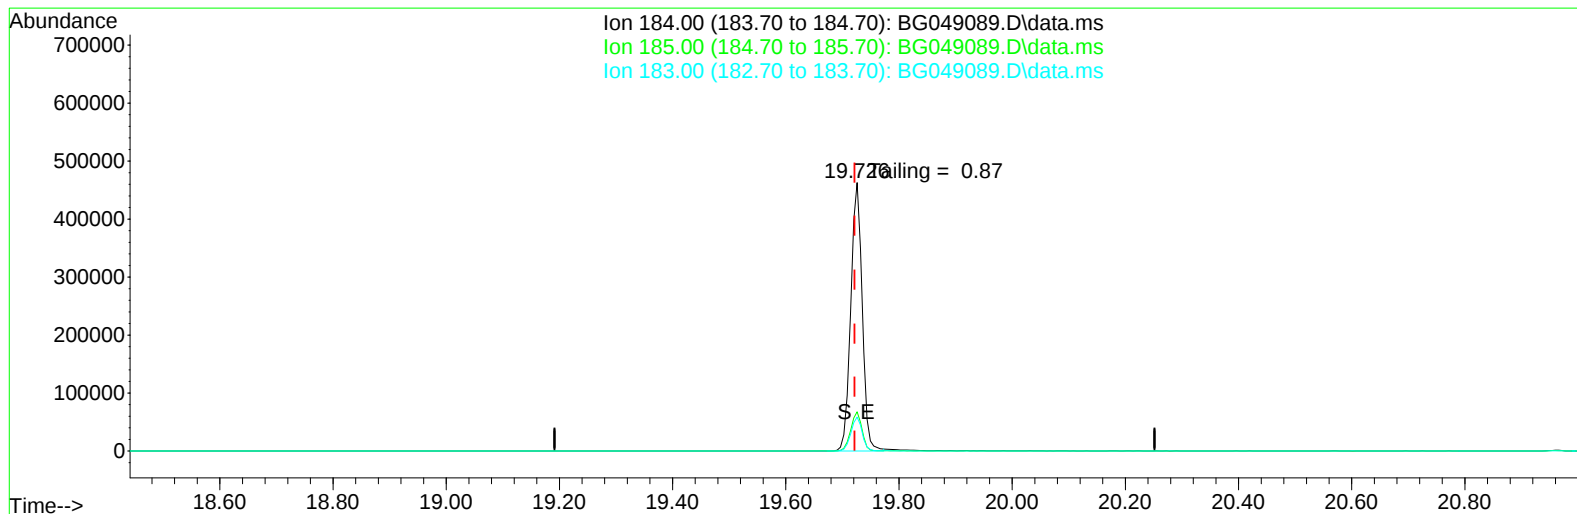

TIC: BG049089.D\data.ms

(77) Benzidine

19.726min (+ 0.005) 0.00 ng

response 659292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.62
183.00	11.70	12.65
0.00	0.00	0.00