
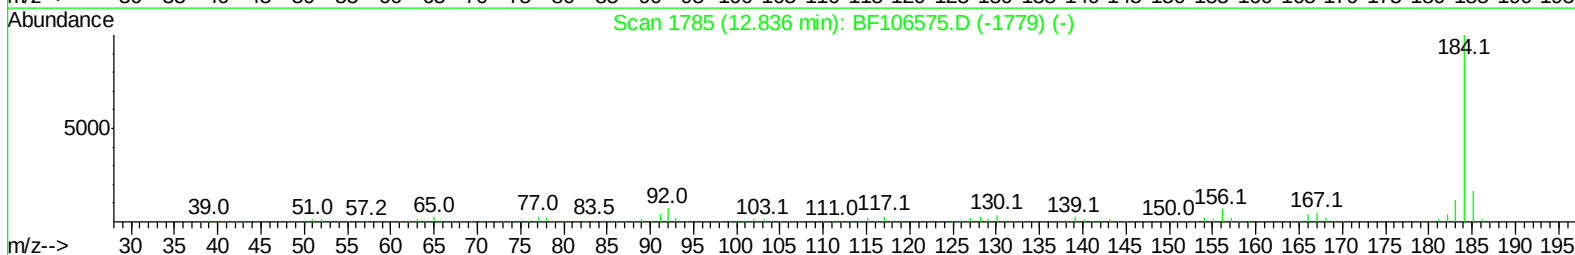
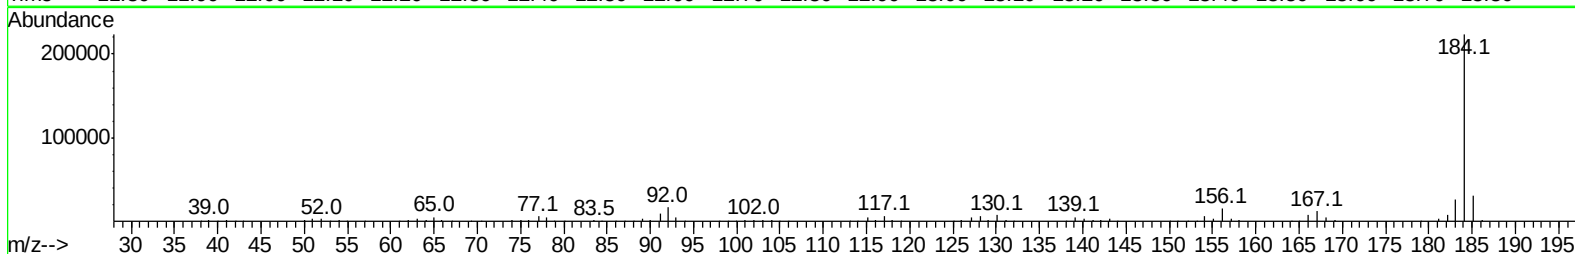


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062718\
Data File : BF106862.D
Acq On : 27 Jun 2018 10:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 09:26:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 25 18:50:17 2018
Response via : Initial Calibration

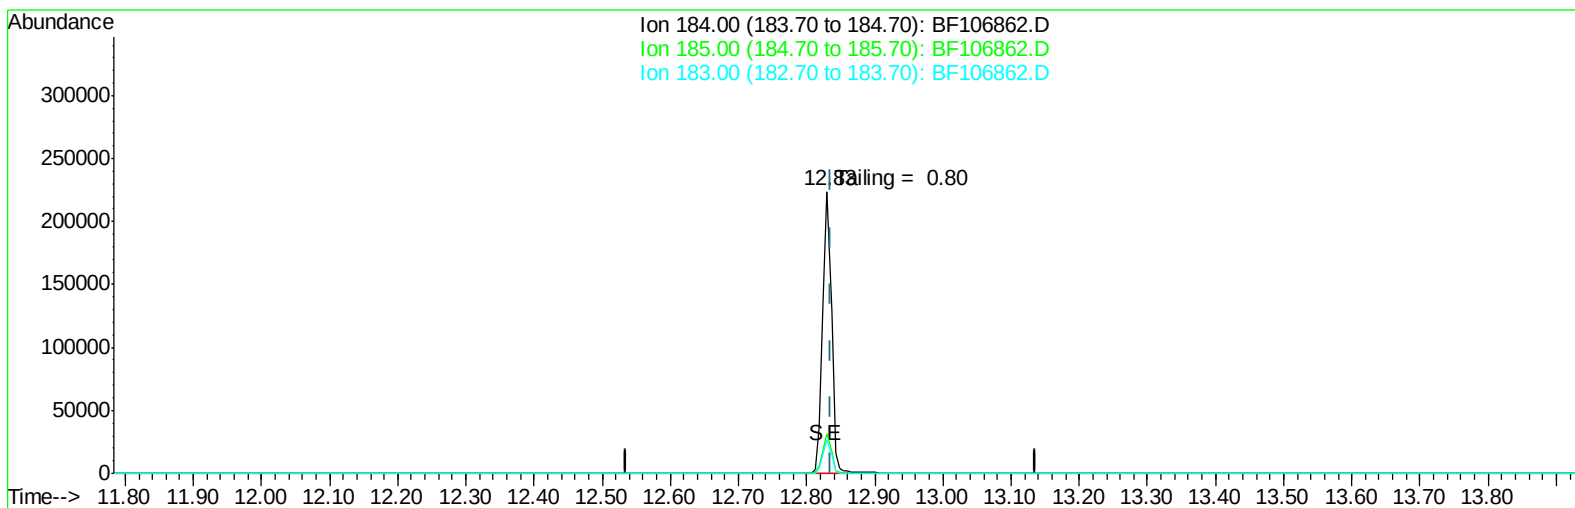

TIC: BF106862.D

(76) Benzidine




12.830min (-0.006) 1115.66ng

response 197441

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.10
183.00	11.60	11.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062718\
Data File : BF106889.D
Acq On : 27 Jun 2018 23:45
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 09:28:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 25 18:50:17 2018
Response via : Initial Calibration

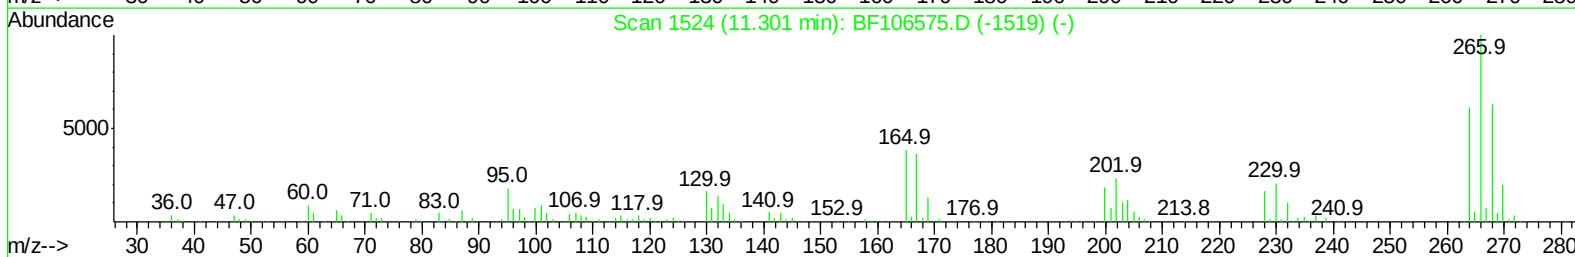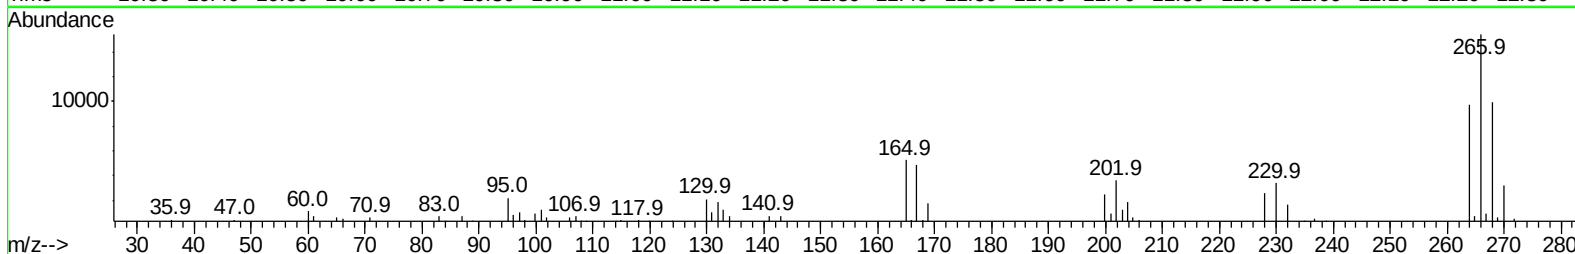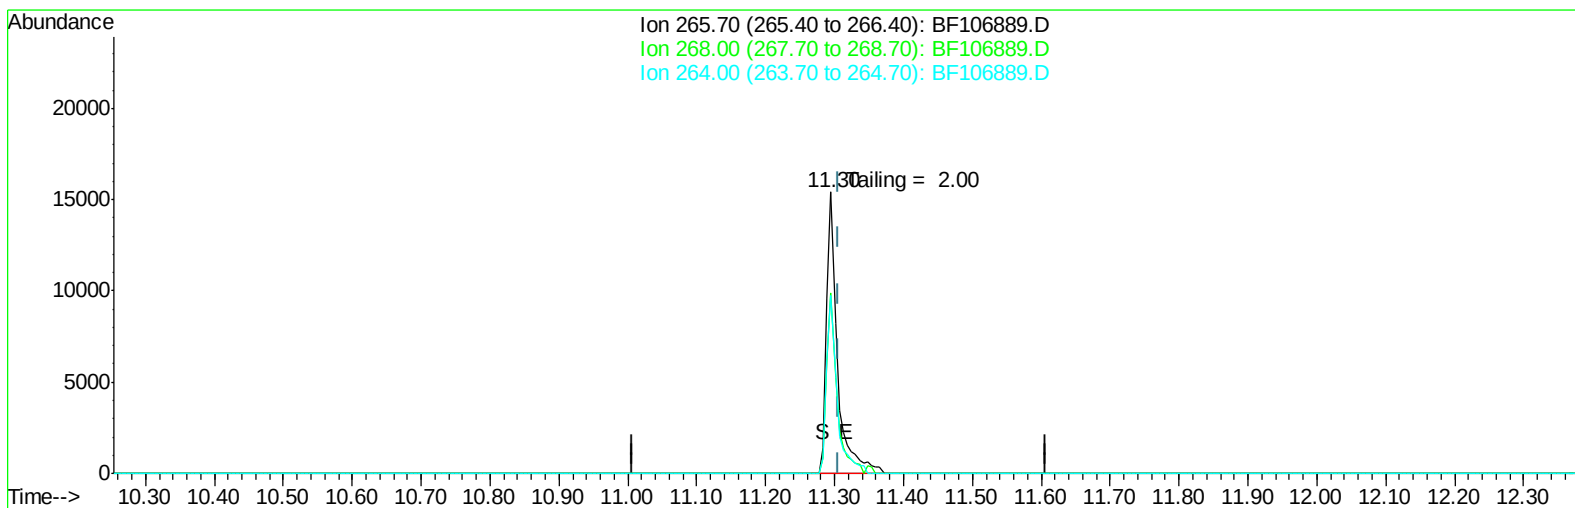

TIC: BF106889.D

(69) Pentachlorophenol (C)

11.295min (-0.012) 0.00ng

response 16597

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.21
264.00	61.90	63.05
0.00	0.00	0.00