
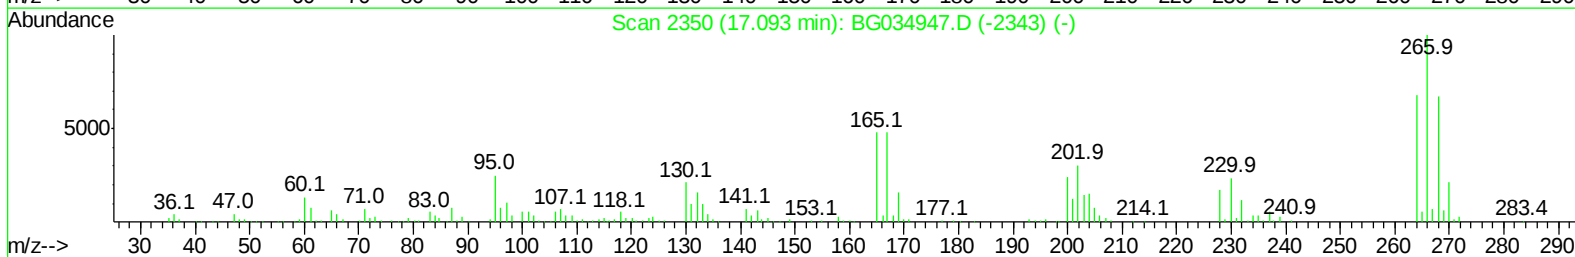
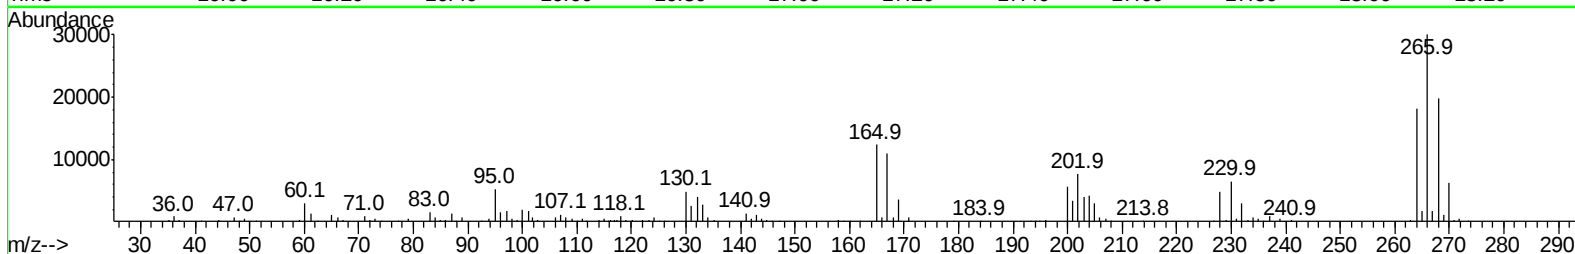


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
Data File : BG035408.D
Acq On : 26 Jun 2018 13:08
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 09:30:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

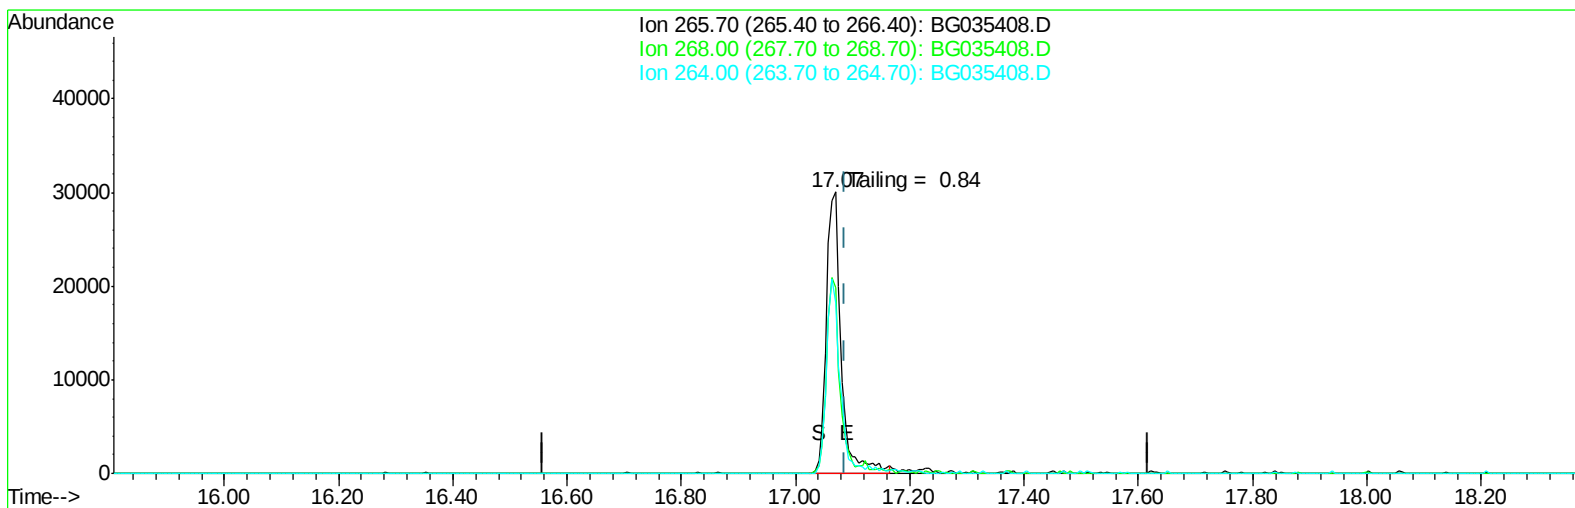

TIC: BG035408.D

(69) Pentachlorophenol (C)




17.069min (-0.018) 0.00ng

response 53569

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.96
264.00	62.00	60.69
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
Data File : BG035408.D
Acq On : 26 Jun 2018 13:08
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 09:30:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

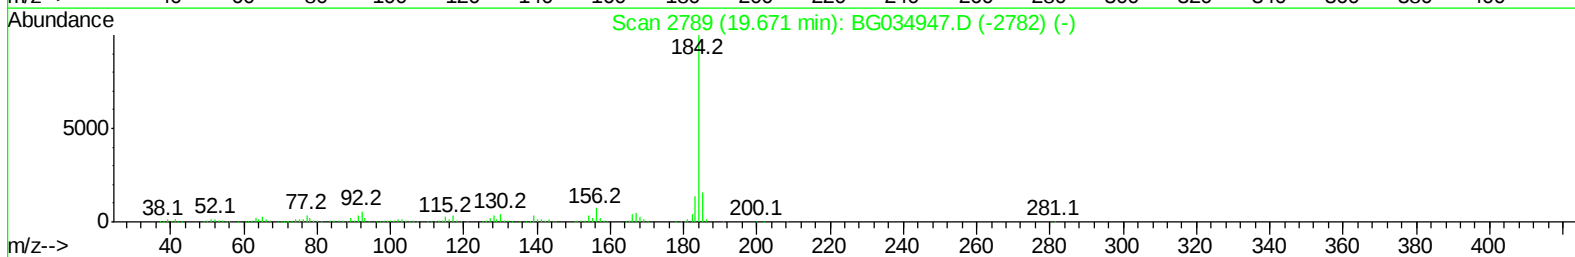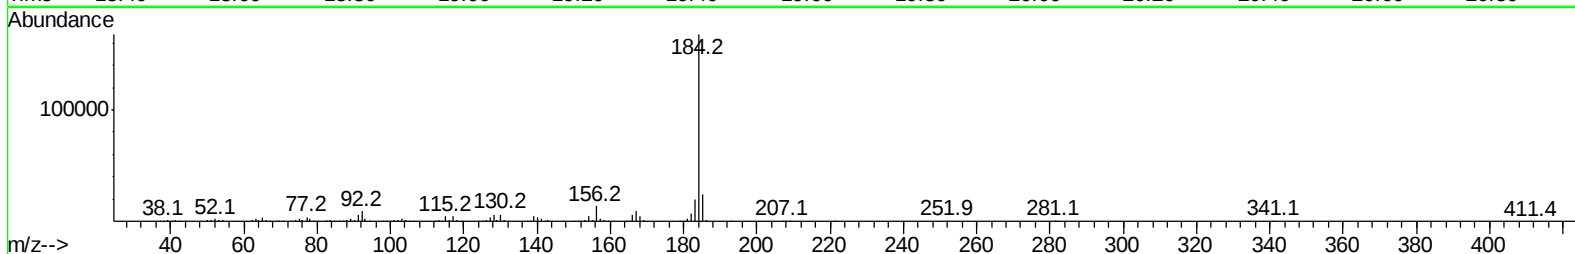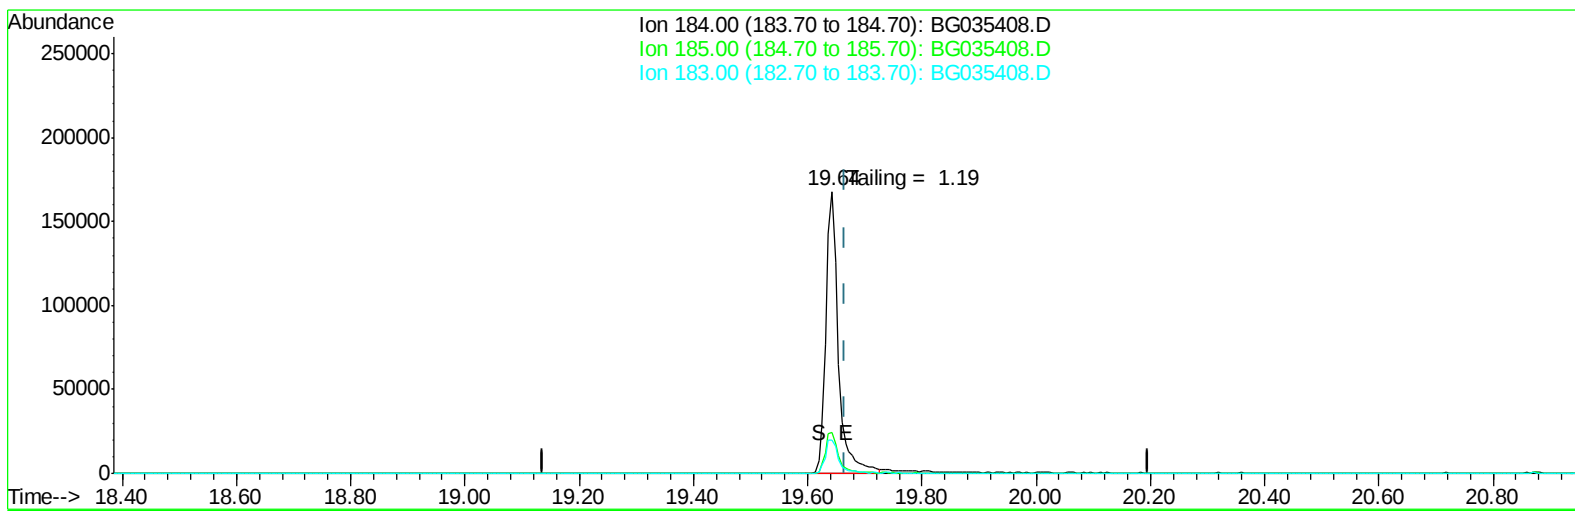

TIC: BG035408.D

(76) Benzidine

19.642min (-0.024) 128243.14ng

response 257640

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.60
183.00	13.30	11.79
0.00	0.00	0.00