
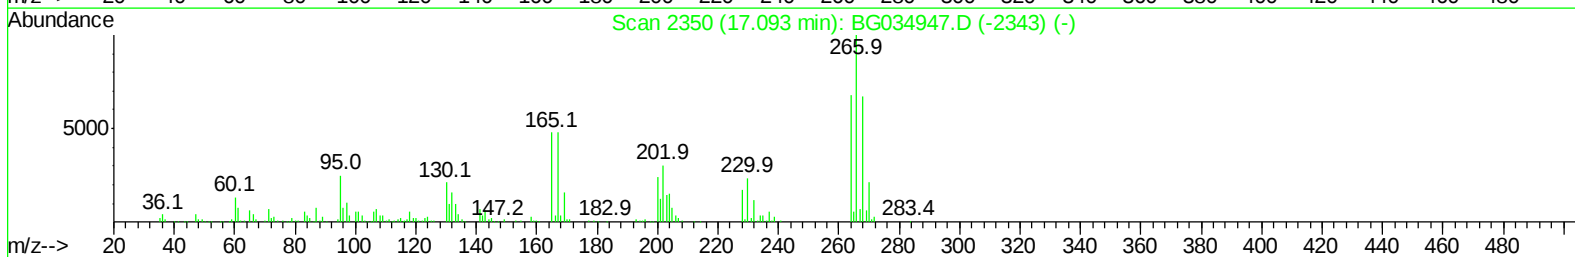
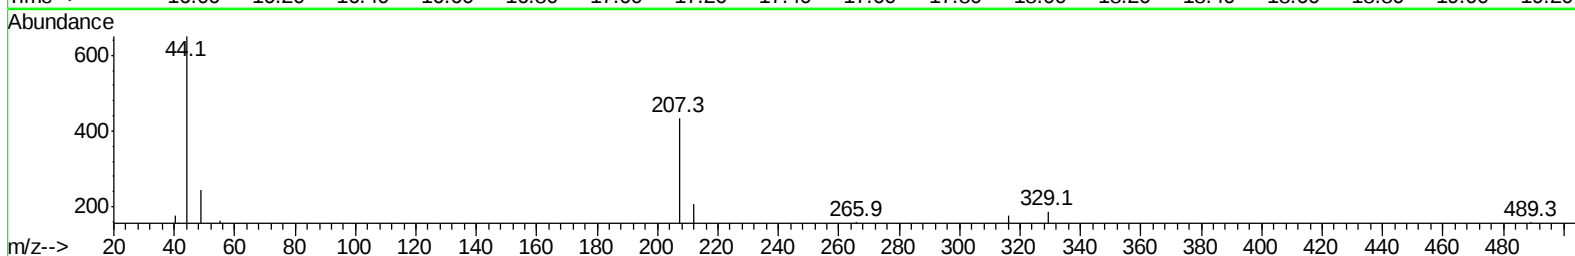


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
Data File : BG035426.D
Acq On : 27 Jun 2018 2:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 09:54:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

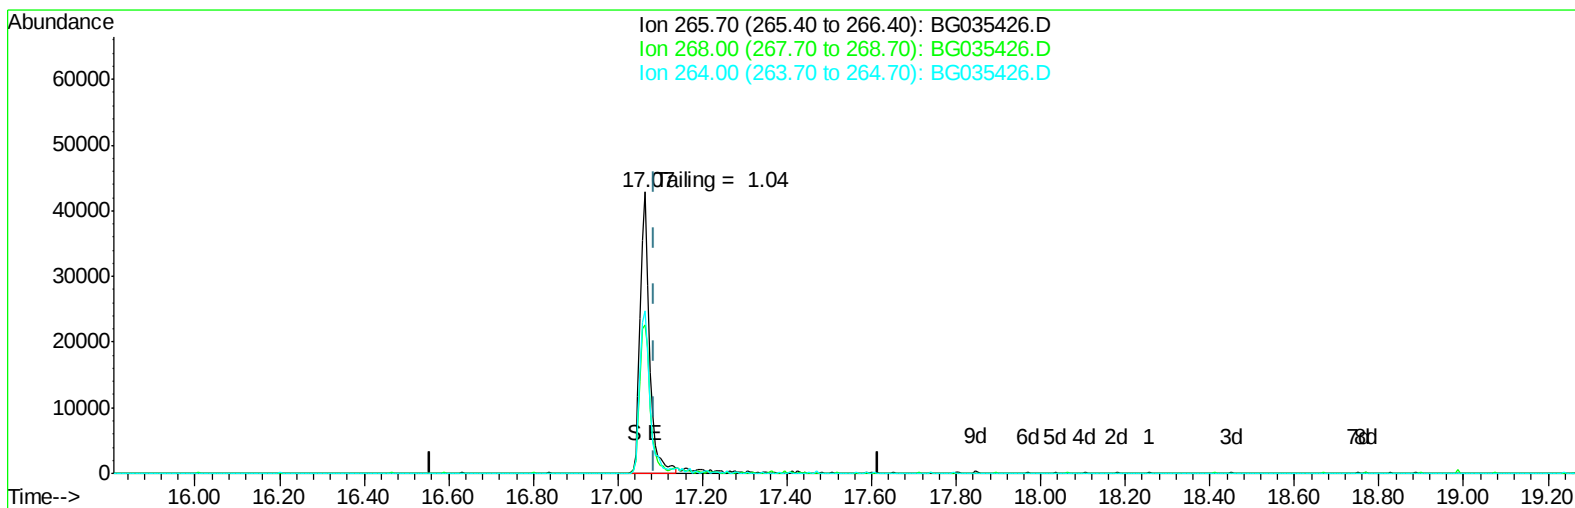

TIC: BG035426.D

(69) Pentachlorophenol (C)




18.258min (+1.170) 77.70ng

response 57

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	0.00#
264.00	62.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
 Data File : BG035426.D
 Acq On : 27 Jun 2018 2:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 09:54:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

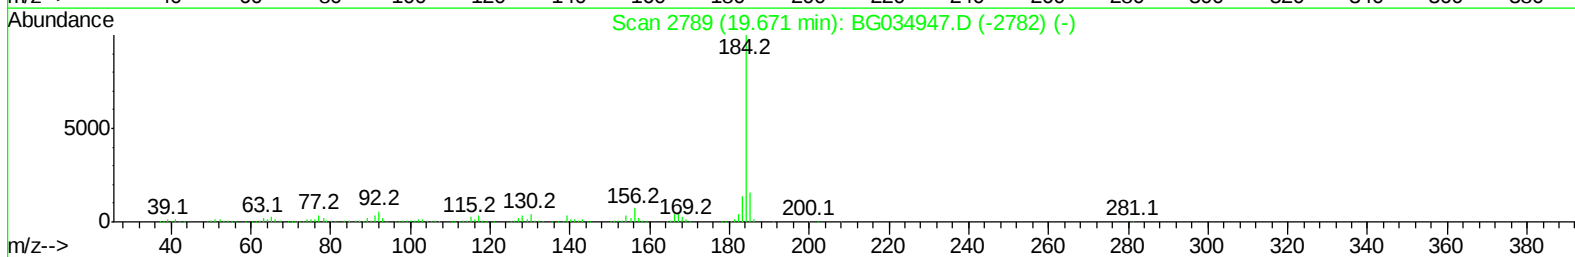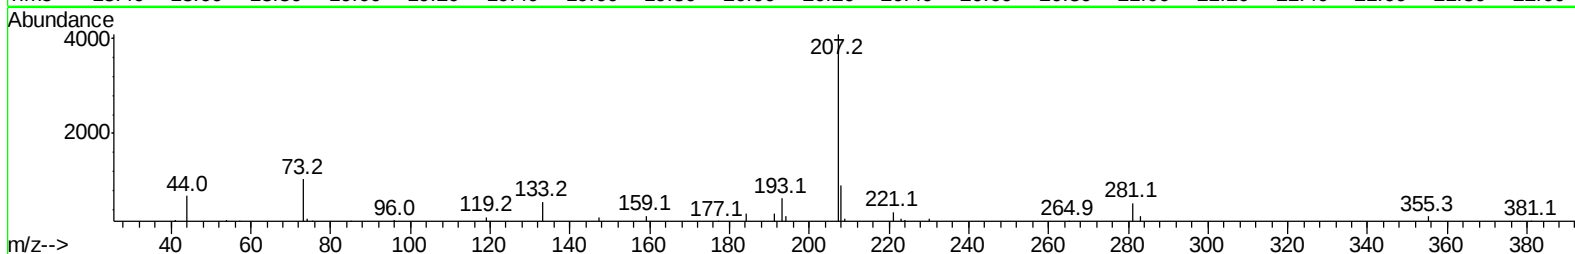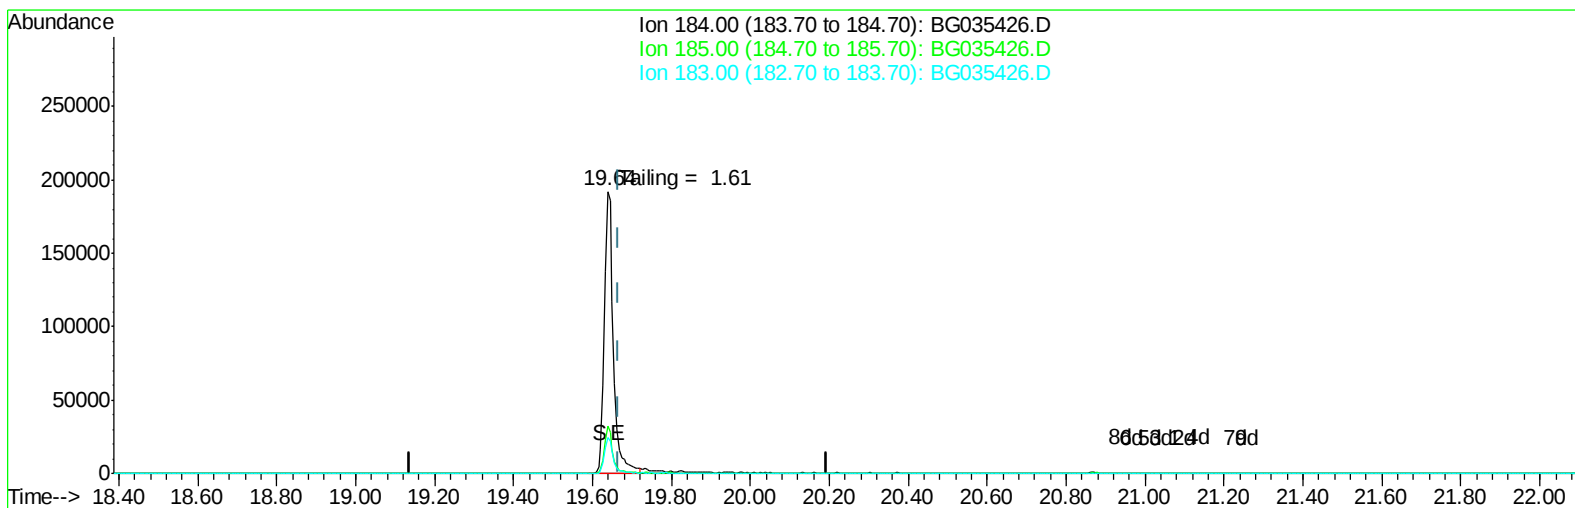

TIC: BG035426.D

(76) Benzidine

21.077min (+1.411) 73.52ng

response 186

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00