

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
 Data File : BG035423.D
 Acq On : 26 Jun 2018 23:26
 Operator : JU/SJ
 Sample : J3694-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PZ-8

Quant Time: Jun 27 03:17:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	49720	20.00	ng	-0.02
21) Naphthalene-d8	10.85	136	188497	20.00	ng	-0.03
38) Acenaphthene-d10	14.67	164	140927	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	347287	20.00	ng	-0.02
75) Chrysene-d12	21.68	240	374629	20.00	ng	-0.04
86) Perylene-d12	24.90	264	368970	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	224818	76.31	ng	-0.02
7) Phenol-d6	7.21	99	213398	49.08	ng	-0.02
23) Nitrobenzene-d5	9.21	82	443448	111.83	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	314956	174.58	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	936221	86.36	ng	-0.03
78) Terphenyl-d14	20.02	244	1721837	96.27	ng	-0.02
Target Compounds						
49) Dimethylphthalate	14.12	163	39276	3.196	ng	Qvalue # 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
Data File : BG035423.D
Acq On : 26 Jun 2018 23:26
Operator : JU/SJ
Sample : J3694-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PZ-8

Quant Time: Jun 27 03:17:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

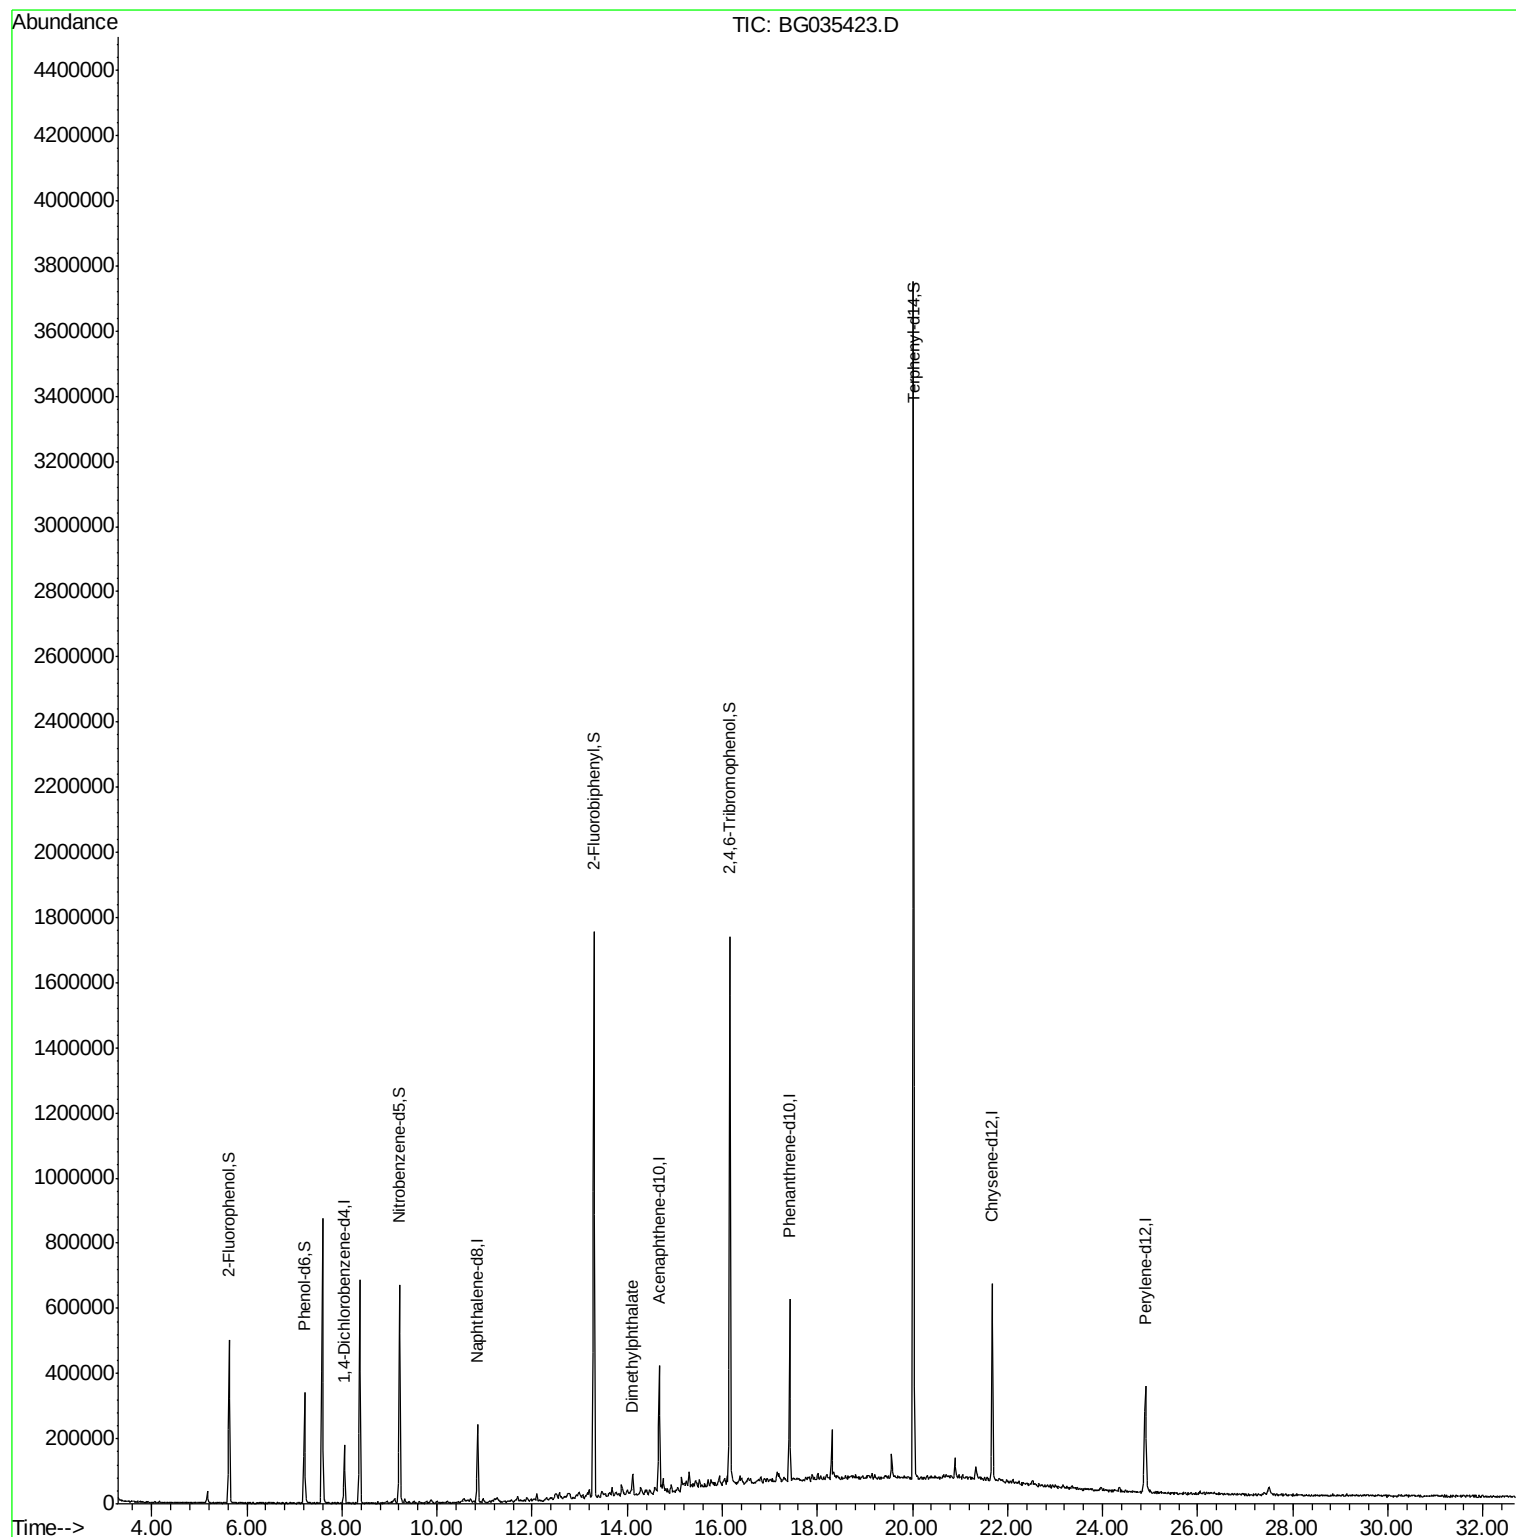

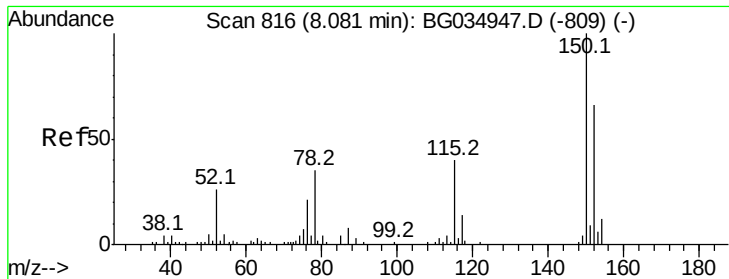


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 811
Delta R.T. -0.02 min
Lab File: BG035423.D
Acq: 26 Jun 2018 23:26

Instrument :
BNA_G
ClientSampleId :
PZ-8

Tot Ion:152 Resp: 49720
Ion Ratio Lower Upper
152 100
150 145.4 126.6 189.8
115 55.4 53.0 79.4

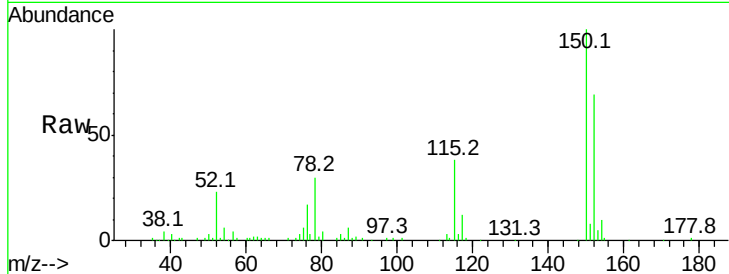


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

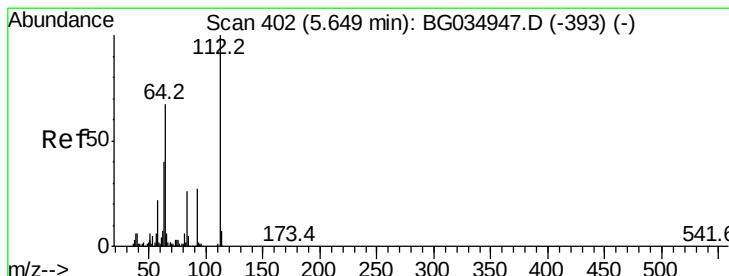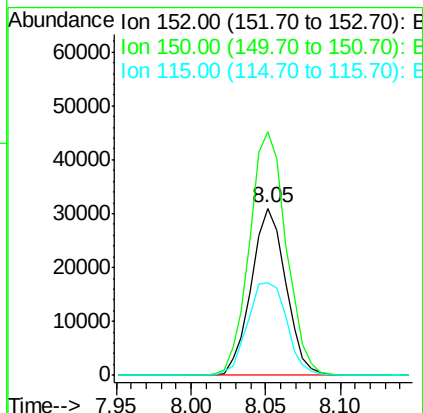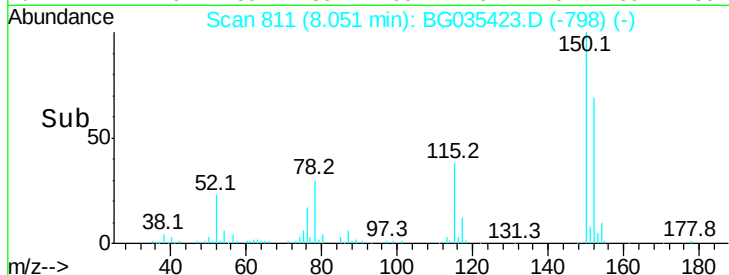



#5


2-Fluorophenol
Concen: 76.308 ng
RT: 5.63 min Scan# 398
Delta R.T. -0.02 min
Lab File: BG035423.D
Acq: 26 Jun 2018 23:26

Tgt Ion:112 Resp: 224818
Ion Ratio Lower Upper
112 100
64 66.0 56.3 84.5
63 36.3 30.1 45.1

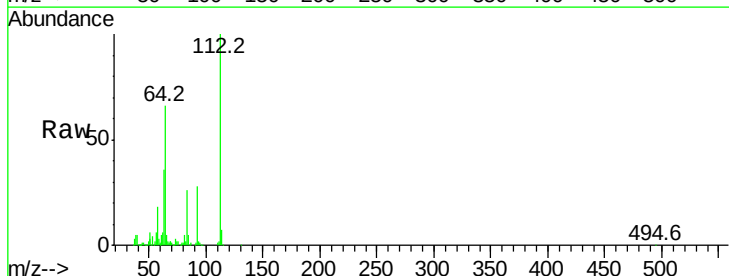

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

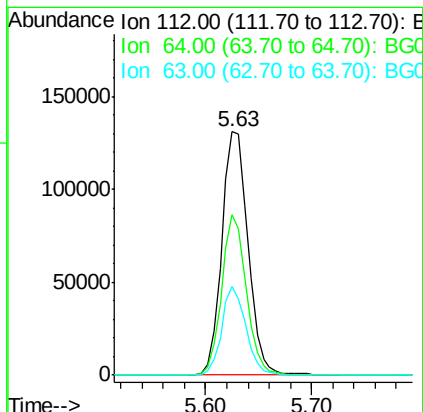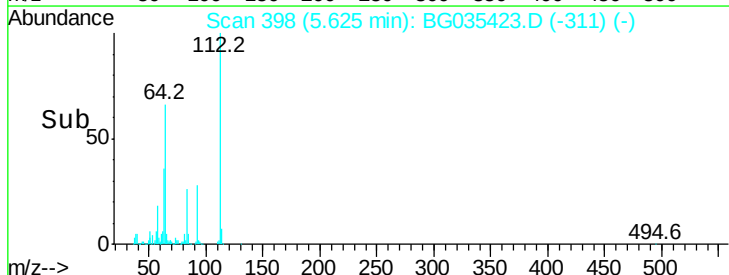

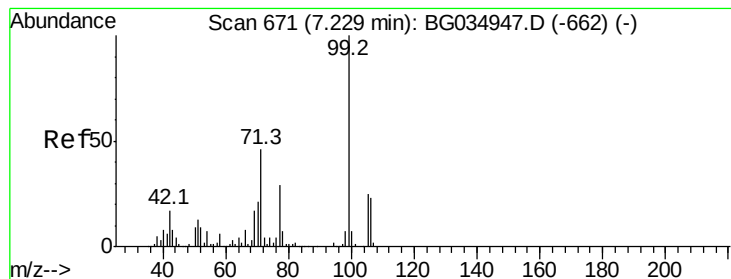

#7

Phenol-d6

Concen: 49.075 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.02 min

Lab File: BG035423.D

Acq: 26 Jun 2018 23:26

Instrument :

BNA_G

ClientSampleId :

PZ-8


Tot Ion: 99 Resp: 213398

Ion Ratio Lower Upper




99 100

42 14.3 14.1 21.1

71 41.6 26.1 39.1#

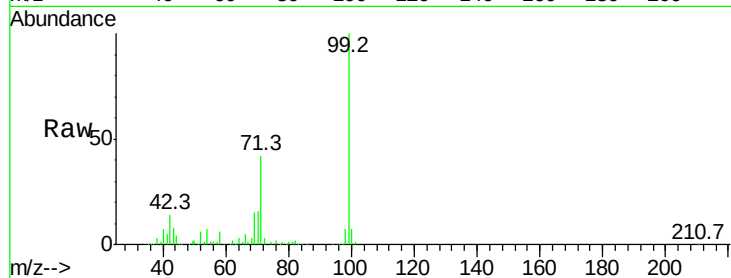

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

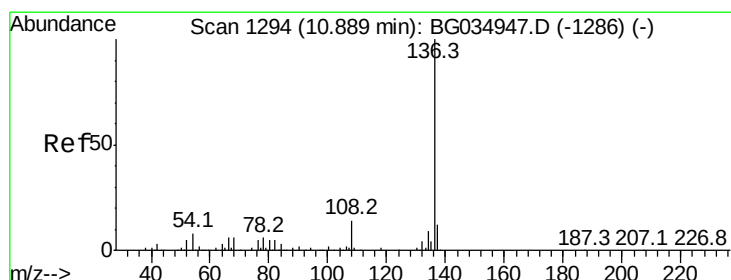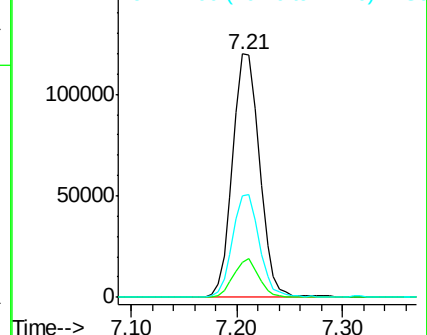

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1288

Delta R.T. -0.03 min

Lab File: BG035423.D

Acq: 26 Jun 2018 23:26

Tgt Ion: 136 Resp: 188497


Ion Ratio Lower Upper

136 100



137 12.6 9.2 13.8


54 8.0 10.3 15.5#

68 5.6 4.5 6.7

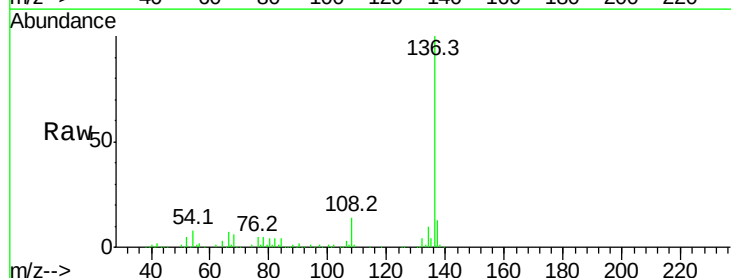

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




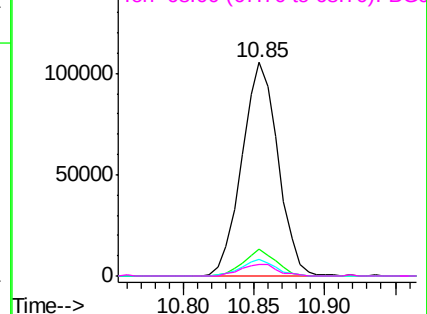




#23
 Nitrobenzene-d5
 Concen: 111.827 ng
 RT: 9.21 min Scan# 1009
 Delta R.T. -0.02 min
 Lab File: BG035423.D
 Acq: 26 Jun 2018 23:26




Instrument :
 BNA_G
 ClientSampleId :
 PZ-8


Tot Ion	Ratio	Lower	Upper
82	100		
128	35.9	29.7	44.5
54	42.8	43.1	64.7#

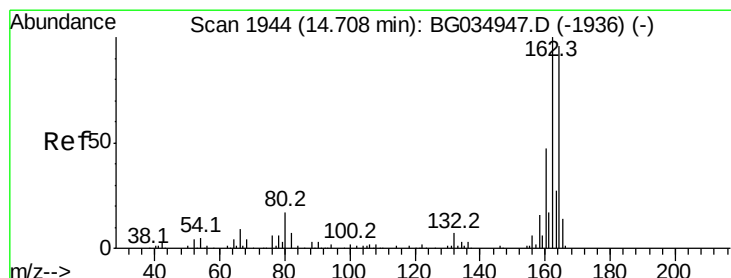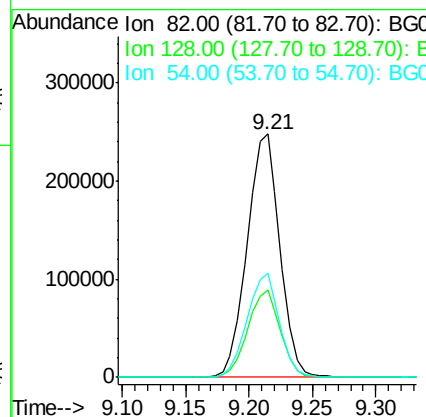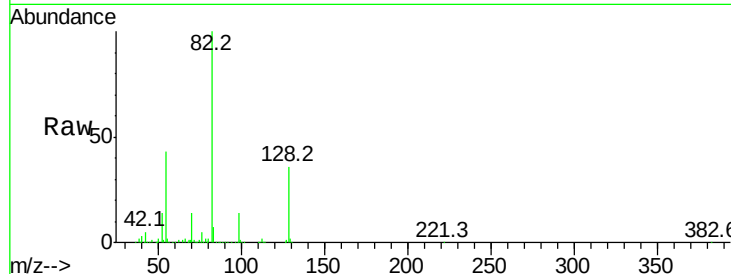

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.67 min Scan# 1938
 Delta R.T. -0.02 min
 Lab File: BG035423.D
 Acq: 26 Jun 2018 23:26

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.8	78.8	118.2
160	46.0	35.4	53.0

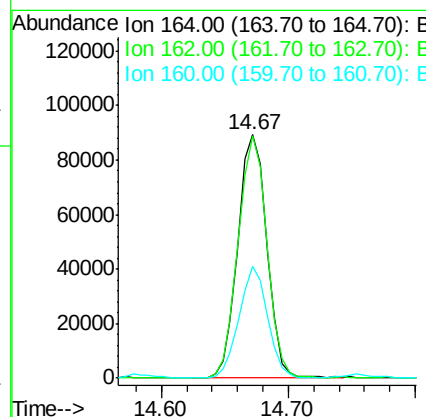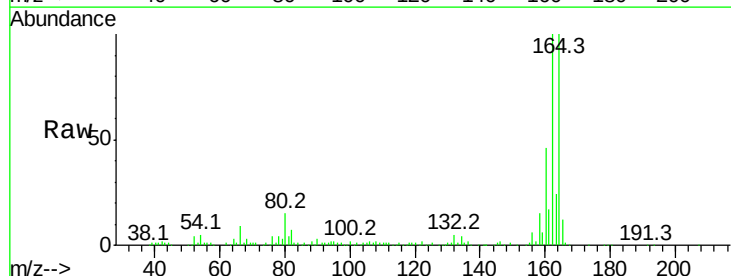







#41
 2,4,6-Tribromophenol
 Concen: 174.583 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.02 min
 Lab File: BG035423.D
 Acq: 26 Jun 2018 23:26

Instrument :
 BNA_G
 ClientSampled :
 PZ-8

Tot Ion:330 Resp: 314956
 Ion Ratio Lower Upper
 330 100
 332 93.6 77.0 115.6
 141 38.8 25.2 37.8#

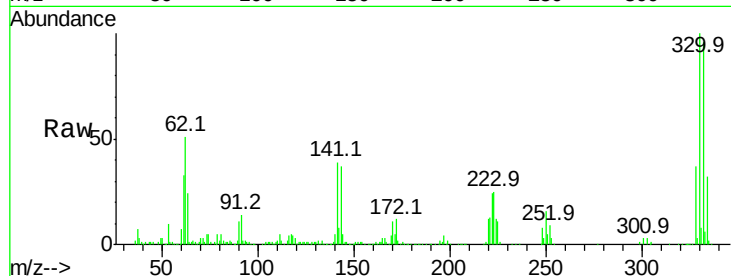


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

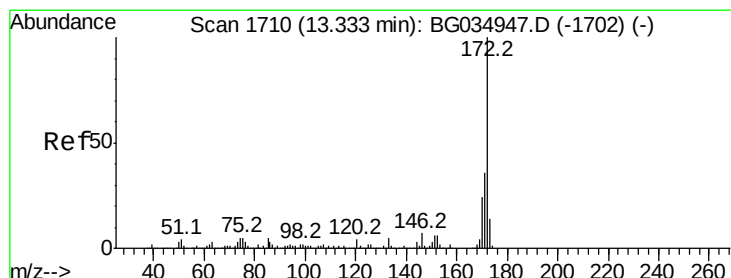
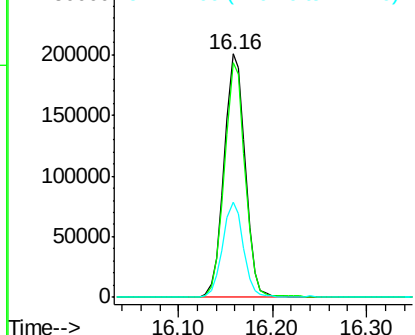



#44
 2-Fluorobiphenyl
 Concen: 86.363 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.03 min
 Lab File: BG035423.D
 Acq: 26 Jun 2018 23:26

Tgt Ion:172 Resp: 936221
 Ion Ratio Lower Upper
 172 100
 171 34.4 30.0 45.0
 170 24.1 19.5 29.3

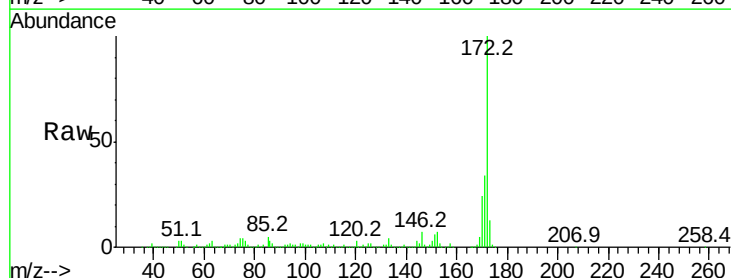

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




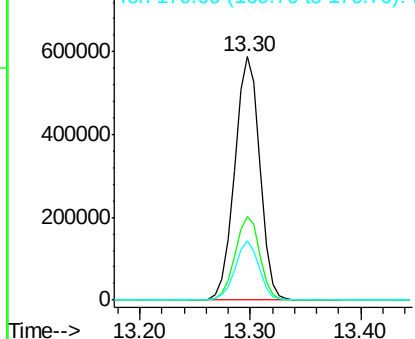




#49
Dimethylphthalate
Concen: 3.196 ng
RT: 14.12 min Scan# 1844
Delta R.T. -0.04 min
Lab File: BG035423.D
Acq: 26 Jun 2018 23:26




Instrument :
BNA_G
ClientSampleId :
PZ-8


Tot Ion:163 Resp: 39276
Ion Ratio Lower Upper
163 100
194 6.5 3.4 5.2#
164 10.3 8.2 12.4

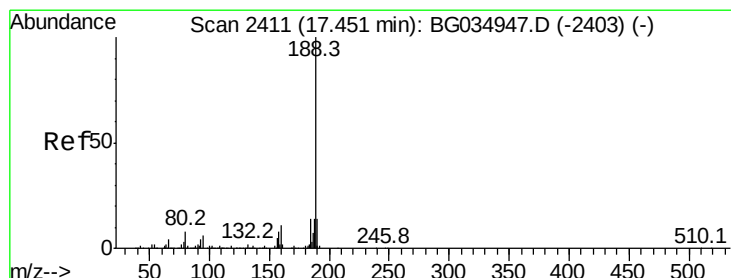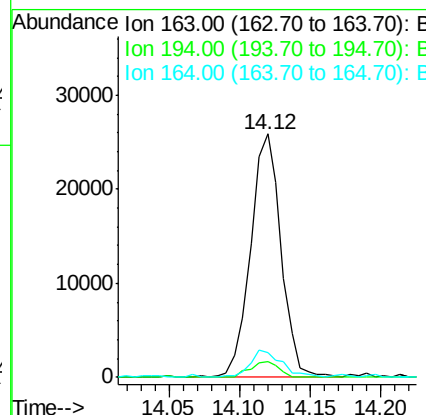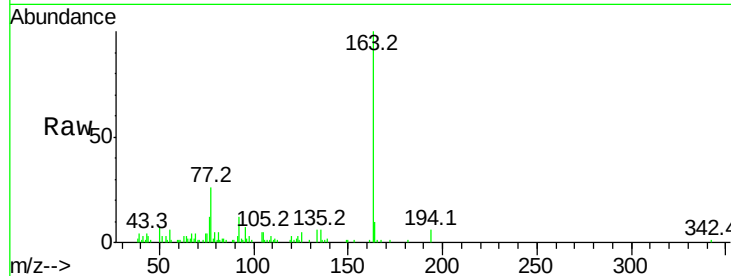

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2405
Delta R.T. -0.02 min
Lab File: BG035423.D
Acq: 26 Jun 2018 23:26

Tgt Ion:188 Resp: 347287
Ion Ratio Lower Upper
188 100
94 5.5 6.9 10.3#
80 6.9 7.7 11.5#

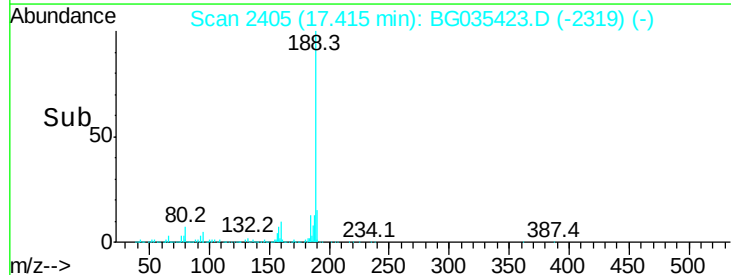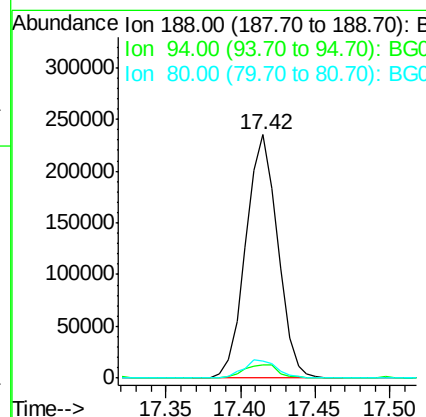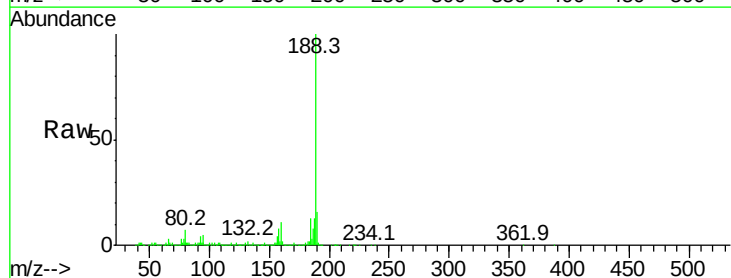

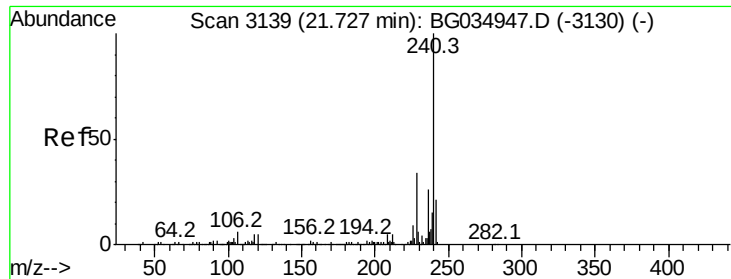

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3131

Delta R.T. -0.04 min

Lab File: BG035423.D

Acq: 26 Jun 2018 23:26

Instrument :

BNA_G

ClientSampleId :

PZ-8


Tot Ion:240 Resp: 374629

Ion Ratio Lower Upper

240 100

120 5.5 6.8 10.2#




236 27.0 20.9 31.3

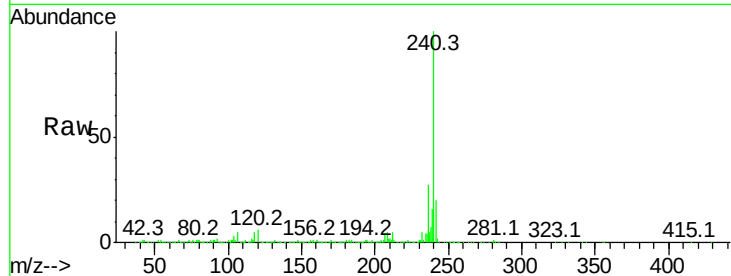

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

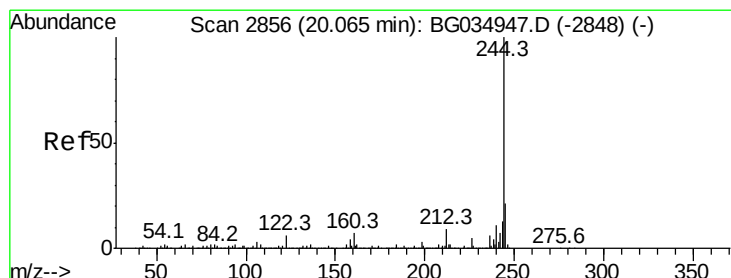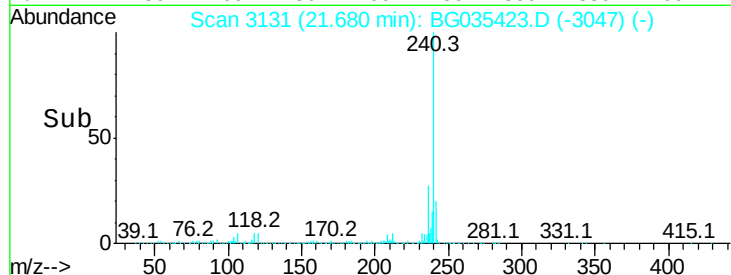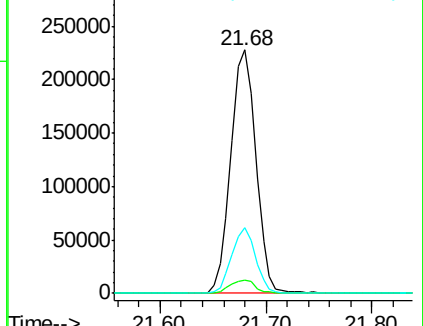

#78

Terphenyl-d14

Concen: 96.274 ng

RT: 20.02 min Scan# 2849

Delta R.T. -0.02 min

Lab File: BG035423.D

Acq: 26 Jun 2018 23:26


Tgt Ion:244 Resp: 1721837

Ion Ratio Lower Upper

244 100

212 9.4 5.8 8.8#



122 7.2 7.0 10.4

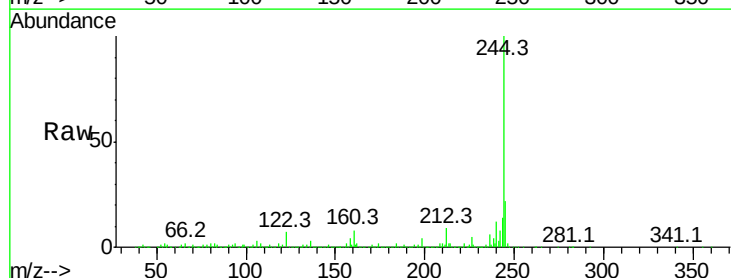


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

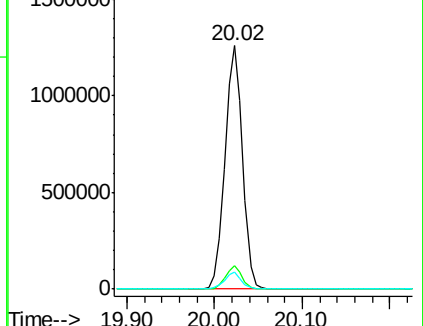


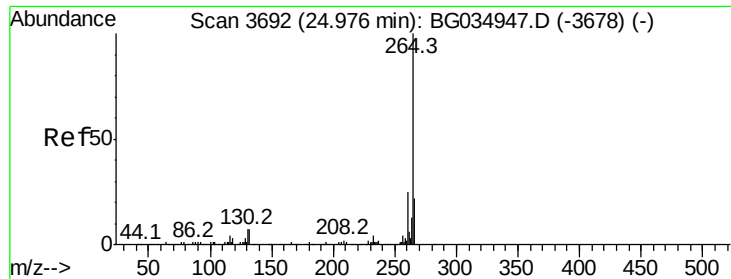

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.90 min Scan# 3679
Delta R.T. -0.05 min
Lab File: BG035423.D
Acq: 26 Jun 2018 23:26

Instrument :
BNA_G
ClientSampleId :
PZ-8

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	17.4	26.0
265	21.9	17.7	26.5

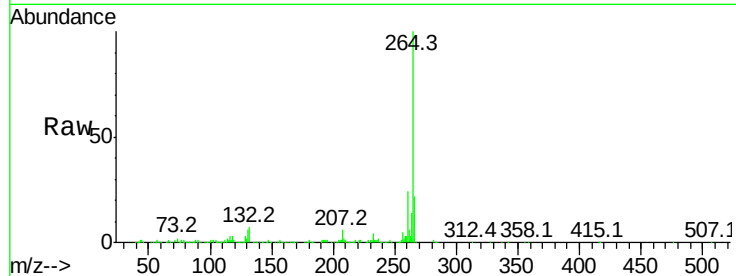

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

