

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
 Data File : BG035442.D
 Acq On : 27 Jun 2018 12:23
 Operator : JU/SJ
 Sample : J3570-12
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20180375-COMPOSITE-CS-1A-ELU

Quant Time: Jun 27 15:53:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	48631	20.00	ng	-0.03
21) Naphthalene-d8	10.85	136	187878	20.00	ng	-0.03
38) Acenaphthene-d10	14.67	164	135541	20.00	ng	-0.02
63) Phenanthrene-d10	17.41	188	349894	20.00	ng	-0.03
75) Chrysene-d12	21.68	240	371392	20.00	ng	-0.04
86) Perylene-d12	24.89	264	368401	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	188223	65.32	ng	-0.02
7) Phenol-d6	7.21	99	214867	50.52	ng	-0.01
23) Nitrobenzene-d5	9.21	82	361346	91.42	ng	-0.03
41) 2,4,6-Tribromophenol	16.16	330	243873	140.55	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	826206	79.24	ng	-0.03
78) Terphenyl-d14	20.02	244	1345554	75.89	ng	-0.02
Target Compounds						
10) Phenol	7.24	94	15625	3.550	ng	97
49) Dimethylphthalate	14.12	163	216572	18.323	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062618\
Data File : BG035442.D
Acq On : 27 Jun 2018 12:23
Operator : JU/SJ
Sample : J3570-12
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20180375-COMPOSITE-CS-1A-ELU

Quant Time: Jun 27 15:53:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

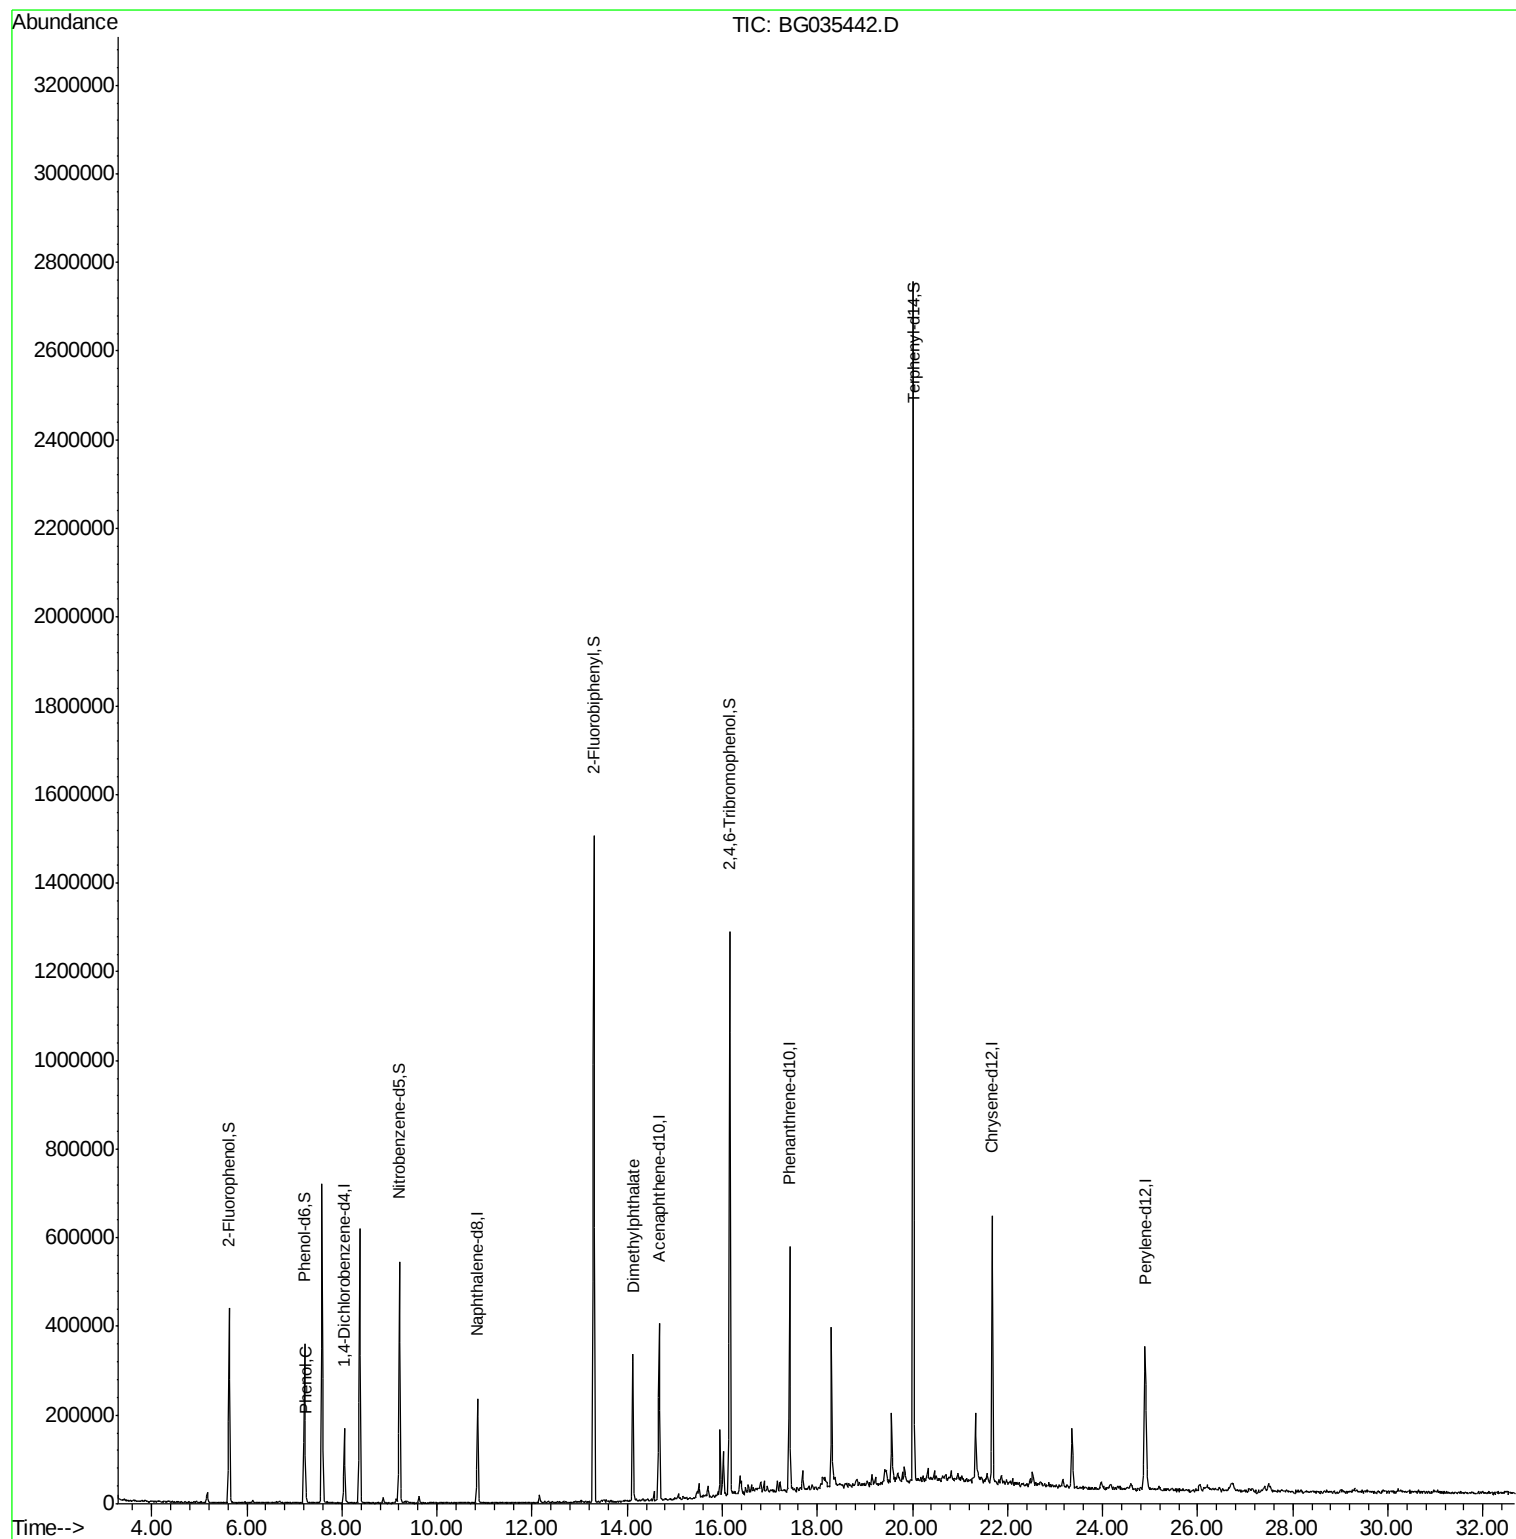

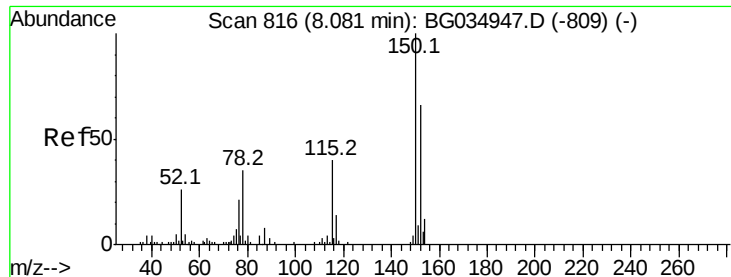

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.05 min Scan# 810

Delta R.T. -0.03 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23

Instrument :

BNA_G

ClientSampleId :

20180375-COMPOSITE-CS-1A-ELU


Tot Ion:152 Resp: 48631

Ion Ratio Lower Upper

152 100

150 151.4 126.6 189.8




115 63.1 53.0 79.4

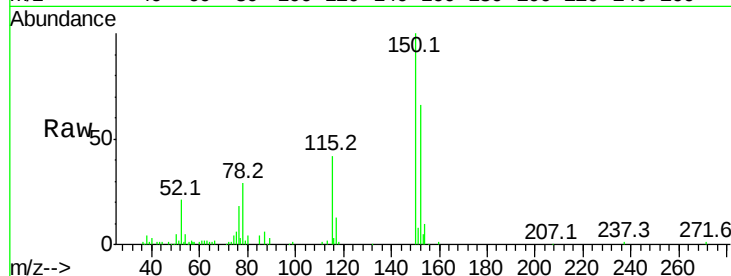

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

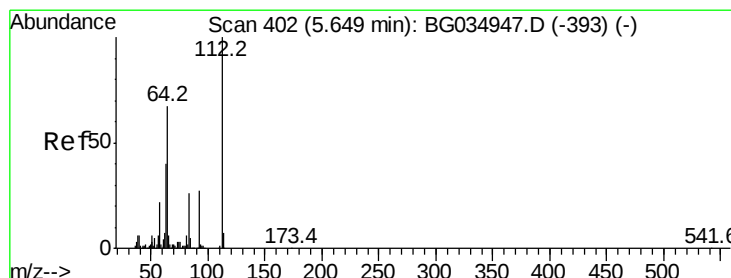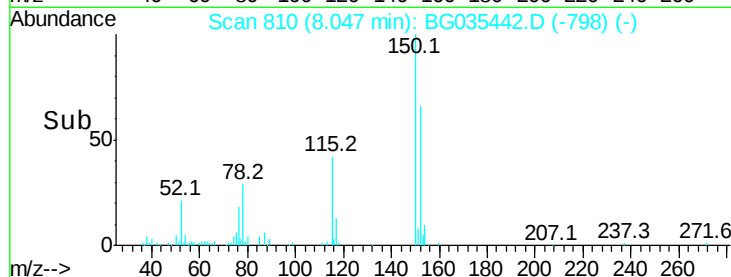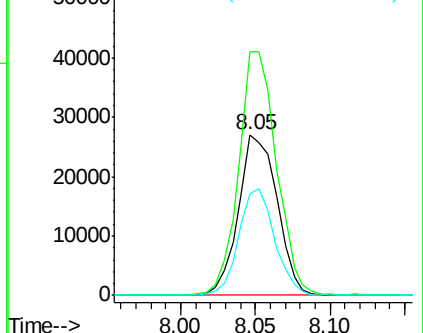

#5

2-Fluorophenol

Concen: 65.318 ng

RT: 5.63 min Scan# 398

Delta R.T. -0.02 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23


Tgt Ion:112 Resp: 188223

Ion Ratio Lower Upper

112 100

64 66.2 56.3 84.5



63 35.0 30.1 45.1

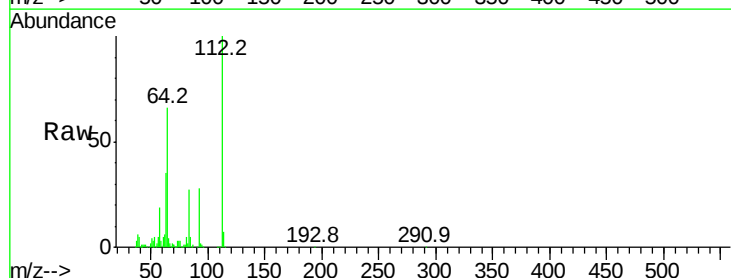


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

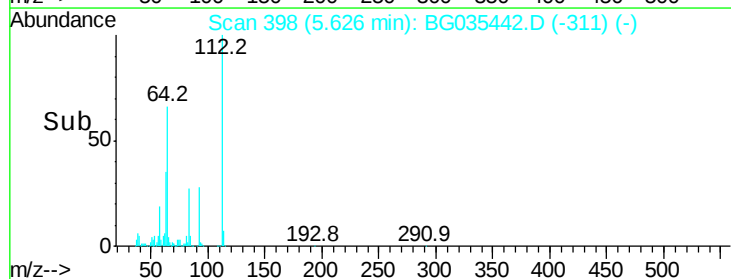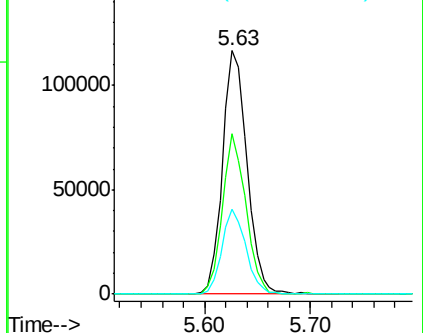

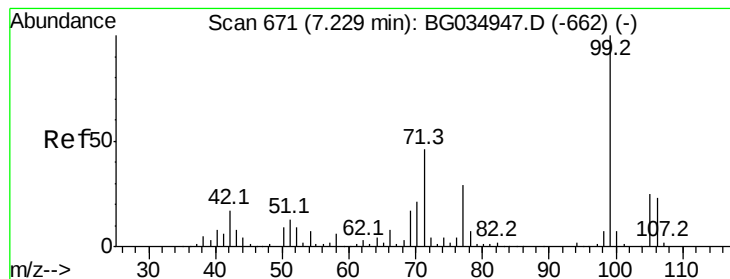

#7

Phenol-d6

Concen: 50.520 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23

Instrument :

BNA_G

ClientSampleId :

20180375-COMPOSITE-CS-1A-ELU


Tot Ion: 99 Resp: 214867

Ion Ratio Lower Upper




99 100

42 15.9 14.1 21.1

71 42.7 26.1 39.1#

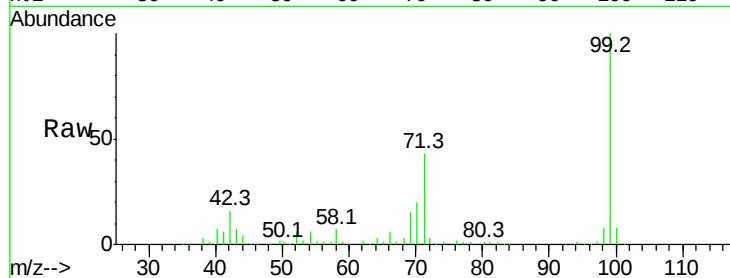

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

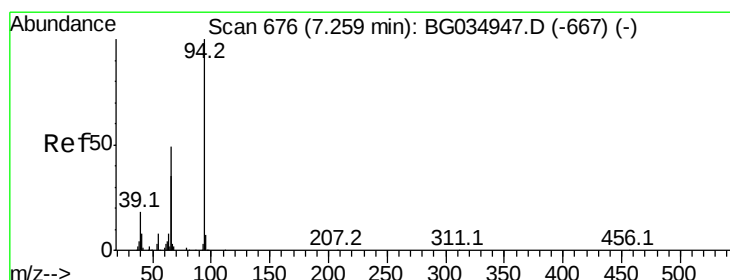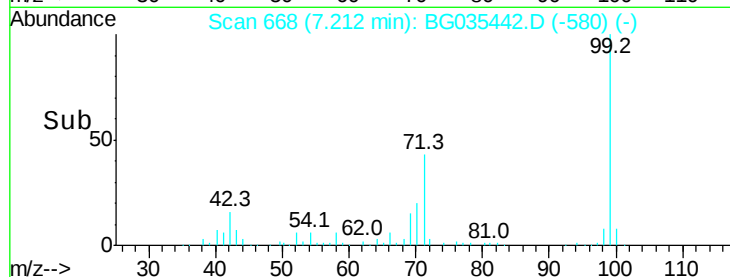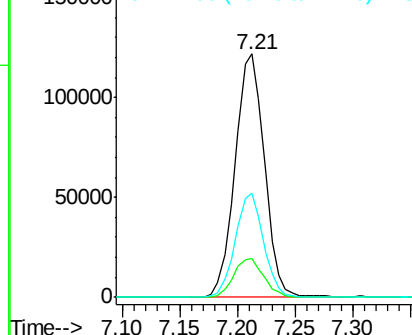

#10

Phenol

Concen: 3.550 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23


Tgt Ion: 94 Resp: 15625

Ion Ratio Lower Upper



94 100


65 29.4 11.9 51.9

66 40.6 22.2 62.2

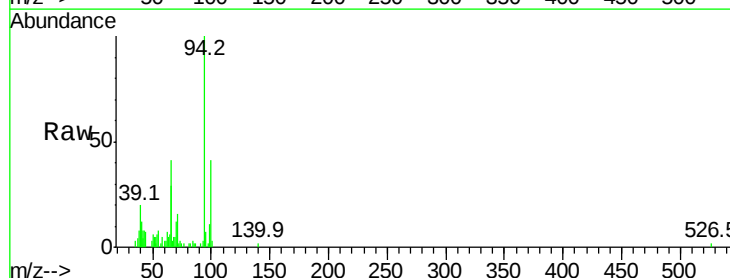

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

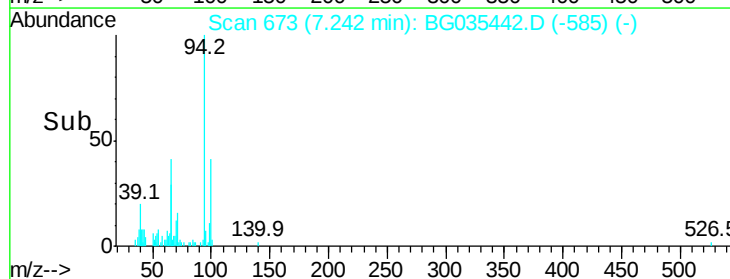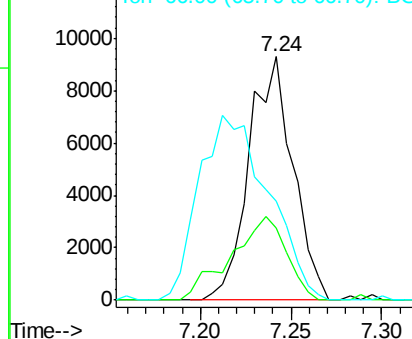


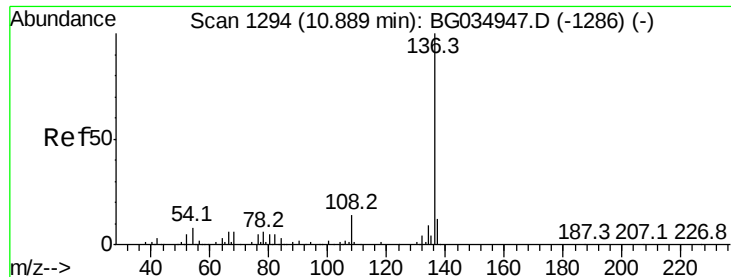




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.85 min Scan# 1288
Delta R.T. -0.03 min
Lab File: BG035442.D
Acq: 27 Jun 2018 12:23

Instrument :
BNA_G
ClientSampleId :
20180375-COMPOSITE-CS-1A-ELU

Tot Ion:	136	Resp:	187878
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.2	13.8
54	7.1	10.3	15.5
68	4.7	4.5	6.7

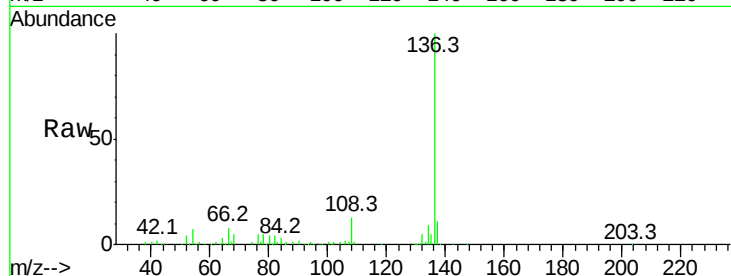


Abundance Ion 136.00 (135.70 to 136.70): B
Ion 137.00 (136.70 to 137.70): B
Ion 54.00 (53.70 to 54.70): B
Ion 68.00 (67.70 to 68.70): B

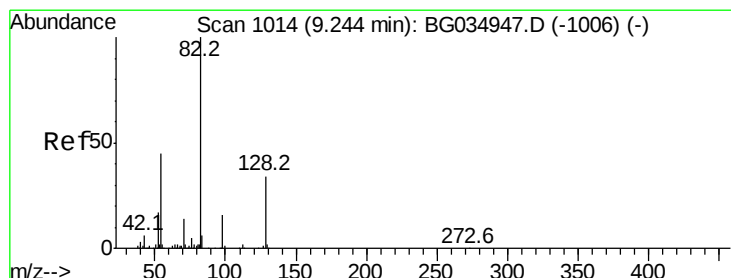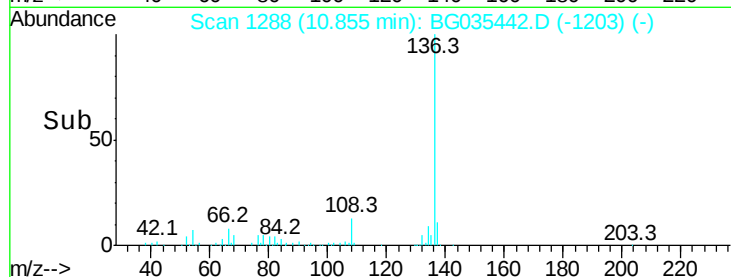
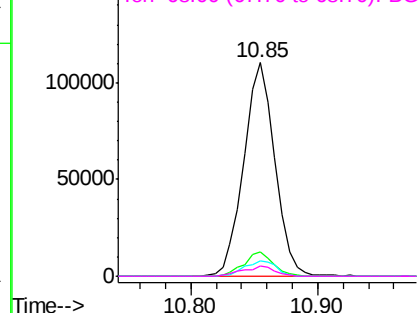



#23
Nitrobenzene-d5
Concen: 91.423 ng
RT: 9.21 min Scan# 1008
Delta R.T. -0.03 min
Lab File: BG035442.D
Acq: 27 Jun 2018 12:23

Tgt Ion:	82	Resp:	361346
Ion	Ratio	Lower	Upper
82	100		
128	36.1	29.7	44.5
54	41.5	43.1	64.7

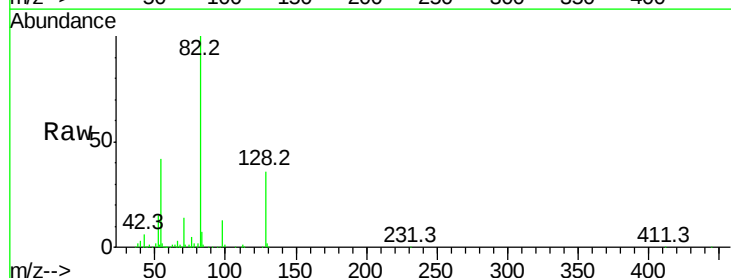

Abundance Ion 82.00 (81.70 to 82.70): B
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): B

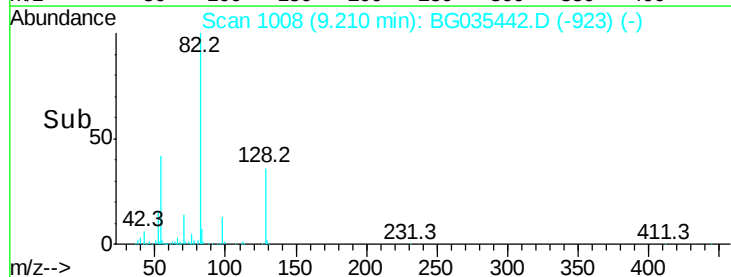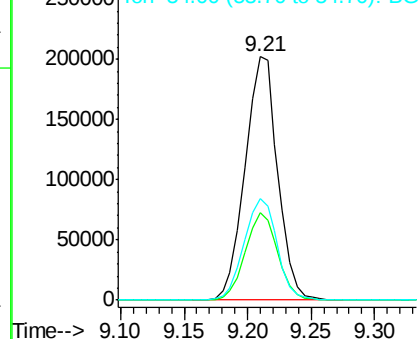

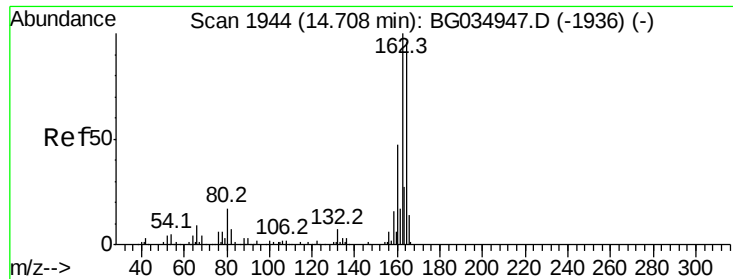

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1938

Delta R.T. -0.02 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23

Instrument :

BNA_G

ClientSampleId :

20180375-COMPOSITE-CS-1A-ELU


Tot Ion:164 Resp: 135541

Ion Ratio Lower Upper

164 100

162 102.6 78.8 118.2




160 44.6 35.4 53.0

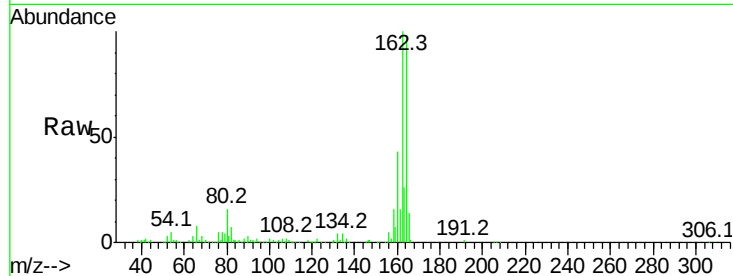

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

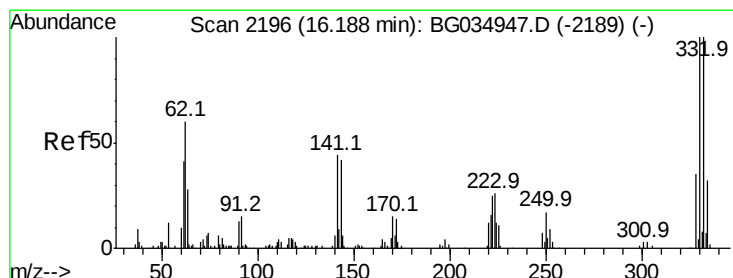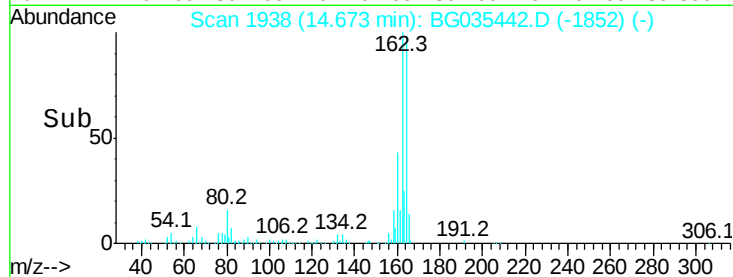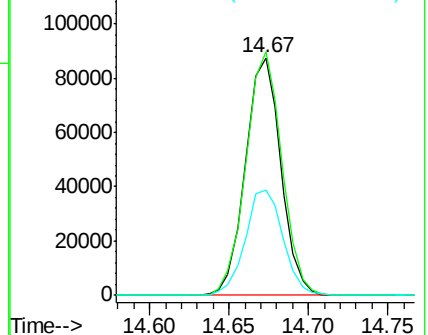

#41

2,4,6-Tribromophenol

Concen: 140.553 ng

RT: 16.16 min Scan# 2191

Delta R.T. -0.02 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23


Tgt Ion:330 Resp: 243873

Ion Ratio Lower Upper

330 100

332 96.5 77.0 115.6



141 37.7 25.2 37.8

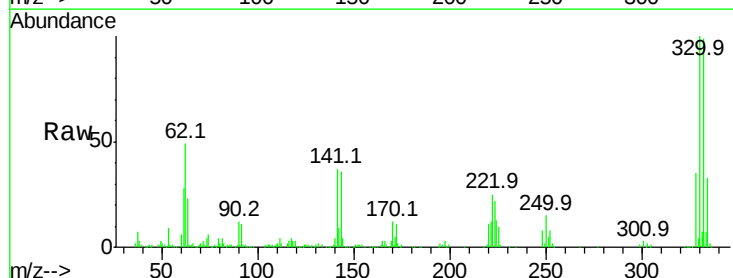


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



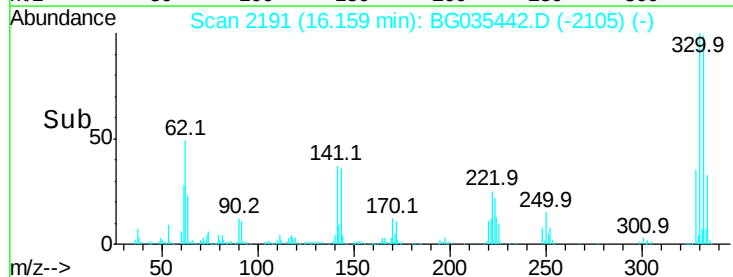
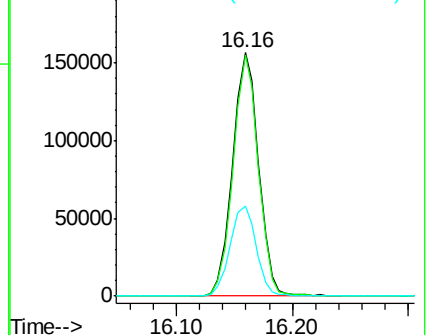


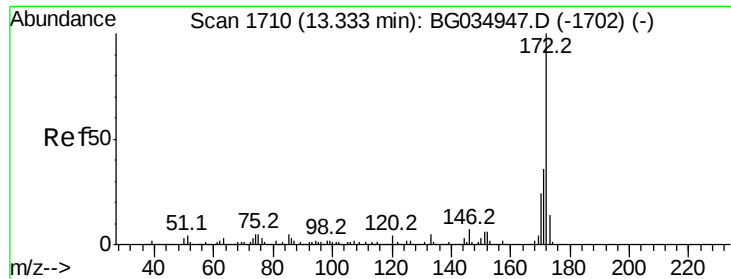

#44
2-Fluorobiphenyl
Concen: 79.243 ng
RT: 13.30 min Scan# 1704
Delta R.T. -0.03 min
Lab File: BG035442.D
Acq: 27 Jun 2018 12:23




Instrument :
BNA_G
ClientSampleId :
20180375-COMPOSITE-CS-1A-ELU


Tot Ion:172 Resp: 826206
Ion Ratio Lower Upper
172 100
171 33.8 30.0 45.0
170 23.8 19.5 29.3

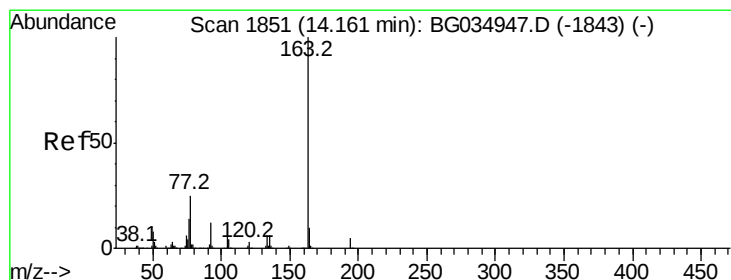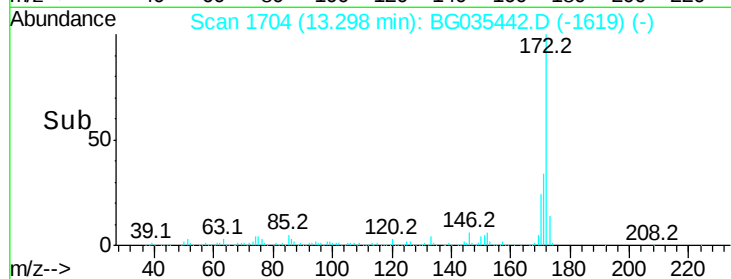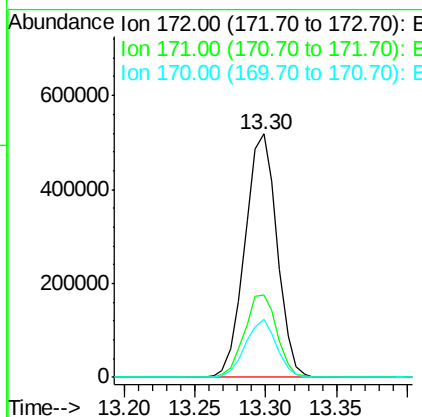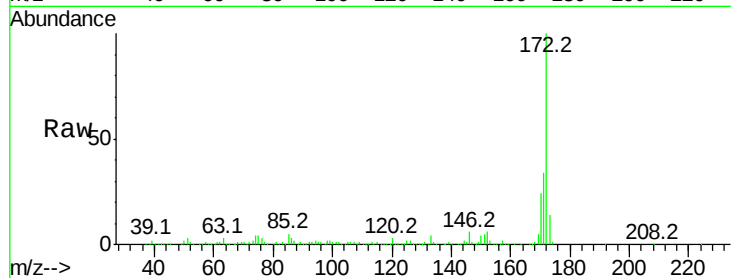

#49
Dimethylphthalate
Concen: 18.323 ng
RT: 14.12 min Scan# 1844
Delta R.T. -0.04 min
Lab File: BG035442.D
Acq: 27 Jun 2018 12:23

Tgt Ion:163 Resp: 216572
Ion Ratio Lower Upper
163 100
194 5.0 3.4 5.2
164 8.7 8.2 12.4

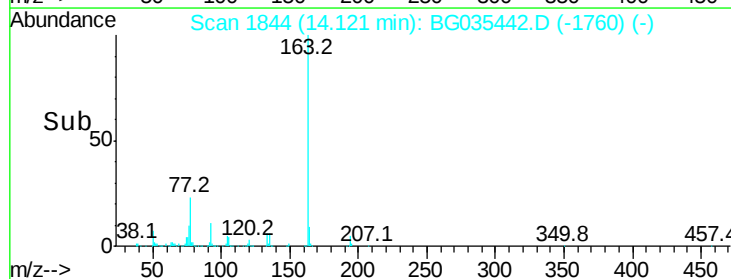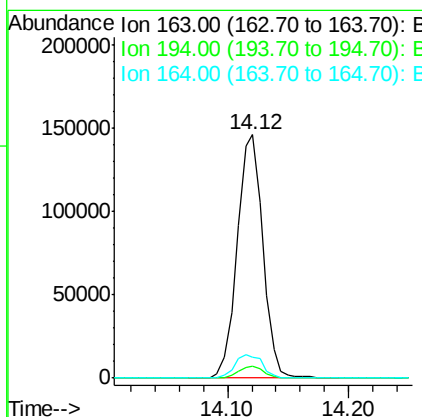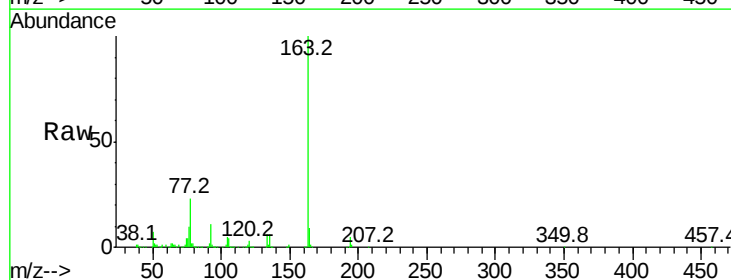

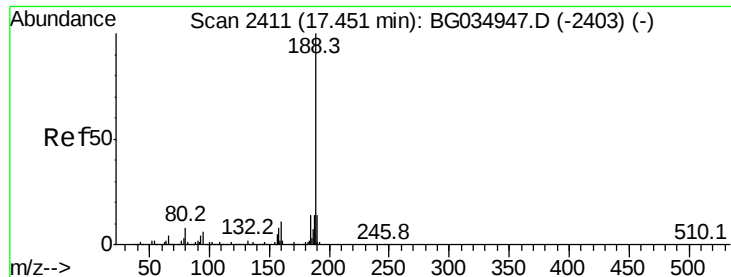

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2404

Delta R.T. -0.03 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23

Instrument :

BNA_G

ClientSampleId :

20180375-COMPOSITE-CS-1A-ELU


Tot Ion:188 Resp: 349894

Ion Ratio Lower Upper

188 100

94 5.6 6.9 10.3#




80 7.2 7.7 11.5#

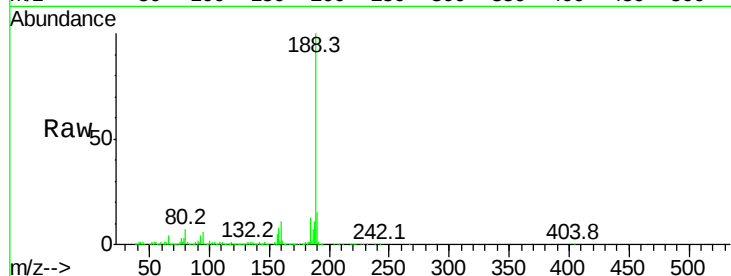

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

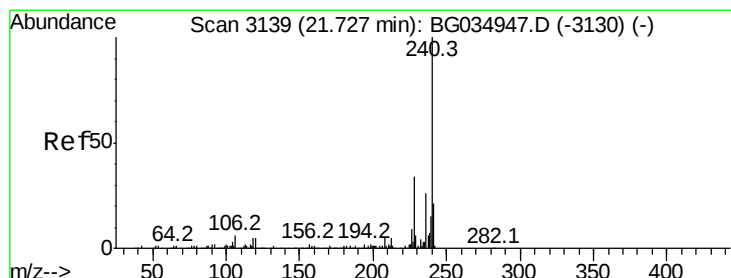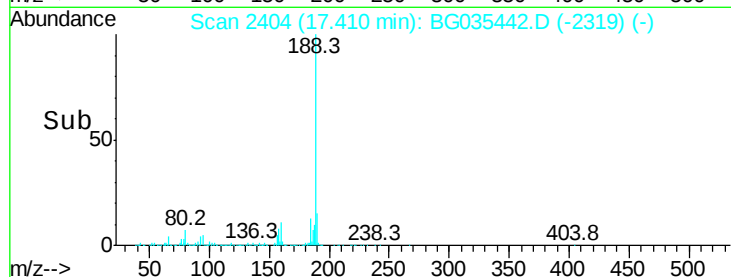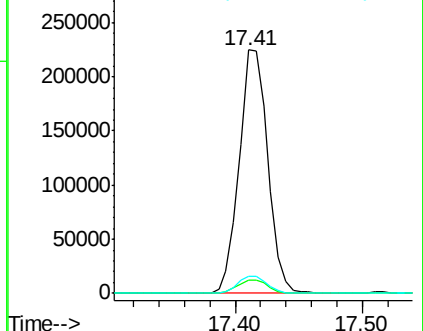

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3131

Delta R.T. -0.04 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23


Tgt Ion:240 Resp: 371392

Ion Ratio Lower Upper

240 100

120 4.8 6.8 10.2#



236 24.6 20.9 31.3

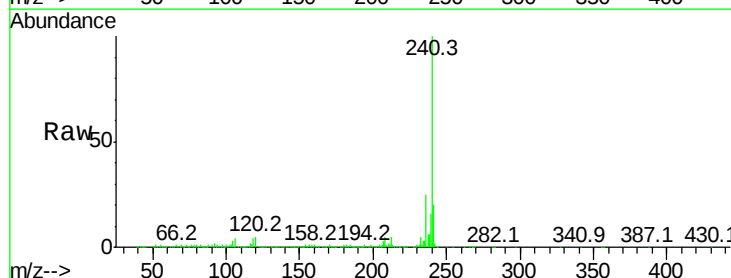


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

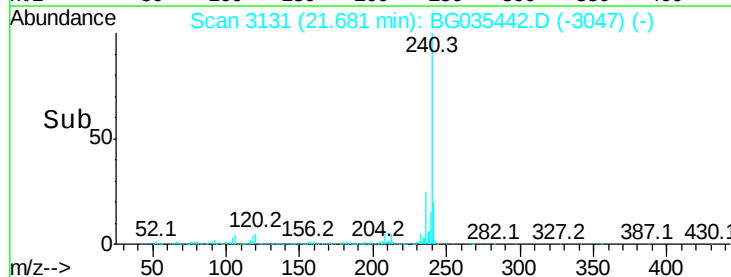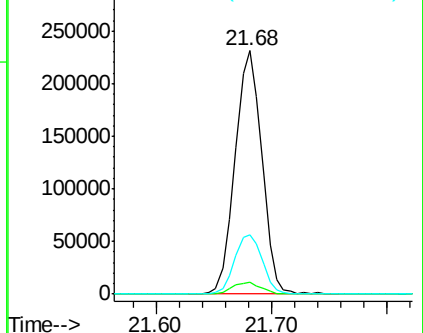

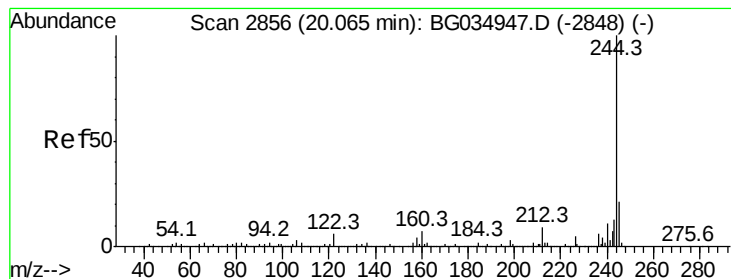

#78

Terphenyl-d14

Concen: 75.890 ng

RT: 20.02 min Scan# 2849

Delta R.T. -0.02 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23

Instrument :

BNA_G

ClientSampleId :

20180375-COMPOSITE-CS-1A-ELU


Tot Ion:244 Resp: 1345554

Ion Ratio Lower Upper

244 100

212 9.0 5.8 8.8#




122 6.1 7.0 10.4#

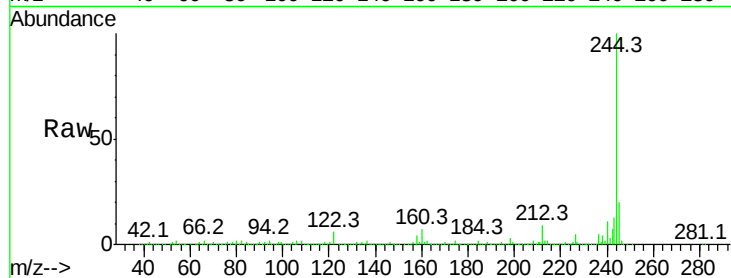

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

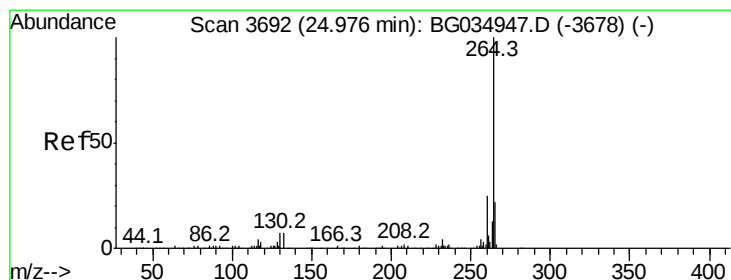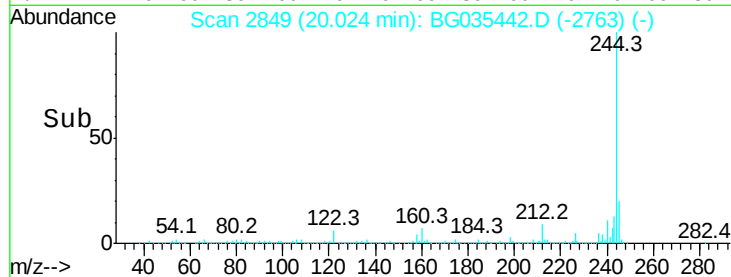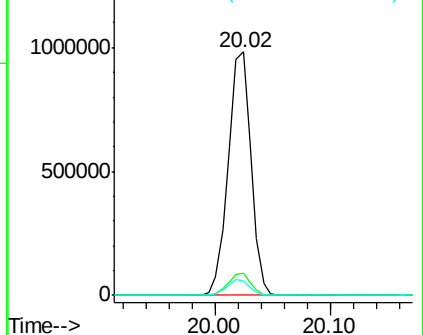

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.89 min Scan# 3678

Delta R.T. -0.06 min

Lab File: BG035442.D

Acq: 27 Jun 2018 12:23


Tgt Ion:264 Resp: 368401

Ion Ratio Lower Upper

264 100

260 21.2 17.4 26.0

265 21.9 17.7 26.5

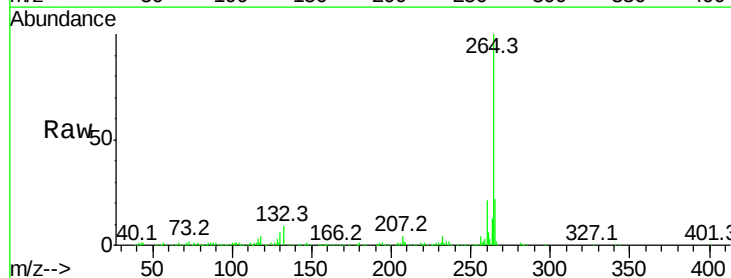

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

