


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062618\
 Data File : BG035426.D
 Acq On : 27 Jun 2018 2:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

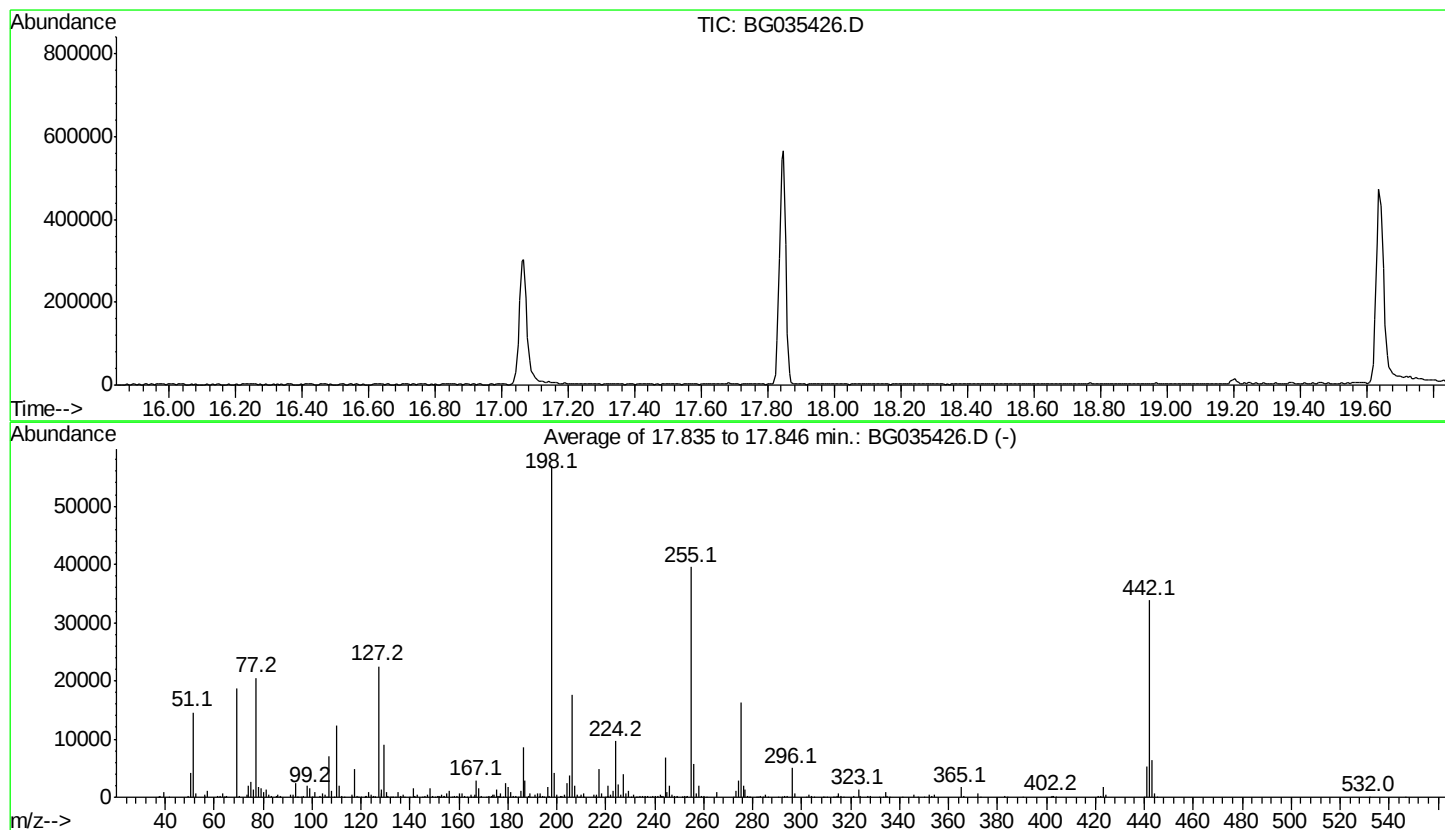

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	14571	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	18593	PASS
70	69	0.00	2	0.7	128	PASS
127	198	10	80	39.5	22485	PASS
197	198	0.00	2	0.3	162	PASS
198	198	100	100	100.0	56965	PASS
199	198	5	9	7.3	4145	PASS
275	198	10	60	28.6	16273	PASS
365	198	1	100	3.0	1705	PASS
441	443	0.01	100	83.0	5205	PASS
442	198	50	100	59.3	33797	PASS
443	442	15	24	18.6	6274	PASS