
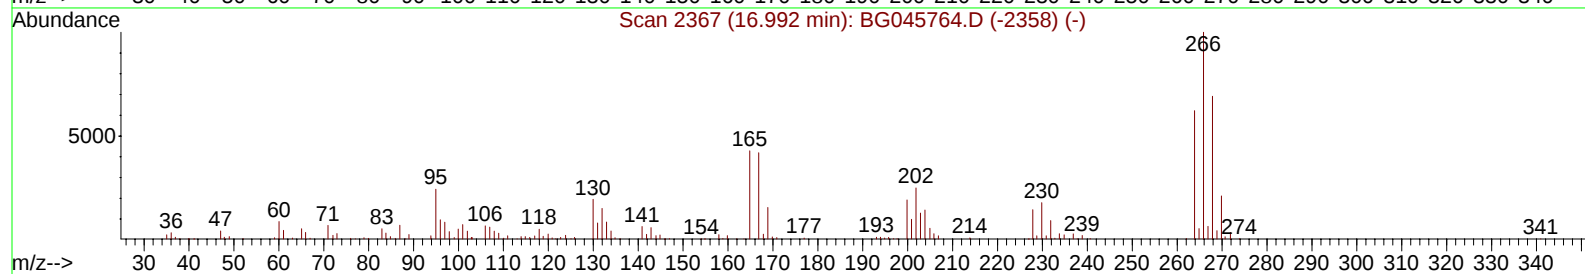
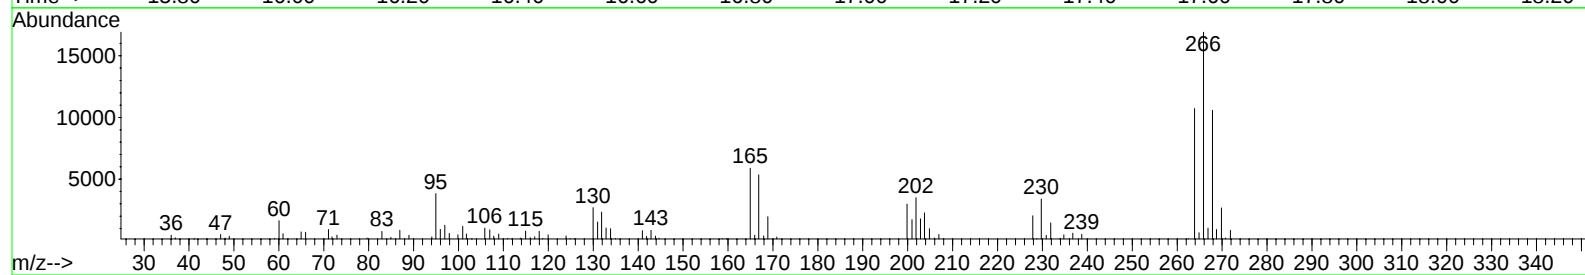


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062620\
Data File : BG045866.D
Acq On : 26 Jun 2020 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 15:46:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 25 15:44:32 2020
Response via : Initial Calibration

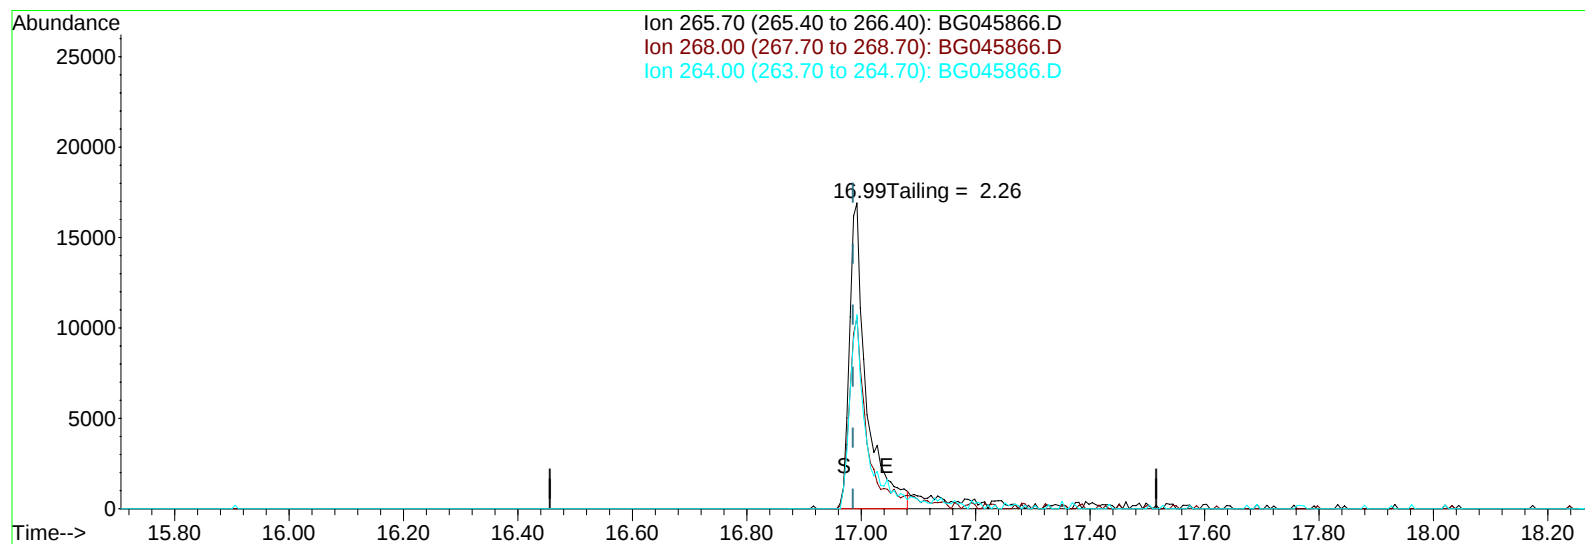

TIC: BG045866.D

(70) Pentachlorophenol (C)




16.993min (+0.007) 67968.07ng

response 35944

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	62.54
264.00	62.20	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062620\
 Data File : BG045866.D
 Acq On : 26 Jun 2020 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 15:46:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 25 15:44:32 2020
 Response via : Initial Calibration

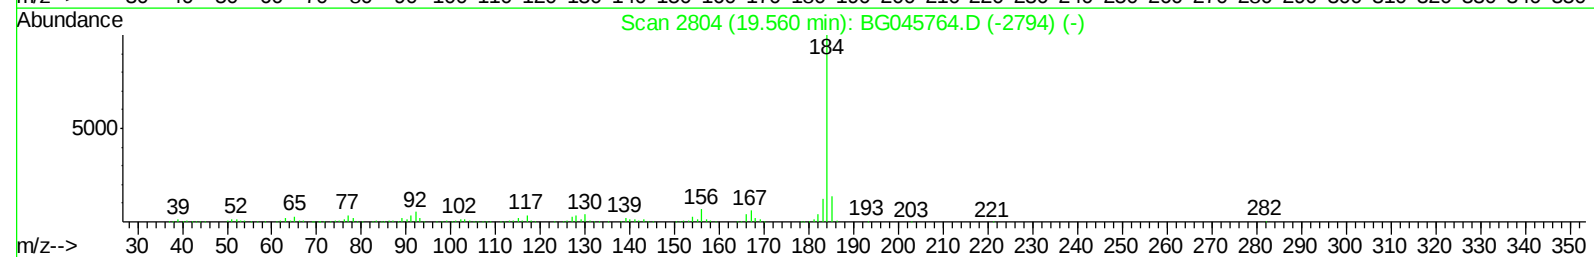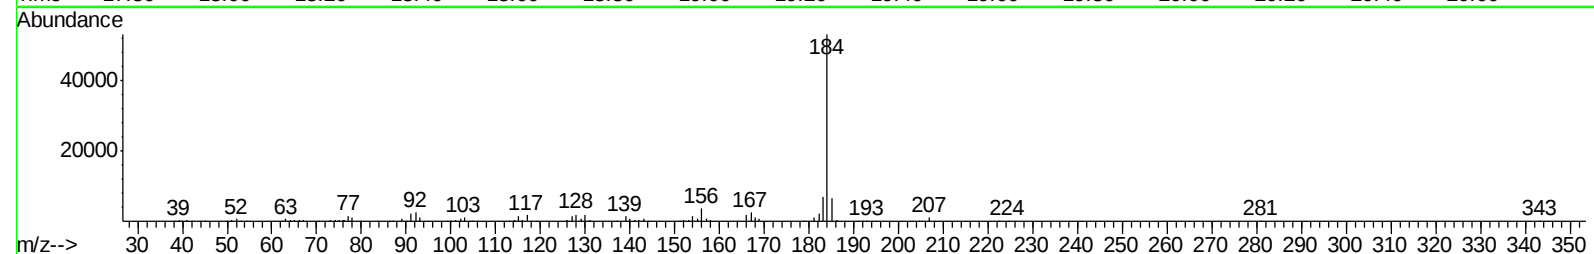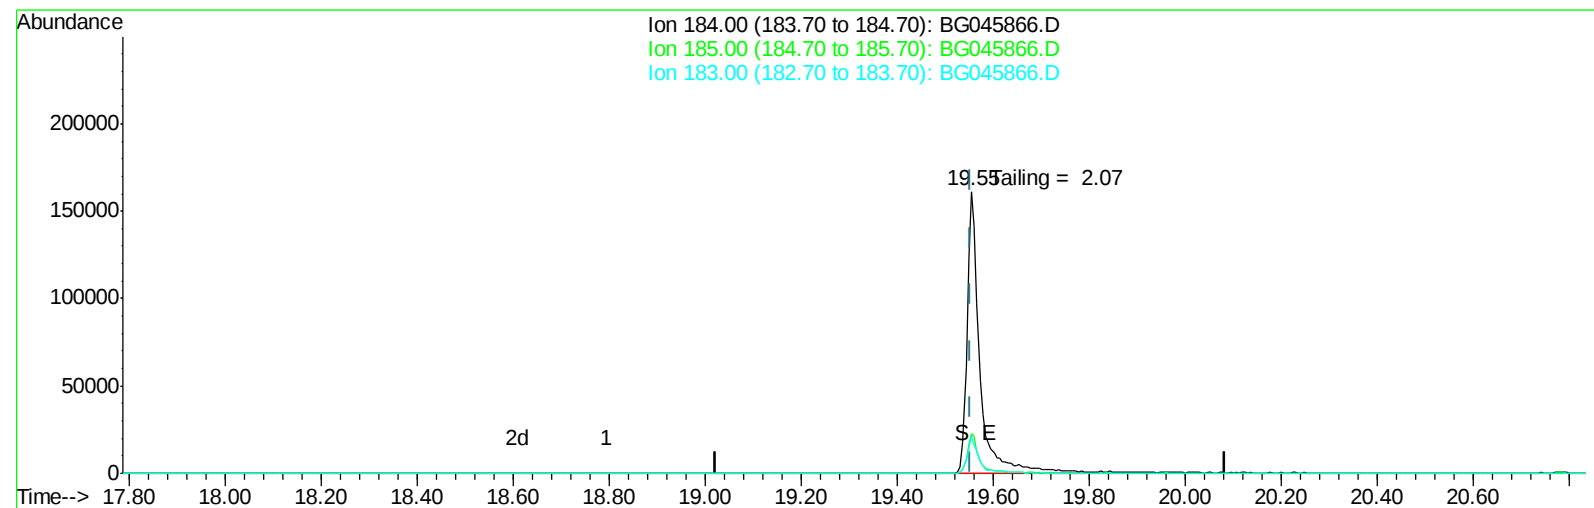

TIC: BG045866.D

(77) Benzidine

18.796min (-0.757) 0.90ng

response 63

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	12.10	0.00#
0.00	0.00	0.00