

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062620\
 Data File : BG045872.D
 Acq On : 26 Jun 2020 14:02
 Operator : CG/JU
 Sample : L3094-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BRENNAN-FL-001

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.519	404	414	430	rBV	707378	1247015	40.33%	6.096%
2	7.134	680	689	699	rBV	802643	1431395	46.30%	6.997%
3	7.916	815	822	831	rBV	222481	382469	12.37%	1.870%
4	8.239	869	877	888	rBV	689335	1199156	38.79%	5.862%
5	9.079	1010	1020	1031	rBV	509826	950588	30.75%	4.647%
6	10.718	1291	1299	1306	rBV	293933	539821	17.46%	2.639%
7	13.179	1710	1718	1730	rBV	1415768	2286385	73.95%	11.177%
8	13.467	1760	1767	1772	rVB2	55230	87900	2.84%	0.430%
9	14.013	1853	1860	1867	rBV	207923	316628	10.24%	1.548%
10	14.566	1947	1954	1961	rBV	459574	745159	24.10%	3.643%
11	15.611	2127	2132	2137	rBV3	24648	37768	1.22%	0.185%
12	16.064	2199	2209	2224	rBV	1145119	1824247	59.00%	8.918%
13	17.315	2415	2422	2426	rBV	590321	900554	29.13%	4.402%
14	17.356	2426	2429	2435	rVB	177262	249021	8.05%	1.217%
15	17.450	2440	2445	2450	rVB	27784	48116	1.56%	0.235%
16	18.190	2567	2571	2575	rBV	30675	45636	1.48%	0.223%
17	18.237	2576	2579	2584	rVB	37441	57460	1.86%	0.281%
18	18.384	2598	2604	2608	rBV4	45297	80333	2.60%	0.393%
19	18.425	2608	2611	2616	rVB2	25727	35705	1.15%	0.175%
20	19.112	2724	2728	2733	rBV3	18131	32249	1.04%	0.158%
21	19.371	2767	2772	2779	rBV	196775	273167	8.84%	1.335%
22	19.629	2813	2816	2819	rVB5	33610	39991	1.29%	0.195%
23	19.729	2826	2833	2842	rVB	166845	279797	9.05%	1.368%
24	19.929	2861	2867	2873	rBV	2278269	3091742	100.00%	15.114%
25	20.387	2941	2945	2950	rVB2	20060	31974	1.03%	0.156%
26	20.528	2964	2969	2973	rBV3	23418	45783	1.48%	0.224%
27	20.669	2990	2993	2997	rBV5	31474	38486	1.24%	0.188%
28	21.016	3045	3052	3054	rBV7	55476	127082	4.11%	0.621%
29	21.227	3084	3088	3097	rVB4	151875	243769	7.88%	1.192%
30	21.574	3134	3147	3167	rVB2	844861	2811453	90.93%	13.744%
31	22.966	3380	3384	3385	rBV4	43262	57272	1.85%	0.280%
32	24.705	3670	3680	3690	rBV2	309724	918378	29.70%	4.489%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062620\
Data File : BG045872.D
Acq On : 26 Jun 2020 14:02
Operator : CG/JU
Sample : L3094-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BRENNAN-FL-001

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 20456499

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062620\
Data File : BG045872.D
Acq On : 26 Jun 2020 14:02
Operator : CG/JU
Sample : L3094-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BRENNAN-FL-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

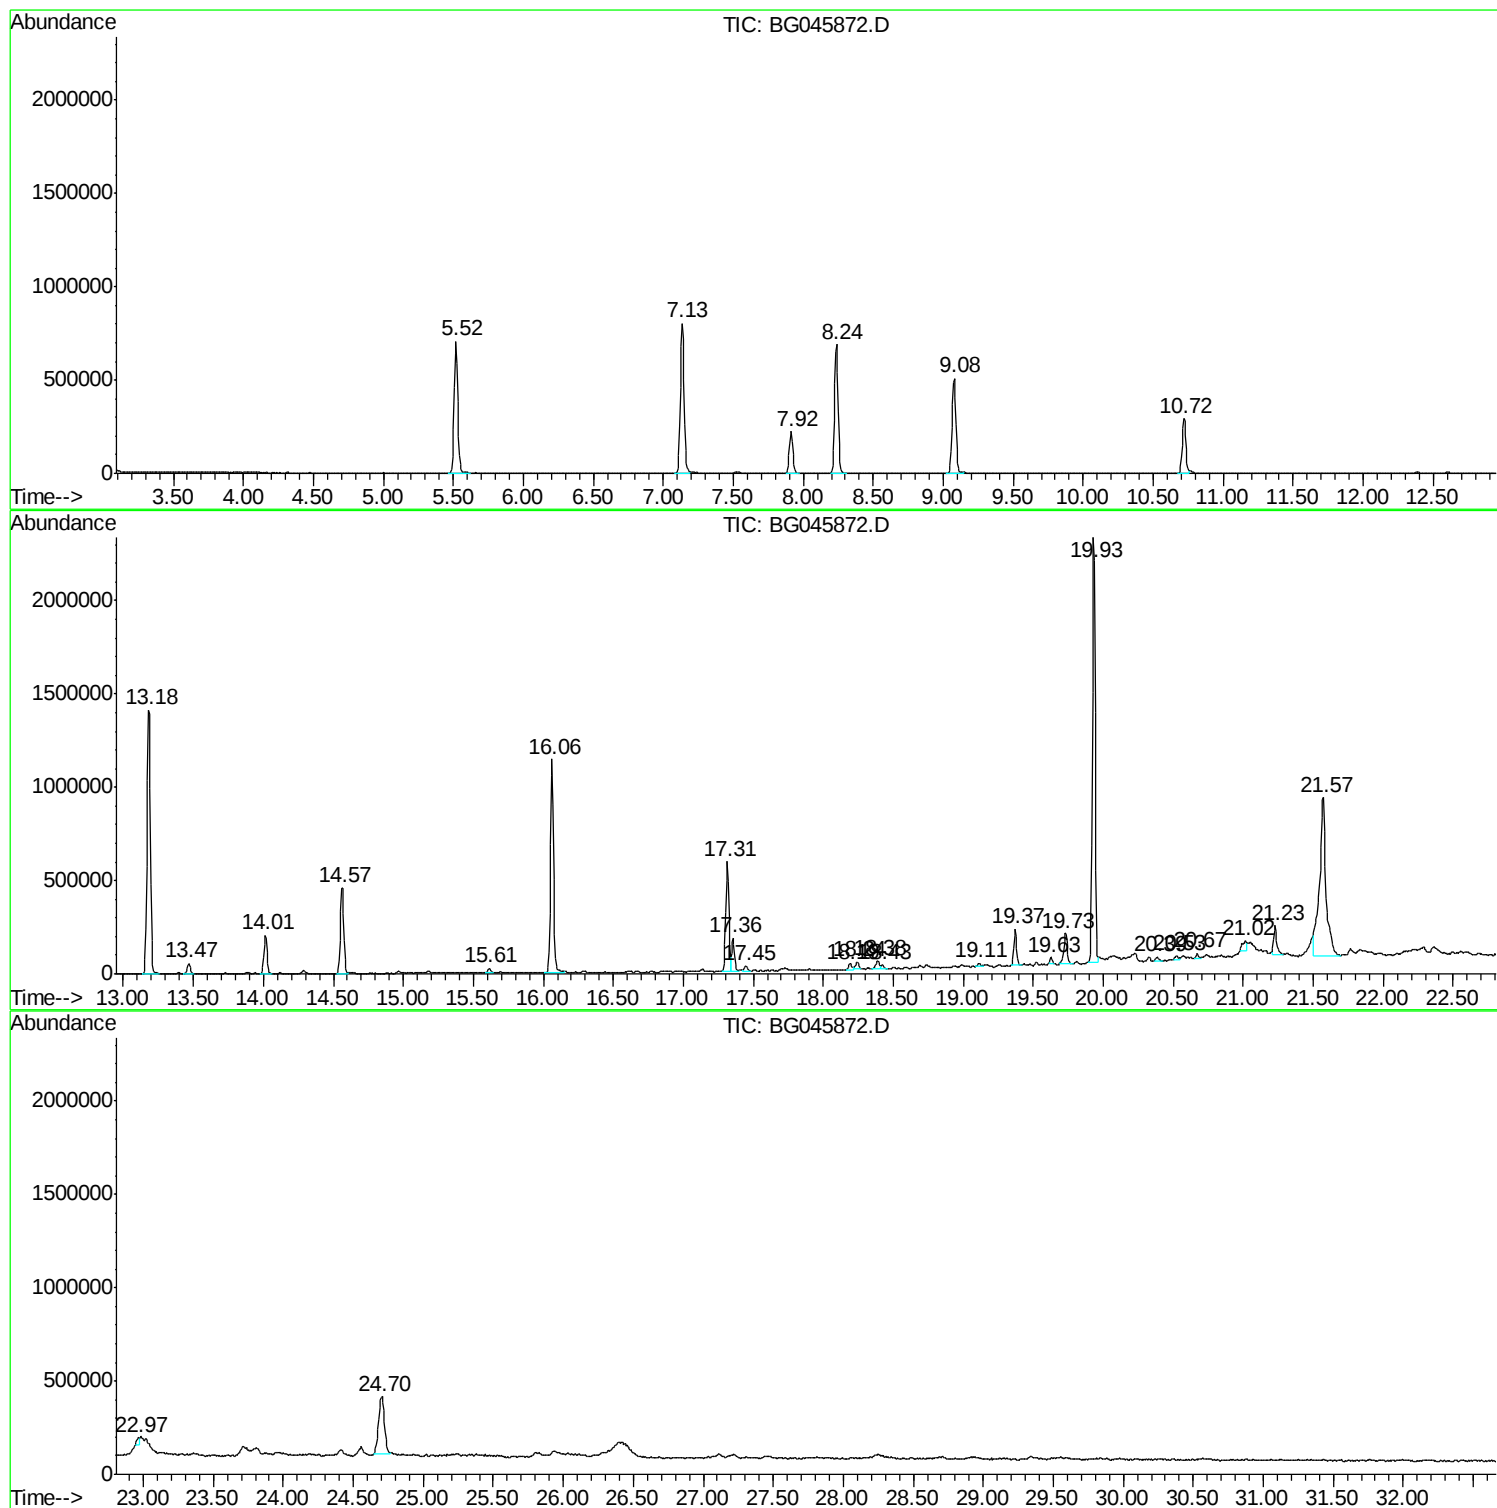

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062620\
Data File : BG045872.D
Acq On : 26 Jun 2020 14:02
Operator : CG/JU
Sample : L3094-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BRENNAN-FL-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062620\
Data File : BG045872.D
Acq On : 26 Jun 2020 14:02
Operator : CG/JU
Sample : L3094-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BRENNAN-FL-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc