

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062620\
 Data File : BG045873.D
 Acq On : 26 Jun 2020 14:42
 Operator : CG/JU
 Sample : L3094-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 2020-06-22-FD04

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.514	406	413	427	rBV	637817	1151562	38.37%	6.905%
2	7.136	681	689	702	rBV	706358	1290003	42.98%	7.735%
3	7.911	813	821	832	rBV	207813	364382	12.14%	2.185%
4	8.234	868	876	890	rBV	613195	1090046	36.32%	6.536%
5	9.074	1011	1019	1030	rBV	459878	854509	28.47%	5.124%
6	10.719	1292	1299	1312	rBV	269097	498753	16.62%	2.991%
7	13.181	1711	1718	1727	rBV	1313227	2072038	69.04%	12.425%
8	13.468	1761	1767	1774	rVB2	31474	49458	1.65%	0.297%
9	14.015	1854	1860	1868	rBV	155354	236083	7.87%	1.416%
10	14.561	1947	1953	1961	rBV	440235	713397	23.77%	4.278%
11	16.065	2202	2209	2224	rBV	1093715	1709095	56.95%	10.248%
12	17.316	2415	2422	2427	rBV	570343	901847	30.05%	5.408%
13	17.357	2427	2429	2434	rVB	51058	59499	1.98%	0.357%
14	18.379	2599	2603	2608	rBV6	17242	35010	1.17%	0.210%
15	19.372	2767	2772	2778	rVB	72247	109317	3.64%	0.655%
16	19.631	2811	2816	2824	rVB2	90458	114628	3.82%	0.687%
17	19.736	2826	2834	2839	rBV	69970	139308	4.64%	0.835%
18	19.936	2861	2868	2873	rBV	2160588	3001115	100.00%	17.996%
19	20.670	2990	2993	2997	rVB2	64088	67135	2.24%	0.403%
20	21.229	3083	3088	3097	rVB2	180776	291329	9.71%	1.747%
21	21.575	3139	3147	3153	rBV	531490	955783	31.85%	5.731%
22	21.769	3177	3180	3185	rVB4	30405	43551	1.45%	0.261%
23	24.700	3671	3679	3690	rVB2	323554	929116	30.96%	5.571%


Sum of corrected areas: 16676964

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062620\
Data File : BG045873.D
Acq On : 26 Jun 2020 14:42
Operator : CG/JU
Sample : L3094-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2020-06-22-FD04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

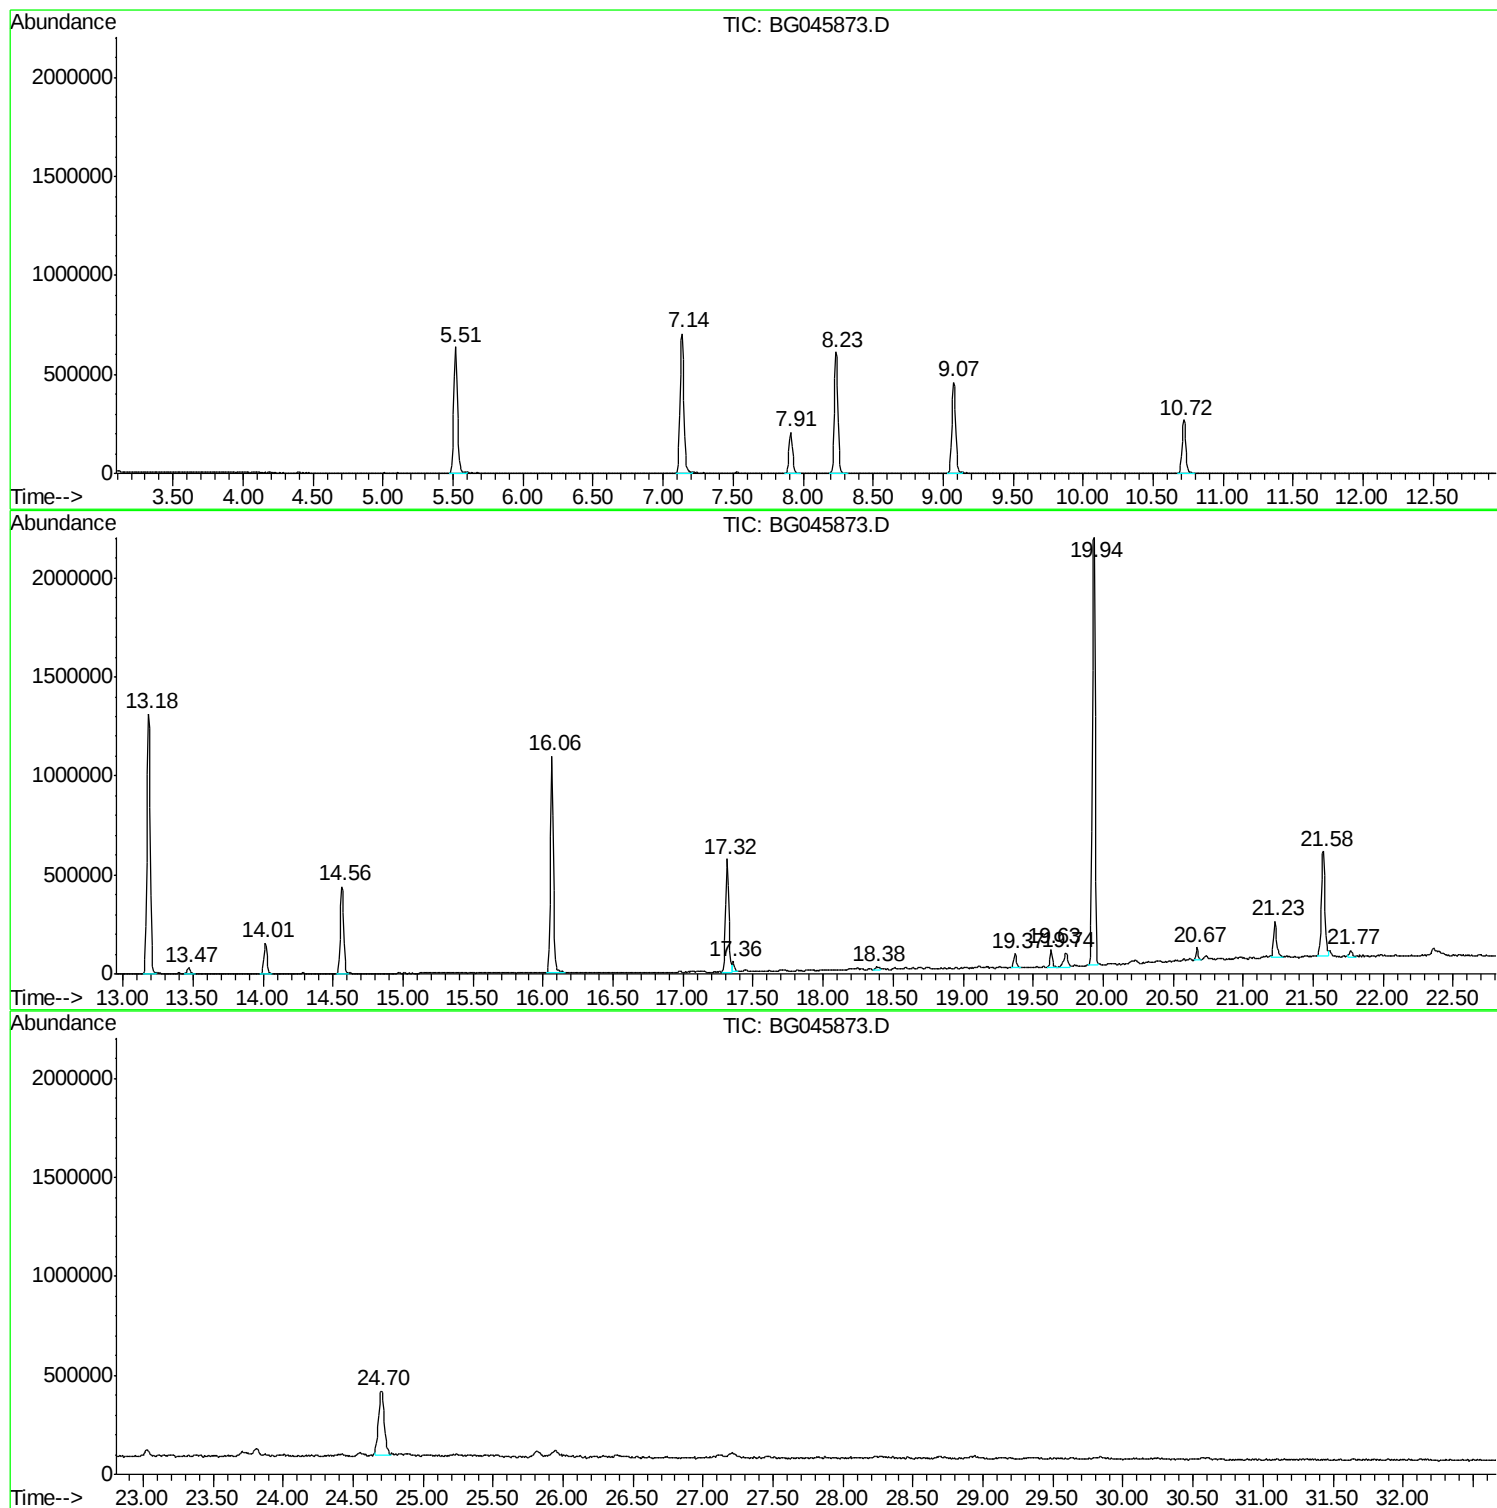

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062620\
Data File : BG045873.D
Acq On : 26 Jun 2020 14:42
Operator : CG/JU
Sample : L3094-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2020-06-22-FD04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062620\
Data File : BG045873.D
Acq On : 26 Jun 2020 14:42
Operator : CG/JU
Sample : L3094-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2020-06-22-FD04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc