


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062620\
 Data File : BG045866.D
 Acq On : 26 Jun 2020 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 25 15:44:32 2020

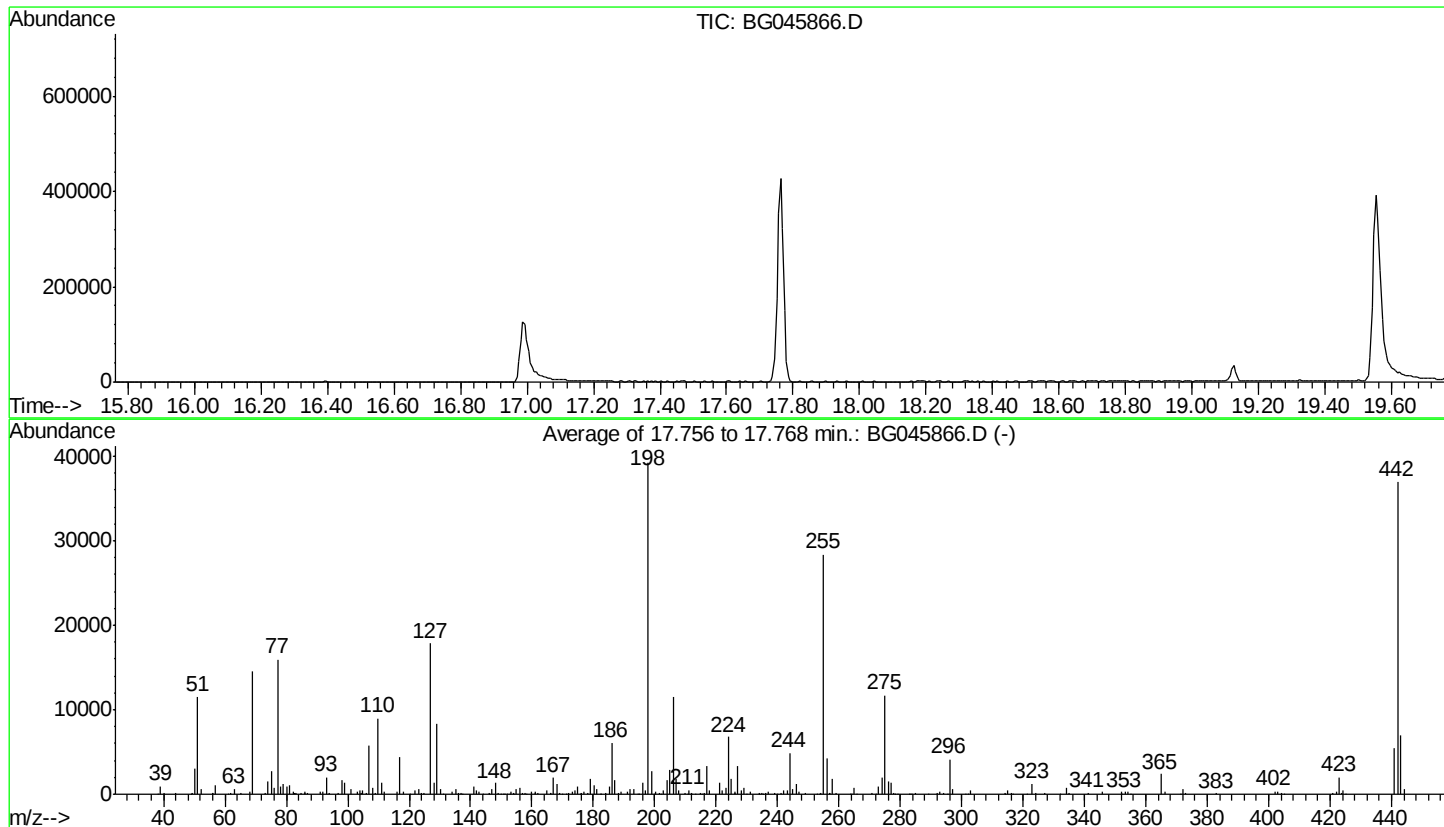

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	11535	PASS
68	69	0.00	2	1.9	272	PASS
69	198	0.00	100	37.0	14540	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.4	17836	PASS
197	198	0.00	2	1.0	394	PASS
198	198	100	100	100.0	39258	PASS
199	198	5	9	6.8	2672	PASS
275	198	10	60	29.8	11712	PASS
365	198	1	100	6.0	2360	PASS
441	198	0.01	100	14.0	5483	PASS
442	198	50	100	94.4	37045	PASS
443	442	15	24	18.7	6935	PASS