
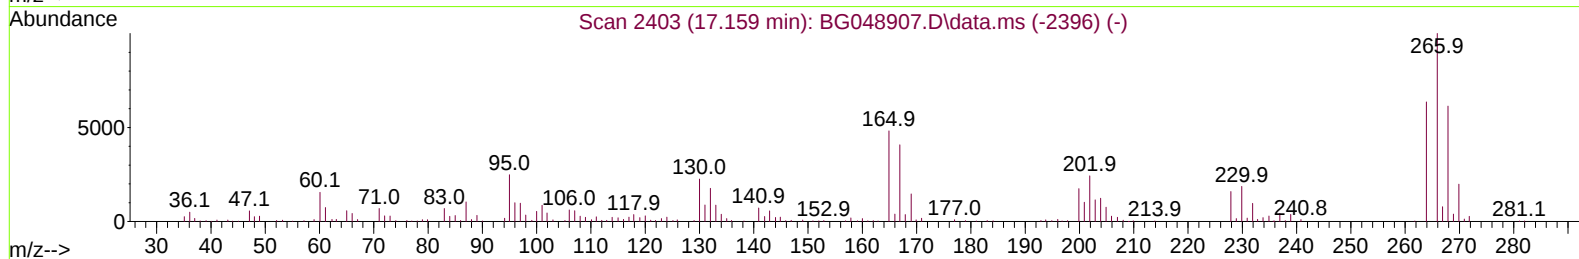
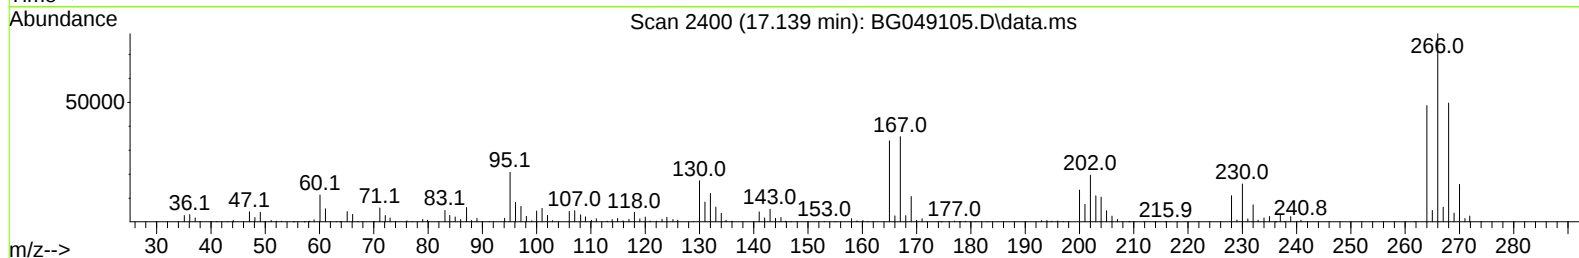


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049105.D
Acq On : 26 Jun 2021 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 05:15:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

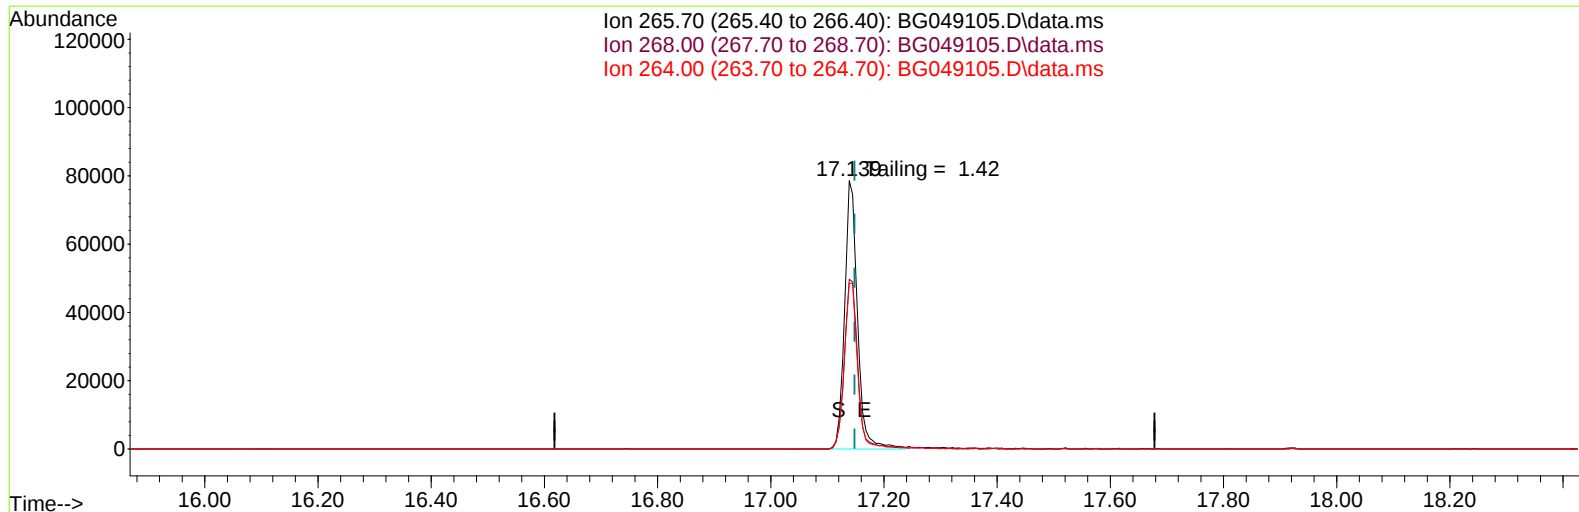

TIC: BG049105.D\data.ms

(70) Pentachlorophenol (C)




17.139min (-0.009) 137280.02 ng

response 125050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.24
264.00	61.30	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049105.D
Acq On : 26 Jun 2021 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 05:15:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

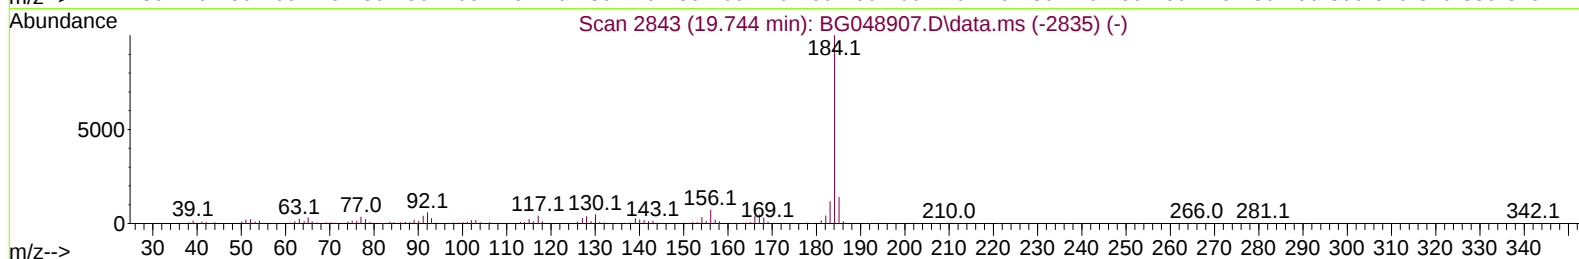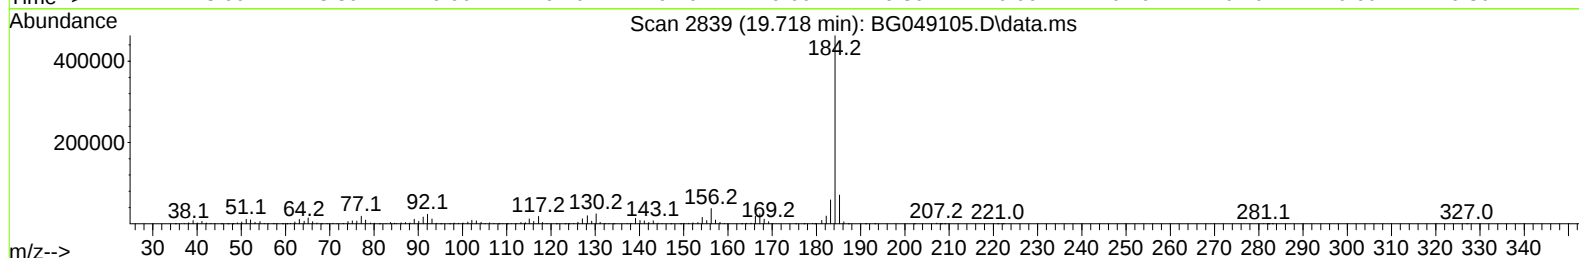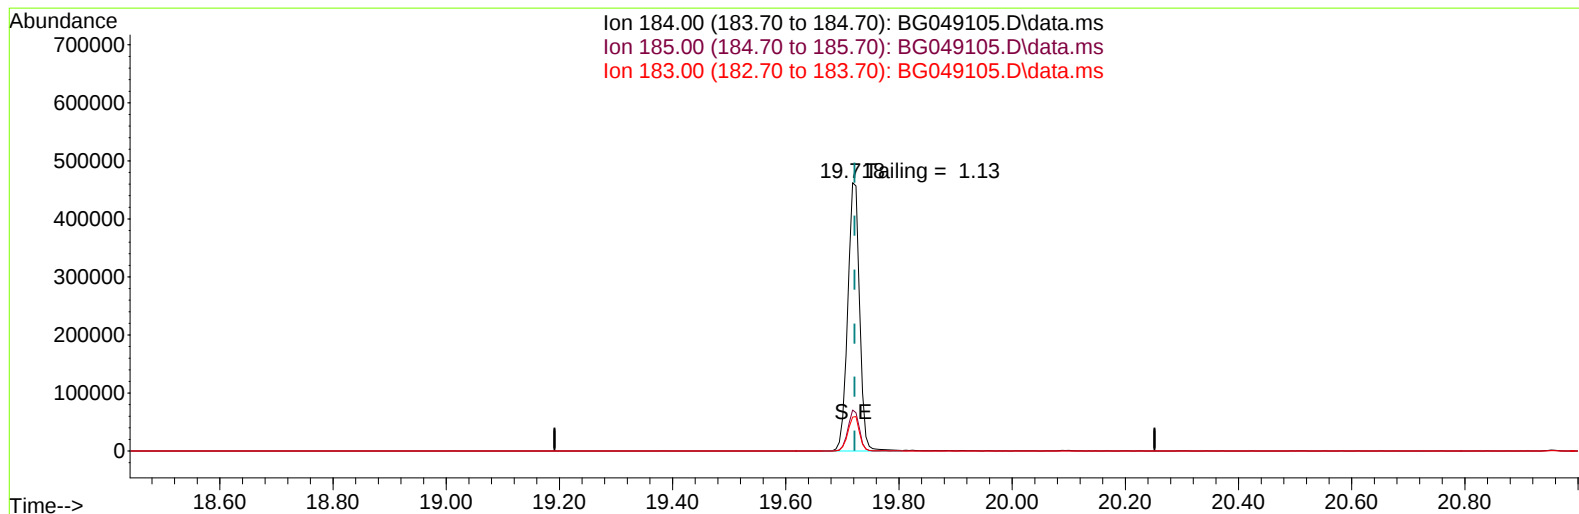

TIC: BG049105.D\data.ms

(77) Benzidine**19.718min (-0.003) 45073.93 ng****response 672837**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.30
183.00	11.70	12.67
0.00	0.00	0.00