

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
 Data File : BG049109.D
 Acq On : 26 Jun 2021 15:12
 Operator : CG/JU
 Sample : M2851-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049109.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.149	13	19	28	rBV	53402	105841	5.26%	1.054%
2	3.226	28	32	39	rVB3	16440	25398	1.26%	0.253%
3	5.652	438	445	458	rBV	470970	787864	39.15%	7.849%
4	7.256	710	718	729	rBV	481954	843473	41.92%	8.403%
5	8.102	854	862	869	rBV	123662	212797	10.58%	2.120%
6	9.272	1053	1061	1070	rVB	287521	535341	26.60%	5.334%
7	10.682	1294	1301	1311	rBV	184955	331283	16.46%	3.301%
8	10.923	1335	1342	1350	rVB	150937	289311	14.38%	2.882%
9	13.367	1751	1758	1765	rBV	722902	1117824	55.55%	11.137%
10	14.742	1985	1992	1998	rBV	266400	419900	20.87%	4.183%
11	16.228	2239	2245	2255	rVB	739571	1160455	57.67%	11.562%
12	17.491	2453	2460	2468	rBV	372760	571475	28.40%	5.694%
13	18.149	2566	2572	2577	rBV2	37394	49975	2.48%	0.498%
14	18.367	2604	2609	2615	rBV2	42928	60823	3.02%	0.606%
15	19.313	2767	2770	2774	rVB3	25781	29319	1.46%	0.292%
16	19.636	2820	2825	2832	rBV7	34644	53383	2.65%	0.532%
17	20.094	2898	2903	2909	rBV	1498408	2012214	100.00%	20.048%
18	21.422	3122	3129	3135	rBV5	39655	98559	4.90%	0.982%
19	21.493	3137	3141	3147	rVB2	29240	41785	2.08%	0.416%
20	21.775	3183	3189	3195	rBV2	366805	620286	30.83%	6.180%
21	25.100	3744	3755	3774	rVB3	209599	669921	33.29%	6.674%




Sum of corrected areas: 10037227

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049109.D
Acq On : 26 Jun 2021 15:12
Operator : CG/JU
Sample : M2851-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-07

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

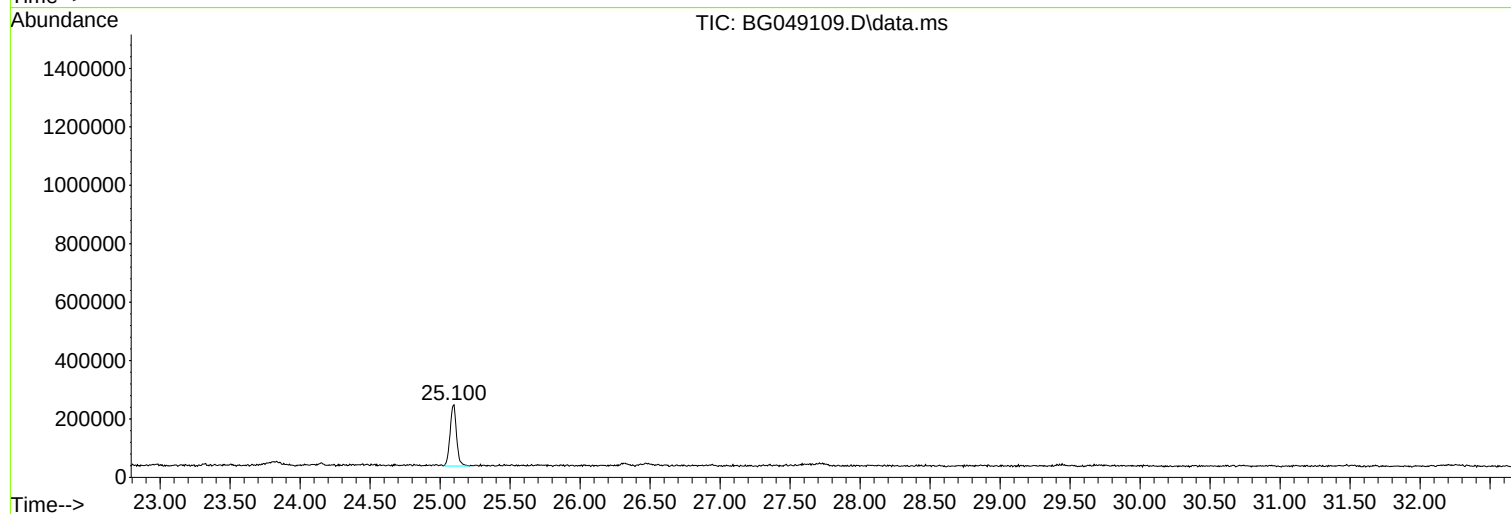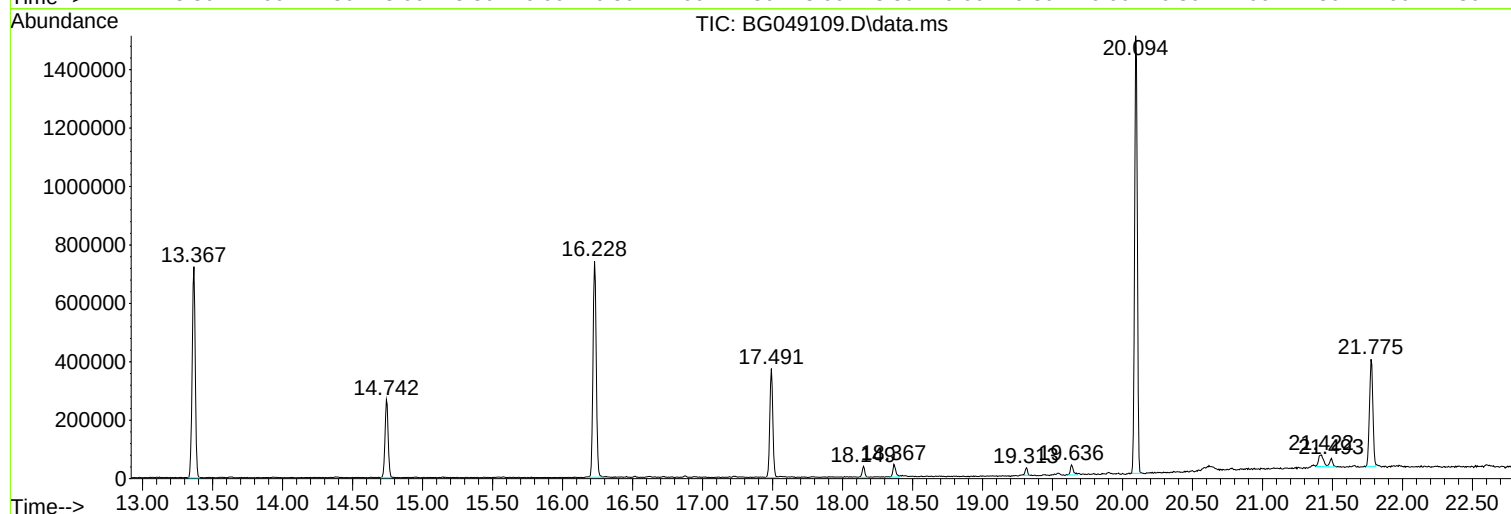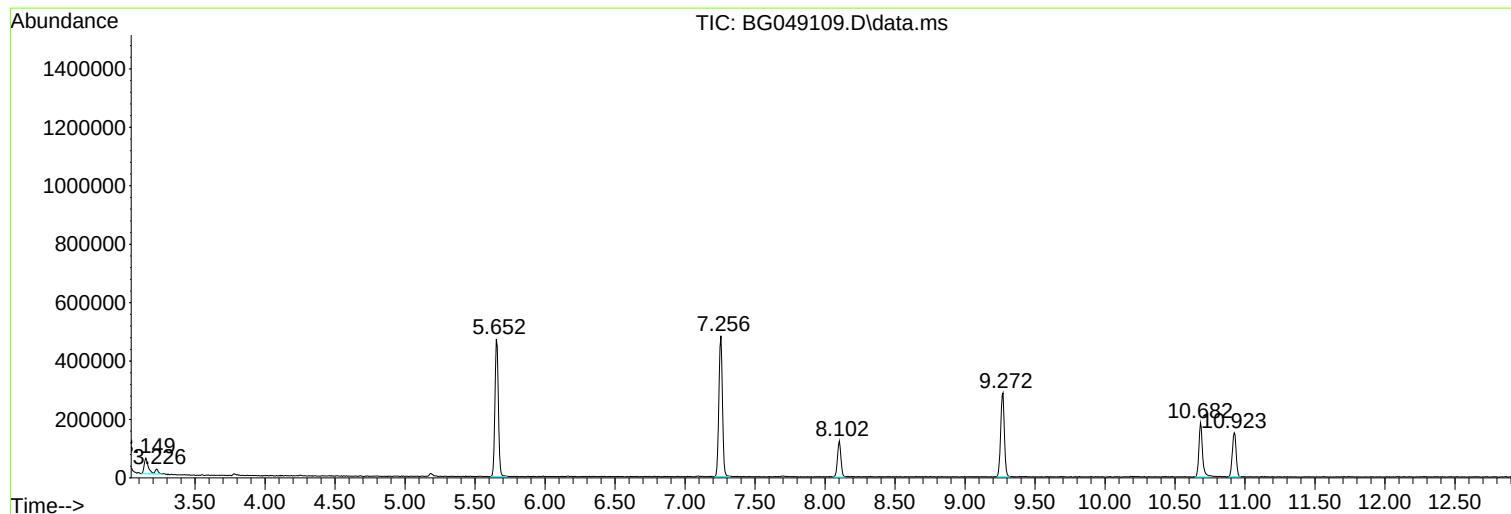

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049109.D
Acq On : 26 Jun 2021 15:12
Operator : CG/JU
Sample : M2851-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-07

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049109.D
Acq On : 26 Jun 2021 15:12
Operator : CG/JU
Sample : M2851-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-07

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------