

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
 Data File : BG049110.D
 Acq On : 26 Jun 2021 15:53
 Operator : CG/JU
 Sample : M2851-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.149	13	19	28	rBV	56494	116160	5.96%	1.162%
2	3.226	28	32	40	rVB2	20413	34842	1.79%	0.349%
3	5.182	361	365	373	rBV3	12786	20589	1.06%	0.206%
4	5.652	438	445	457	rVB	481364	808990	41.54%	8.095%
5	7.256	708	718	728	rBV	501721	880925	45.23%	8.815%
6	8.102	855	862	868	rBV	116964	197275	10.13%	1.974%
7	9.266	1052	1060	1070	rBV	302203	556615	28.58%	5.569%
8	10.682	1295	1301	1311	rBV	207111	366785	18.83%	3.670%
9	10.923	1335	1342	1353	rVB	153305	277578	14.25%	2.777%
10	13.367	1749	1758	1766	rBV	746751	1161663	59.65%	11.624%
11	14.742	1986	1992	1999	rBV	262122	410736	21.09%	4.110%
12	16.228	2239	2245	2254	rBV	763805	1172582	60.21%	11.733%
13	17.491	2453	2460	2468	rBV	368998	544509	27.96%	5.448%
14	18.149	2566	2572	2578	rBV	43865	57313	2.94%	0.573%
15	18.367	2603	2609	2616	rBV5	30091	46129	2.37%	0.462%
16	19.313	2767	2770	2774	rVB2	45939	48926	2.51%	0.490%
17	19.636	2821	2825	2832	rBV7	19342	36978	1.90%	0.370%
18	20.094	2897	2903	2909	rBV	1507274	1947577	100.00%	19.487%
19	21.416	3123	3128	3135	rVB7	38452	77801	3.99%	0.778%
20	21.487	3137	3140	3144	rVB	28992	33739	1.73%	0.338%
21	21.775	3182	3189	3195	rBV2	339523	580373	29.80%	5.807%
22	25.094	3744	3754	3770	rVB2	192523	615950	31.63%	6.163%




Sum of corrected areas: 9994035

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049110.D
Acq On : 26 Jun 2021 15:53
Operator : CG/JU
Sample : M2851-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

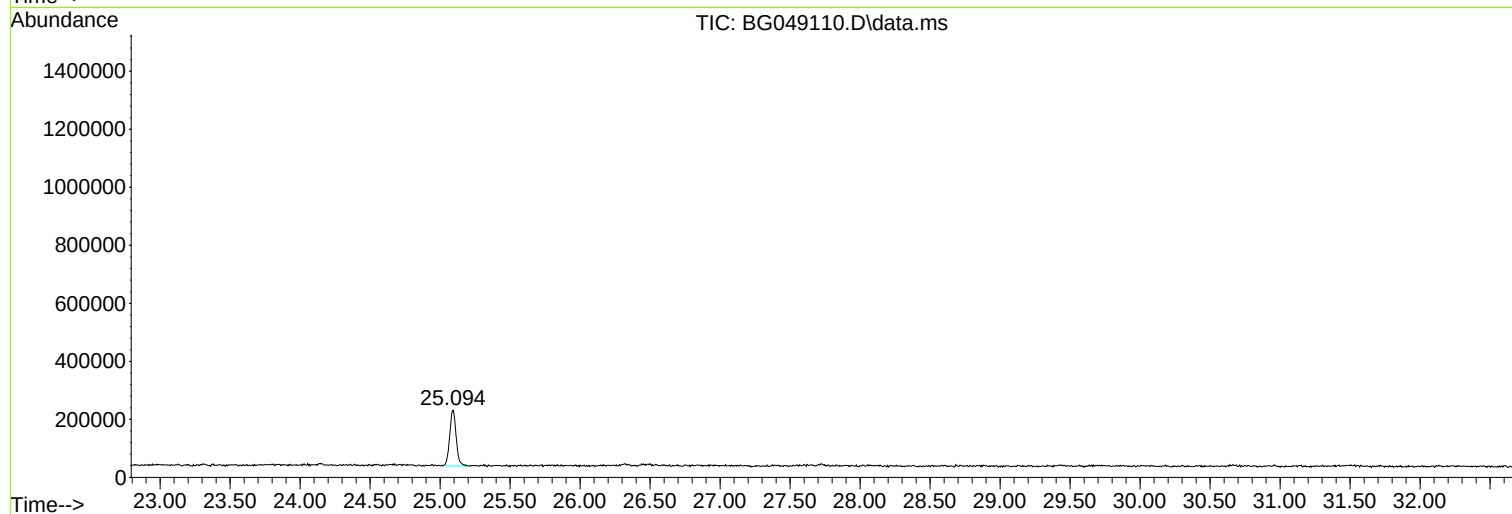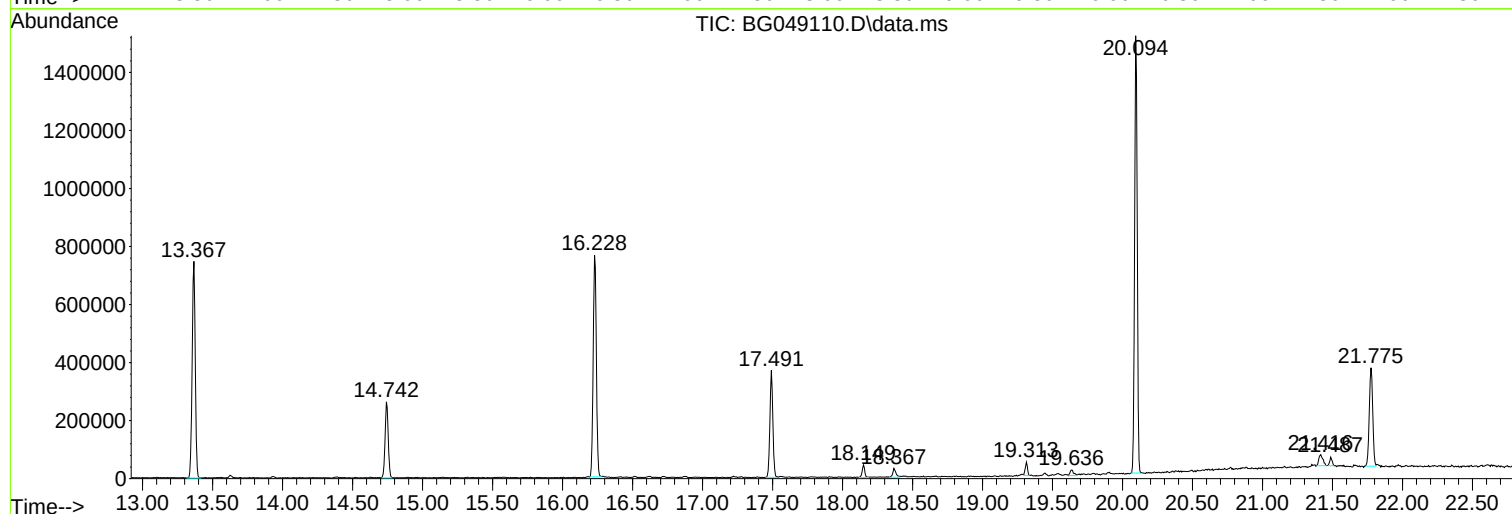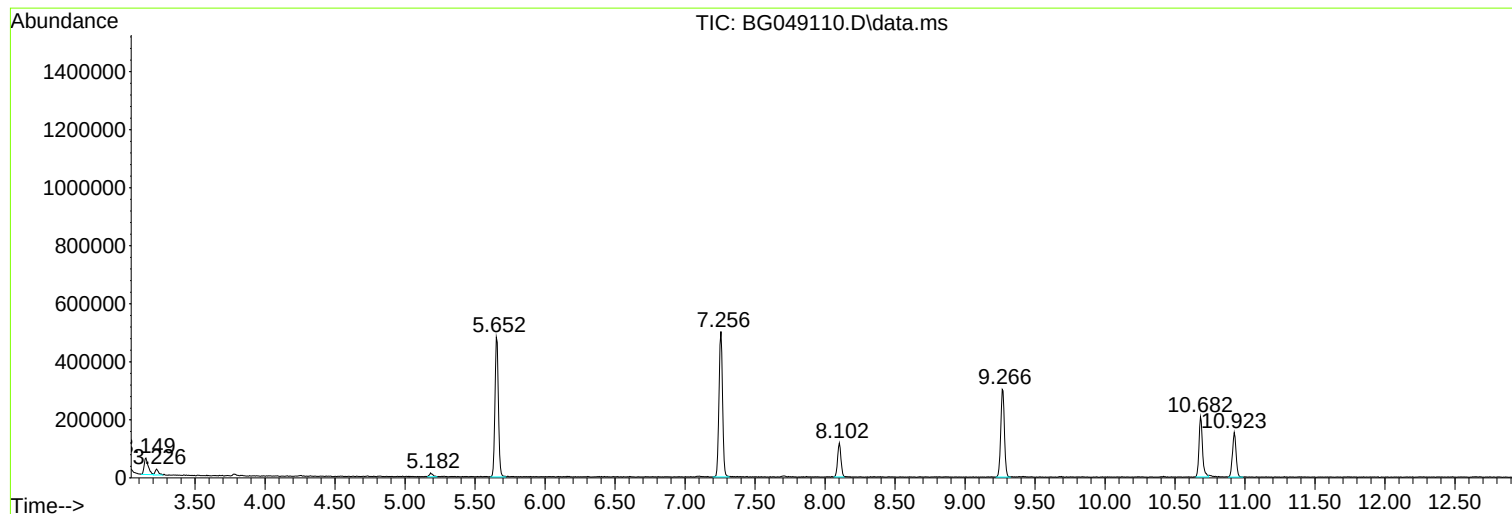

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049110.D
Acq On : 26 Jun 2021 15:53
Operator : CG/JU
Sample : M2851-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049110.D
Acq On : 26 Jun 2021 15:53
Operator : CG/JU
Sample : M2851-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------