
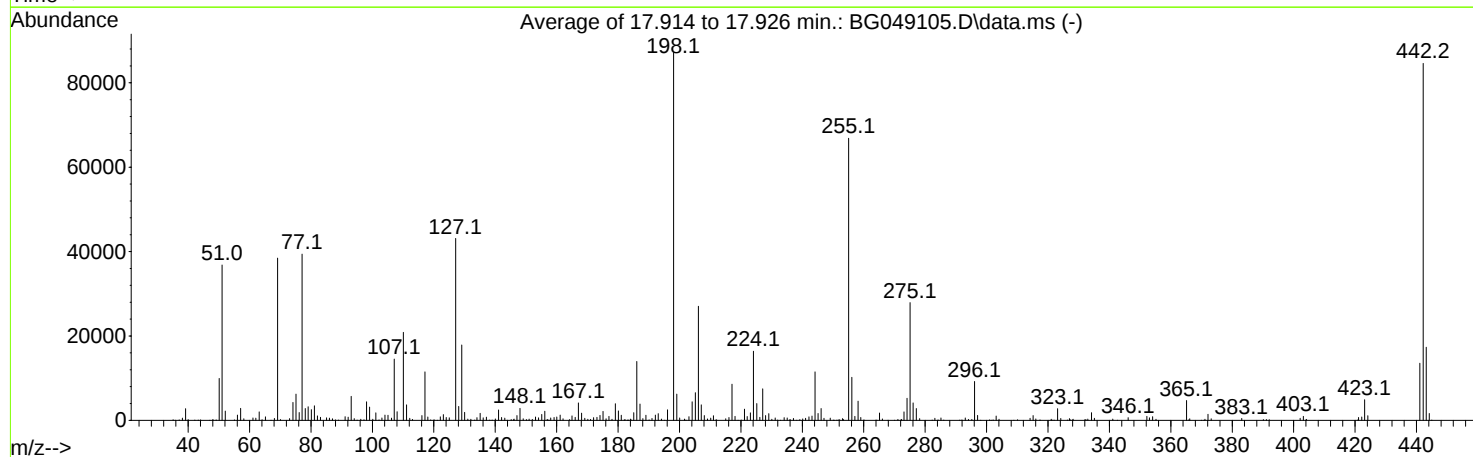


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
 Data File : BG049105.D
 Acq On : 26 Jun 2021 12:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 24 11:02:36 2021

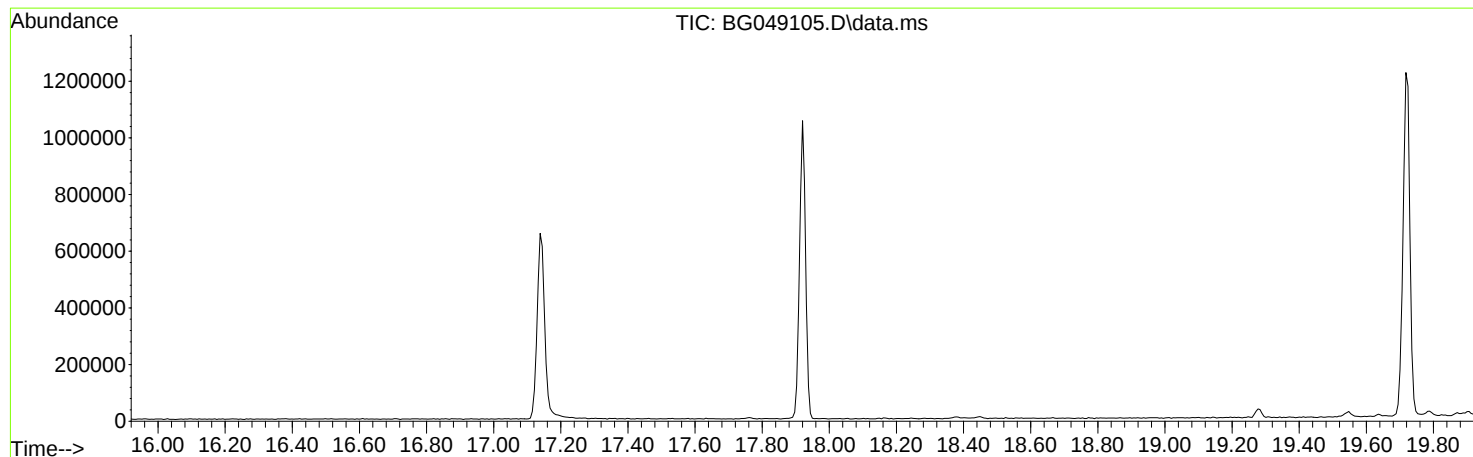

AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	36833	PASS
68	69	0.00	2	1.2	466	PASS
69	198	0.00	100	44.1	38443	PASS
70	69	0.00	2	0.5	207	PASS
127	198	10	80	49.5	43117	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87179	PASS
199	198	5	9	7.1	6228	PASS
275	198	10	60	32.0	27925	PASS
365	198	1	100	5.4	4714	PASS
441	198	0.01	100	15.5	13556	PASS
442	442	100	100	100.0	84611	PASS
443	442	15	24	20.5	17330	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/26/2021	BNA_G	<u>BG049105.D</u>
Compound Name	Response	Retention Time
DDT	331168	20.958
DDD	4812	20.505
DDE	785	20.006
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5597	336765	1.66

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
 Data File : BG049105.D
 Acq On : 26 Jun 2021 12:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 27 05:15:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 24 11:02:36 2021
 Response via : Initial Calibration

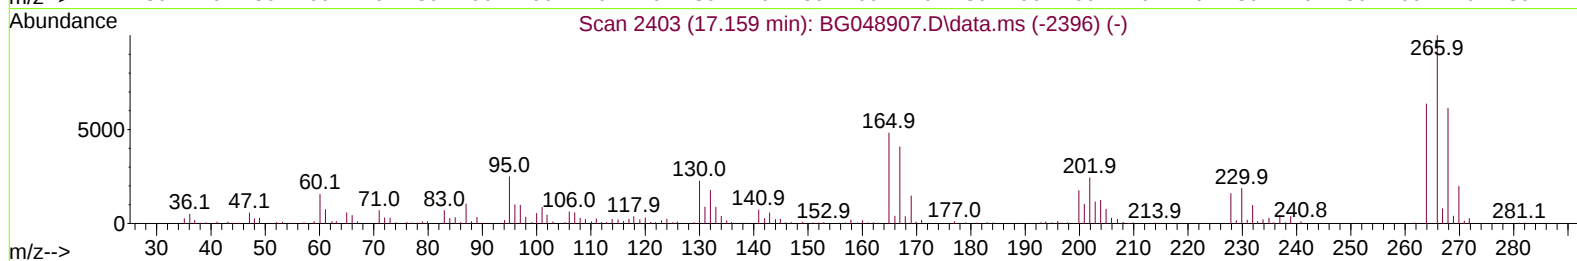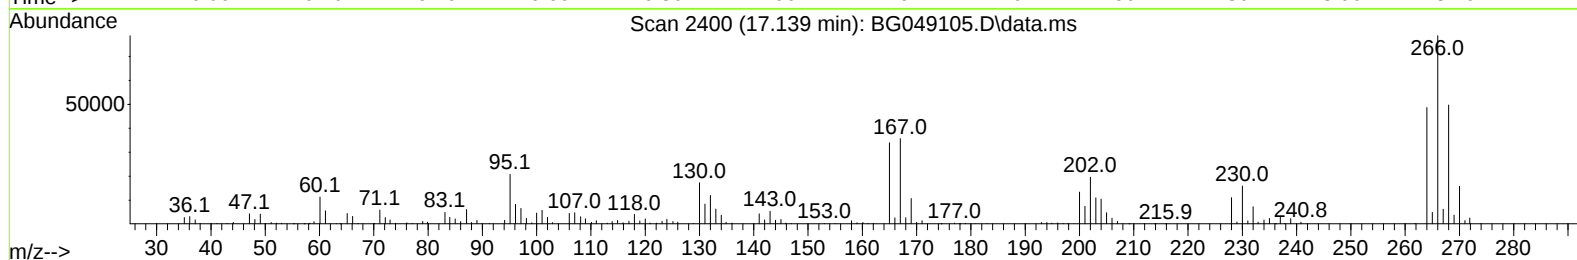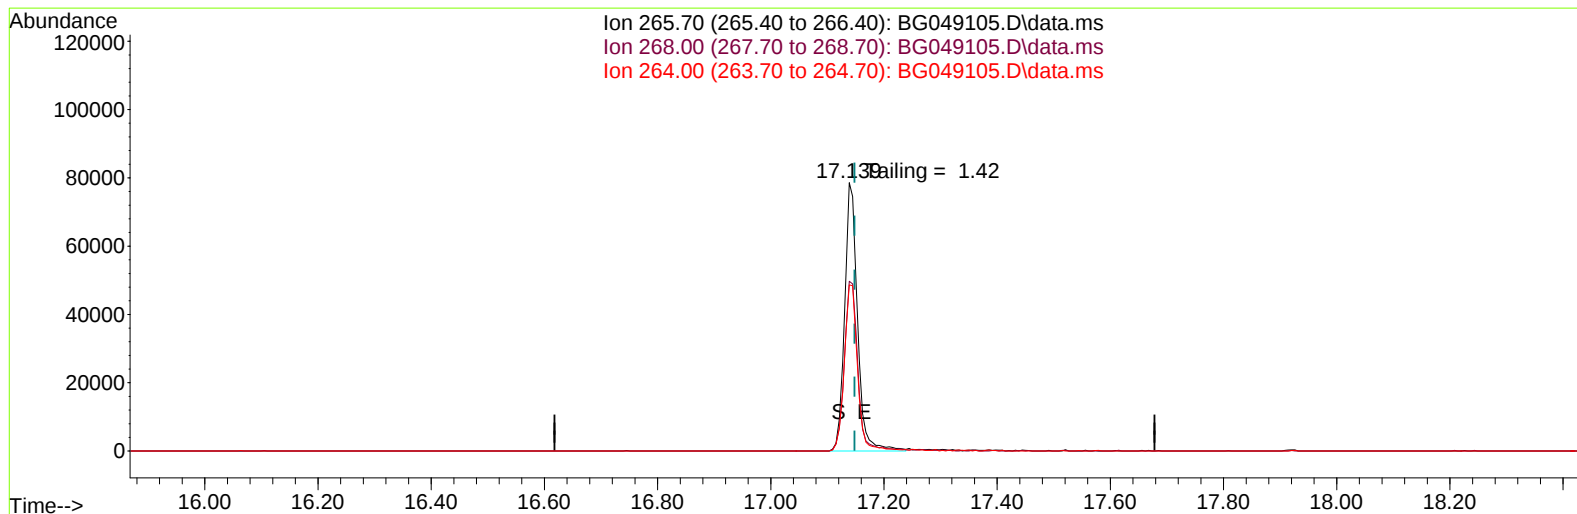

TIC: BG049105.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.009) 137280.02 ng




response 125050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.24
264.00	61.30	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062621\
Data File : BG049105.D
Acq On : 26 Jun 2021 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 27 05:15:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

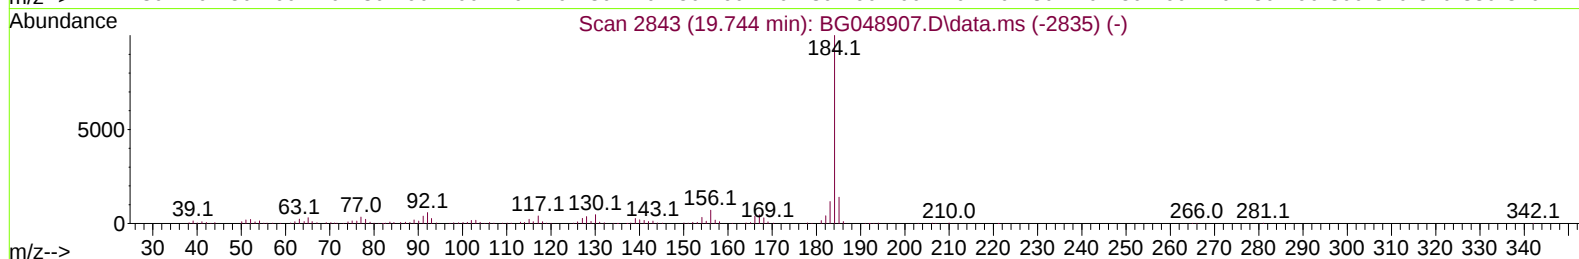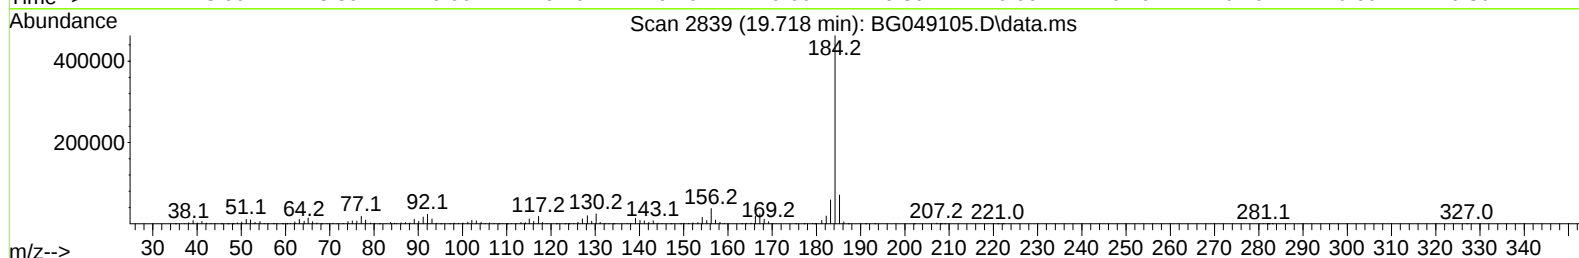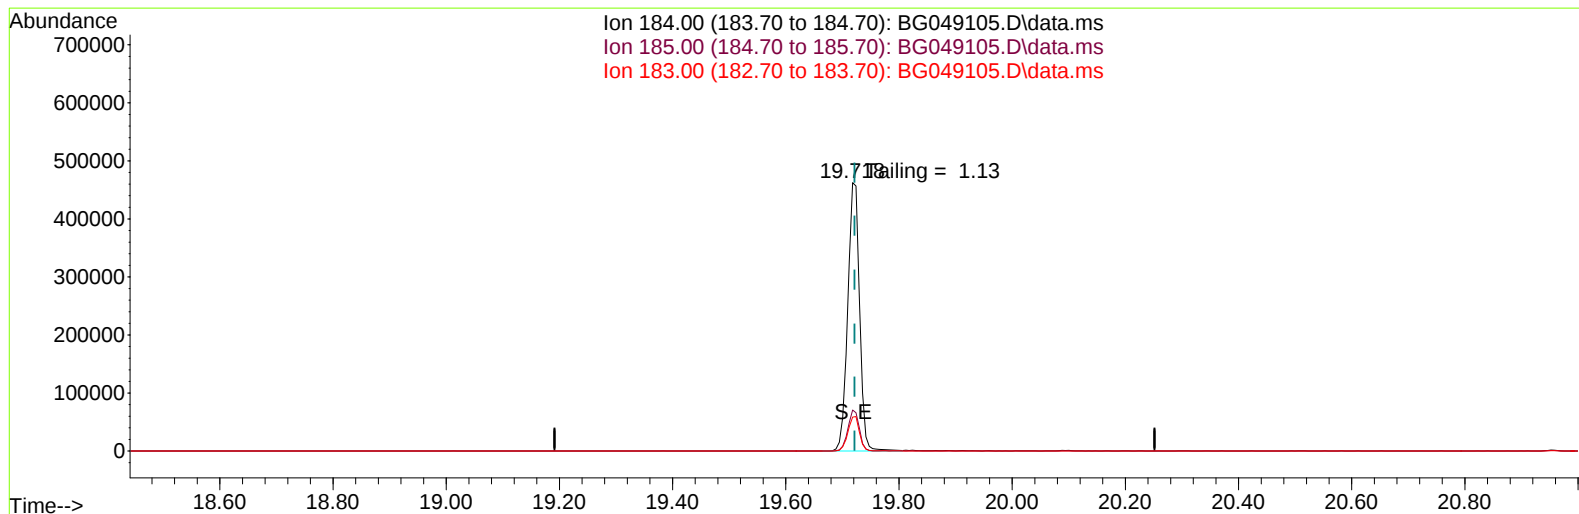

TIC: BG049105.D\data.ms

(77) Benzidine

19.718min (-0.003) 45073.93 ng

response 672837

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.30
183.00	11.70	12.67
0.00	0.00	0.00