


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062718\
 Data File : BG035464.D
 Acq On : 28 Jun 2018 3:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

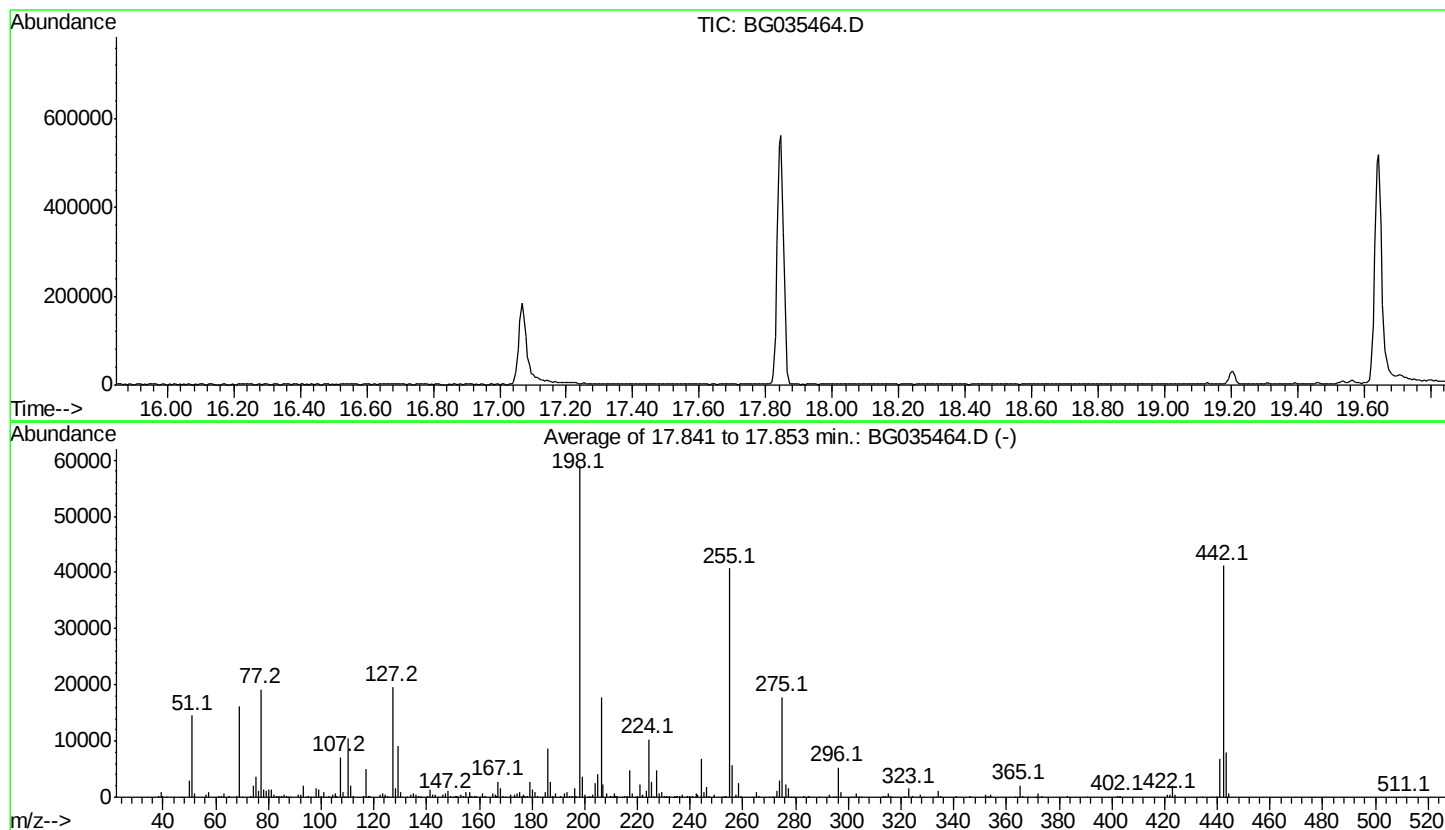

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	14571	PASS
68	69	0.00	2	1.6	262	PASS
69	198	0.00	100	27.5	16232	PASS
70	69	0.00	2	0.4	58	PASS
127	198	10	80	33.3	19657	PASS
197	198	0.00	2	0.6	331	PASS
198	198	100	100	100.0	59029	PASS
199	198	5	9	6.3	3701	PASS
275	198	10	60	30.1	17777	PASS
365	198	1	100	3.5	2055	PASS
441	443	0.01	100	84.6	6739	PASS
442	198	50	100	69.7	41138	PASS
443	442	15	24	19.4	7964	PASS