
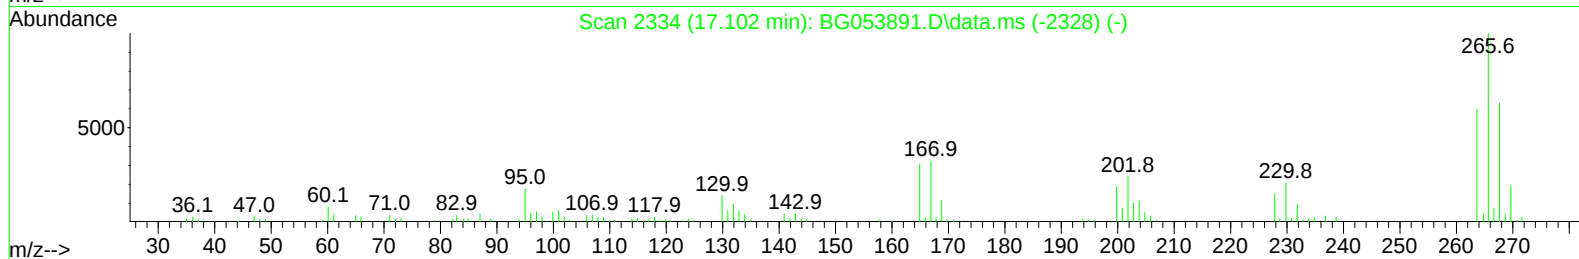
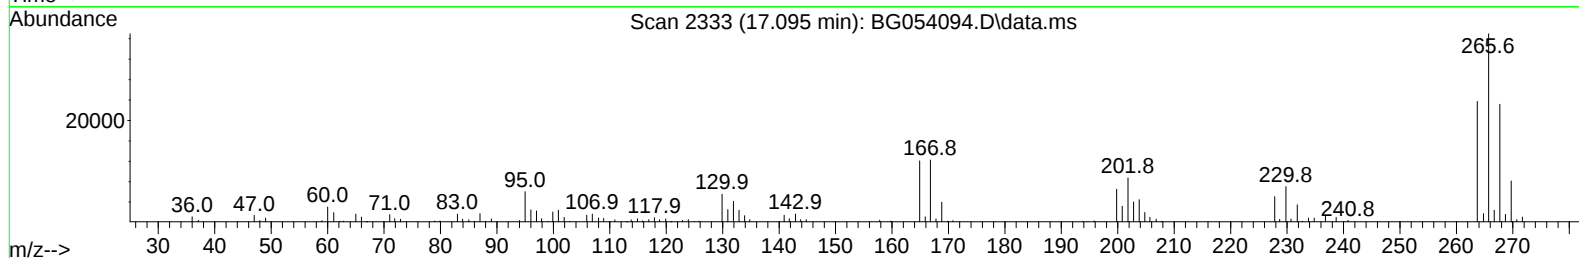


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\  
Data File : BG054094.D  
Acq On    : 27 Jun 2022  16:27  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 28 05:14:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

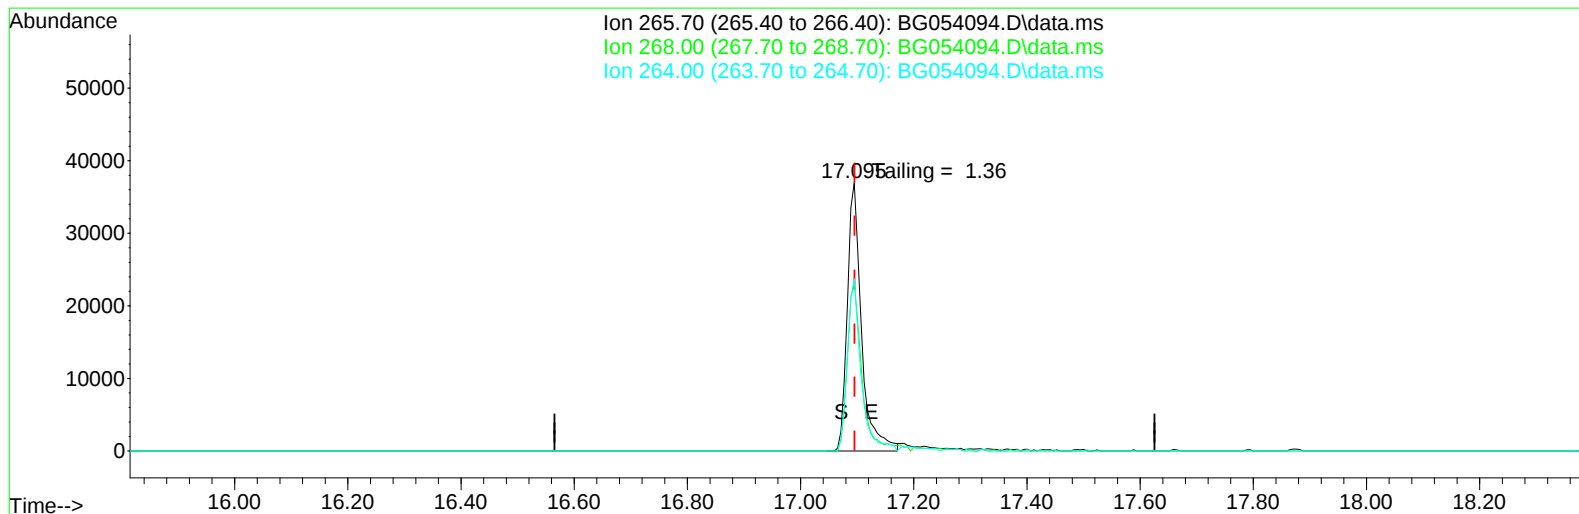

TIC: BG054094.D\data.ms

(70) Pentachlorophenol (C)

17.095min (-0.000) 31468.30 ng

response 66410

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	70.20	67.03
--------	-------	-------

264.00	66.20	64.18
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\
Data File : BG054094.D
Acq On : 27 Jun 2022 16:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 05:14:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

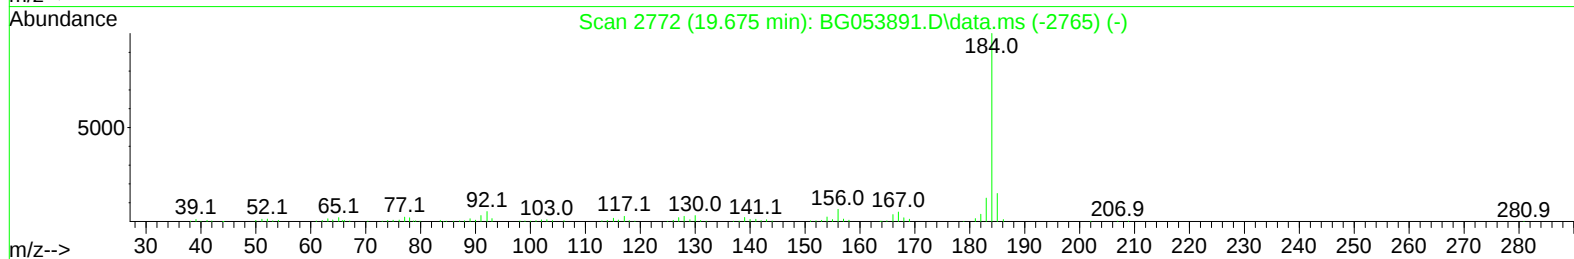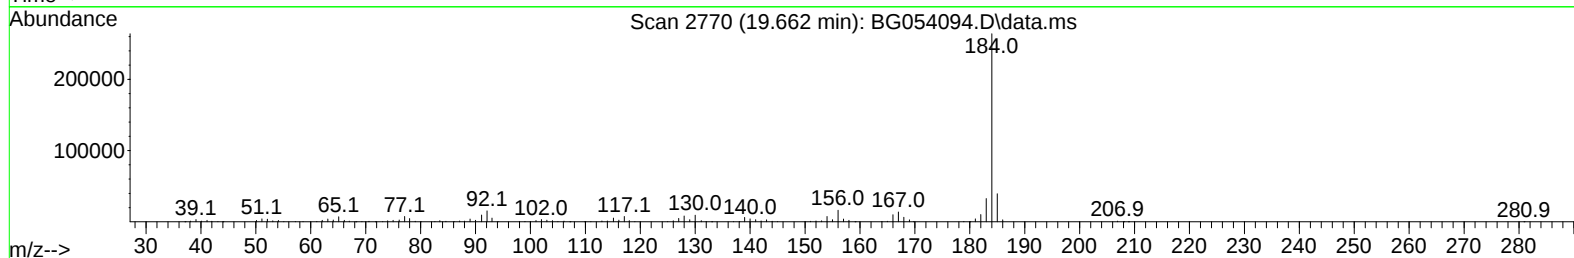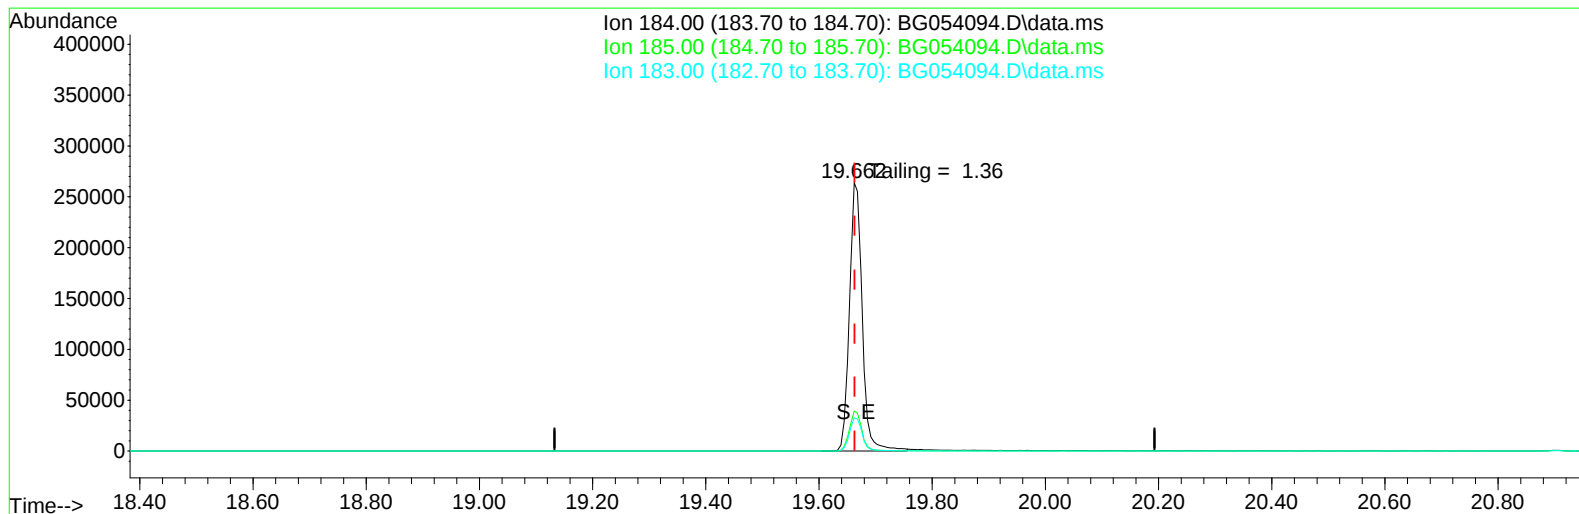

TIC: BG054094.D\data.ms

(77) Benzidine

19.662min (-0.000) 0.00 ng

response 416967

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.93
183.00	11.10	12.40
0.00	0.00	0.00