
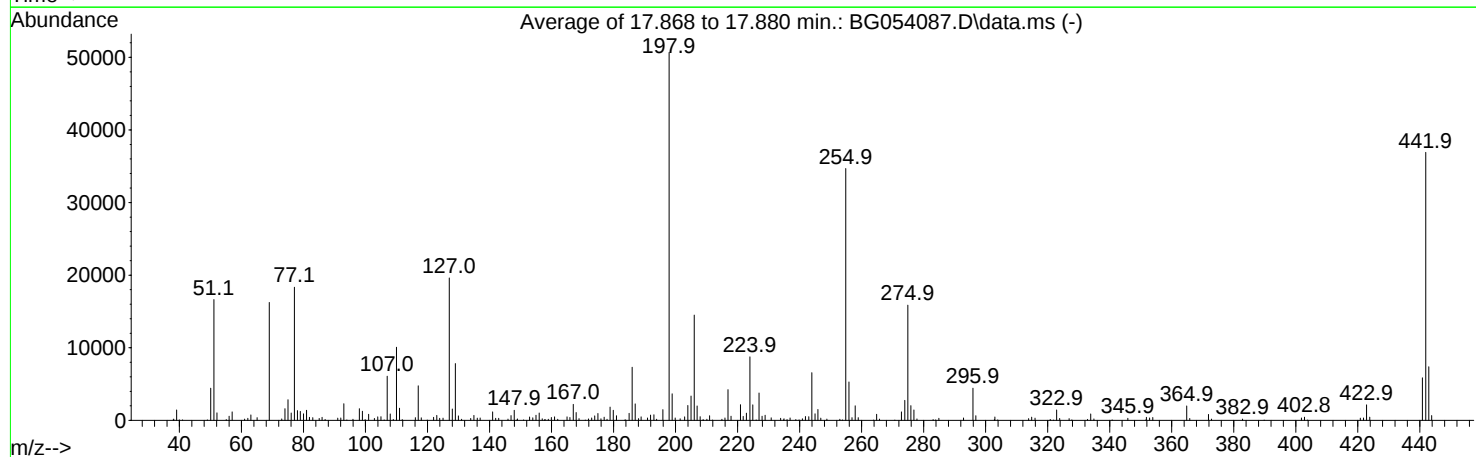


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\
 Data File : BG054087.D
 Acq On : 27 Jun 2022 9:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

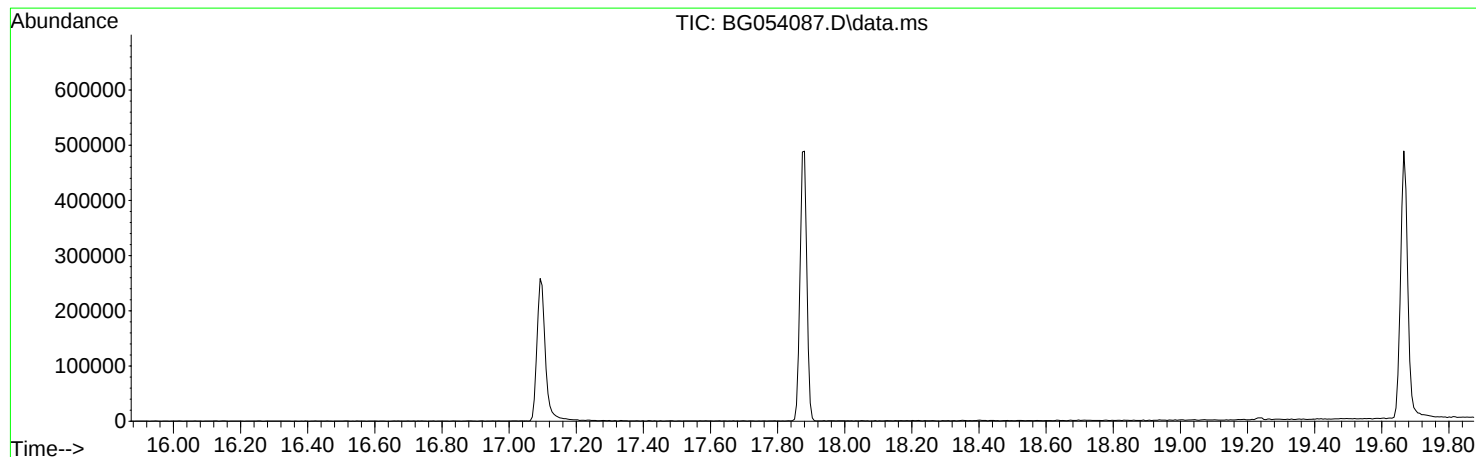




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	16647	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	16242	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.7	19620	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50667	PASS
199	198	5	9	7.2	3649	PASS
275	198	10	60	31.3	15875	PASS
365	198	1	100	3.9	1995	PASS
441	198	0.01	100	11.6	5857	PASS
442	442	50	100	100.0	36907	PASS
443	442	15	24	20.0	7391	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\
Data File : BG054087.D
Acq On : 27 Jun 2022 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 05:16:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

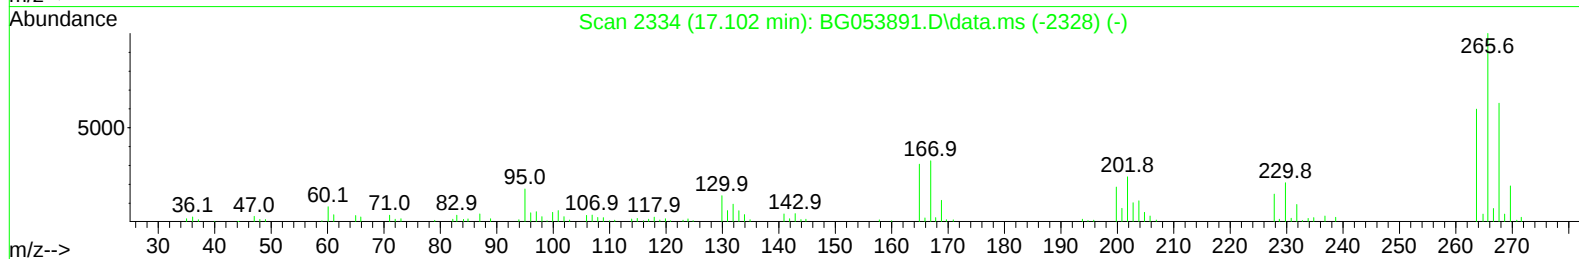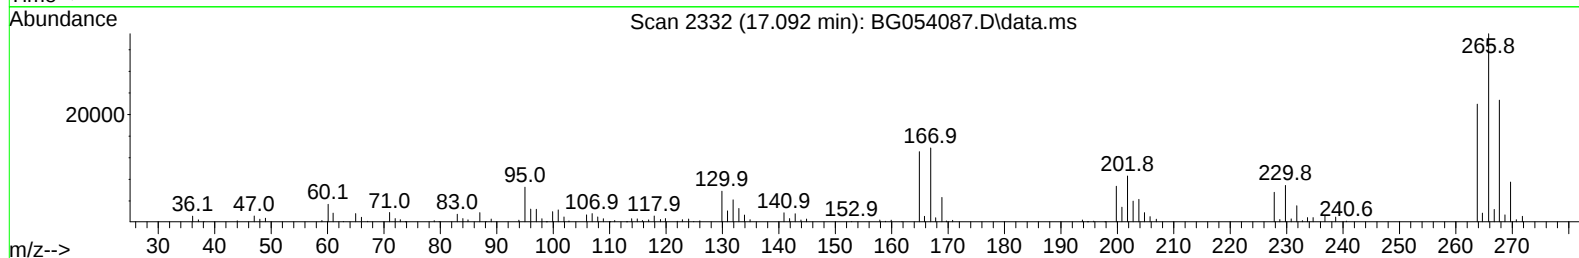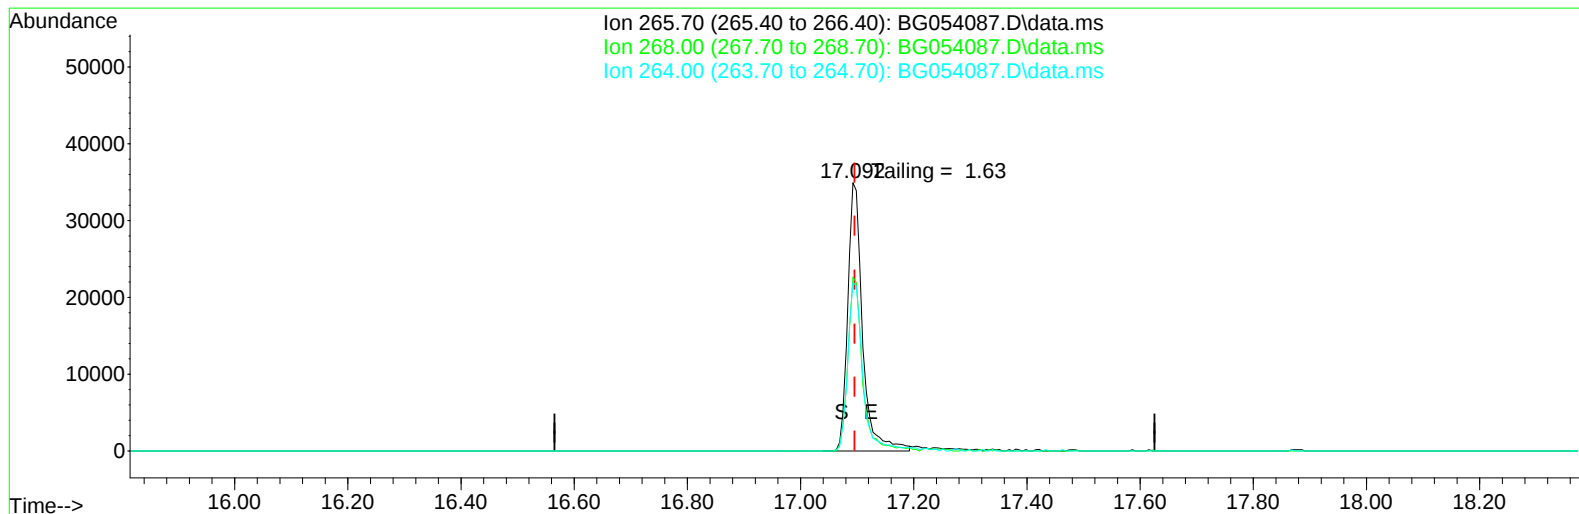

TIC: BG054087.D\data.ms

(70) Pentachlorophenol (C)

17.092min (-0.003) 36647.47 ng




response 64450

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.89
264.00	66.20	67.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\
Data File : BG054087.D
Acq On : 27 Jun 2022 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 05:16:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

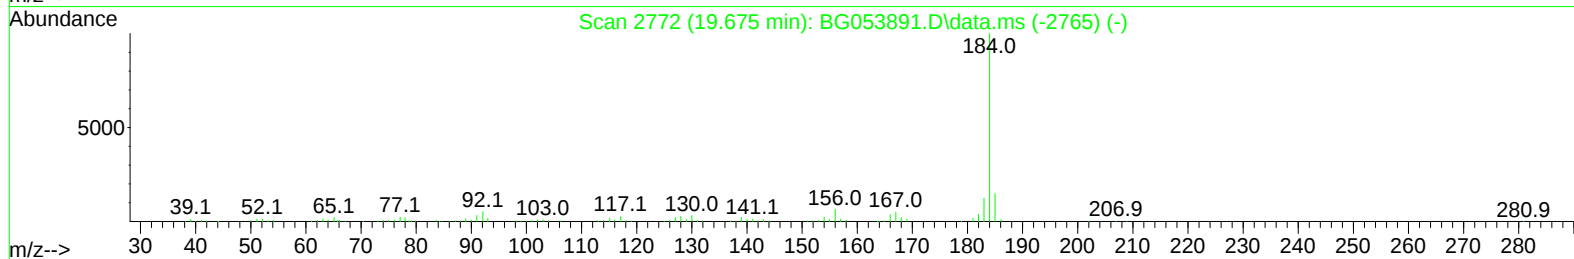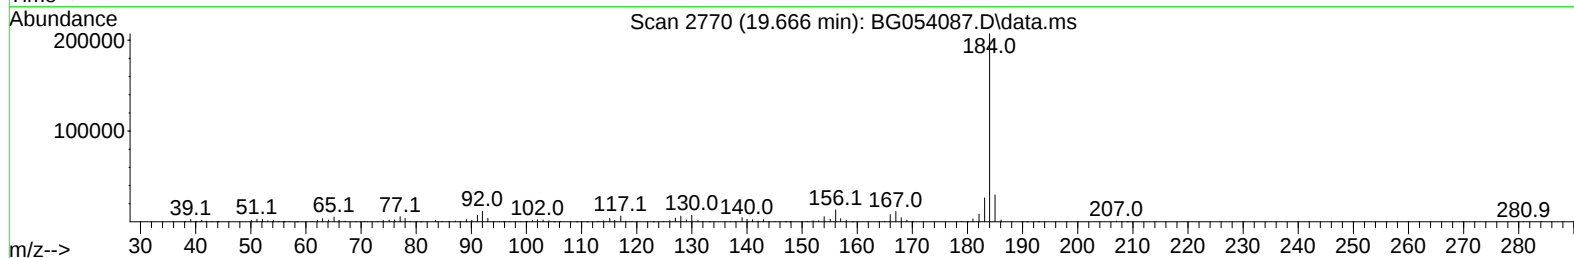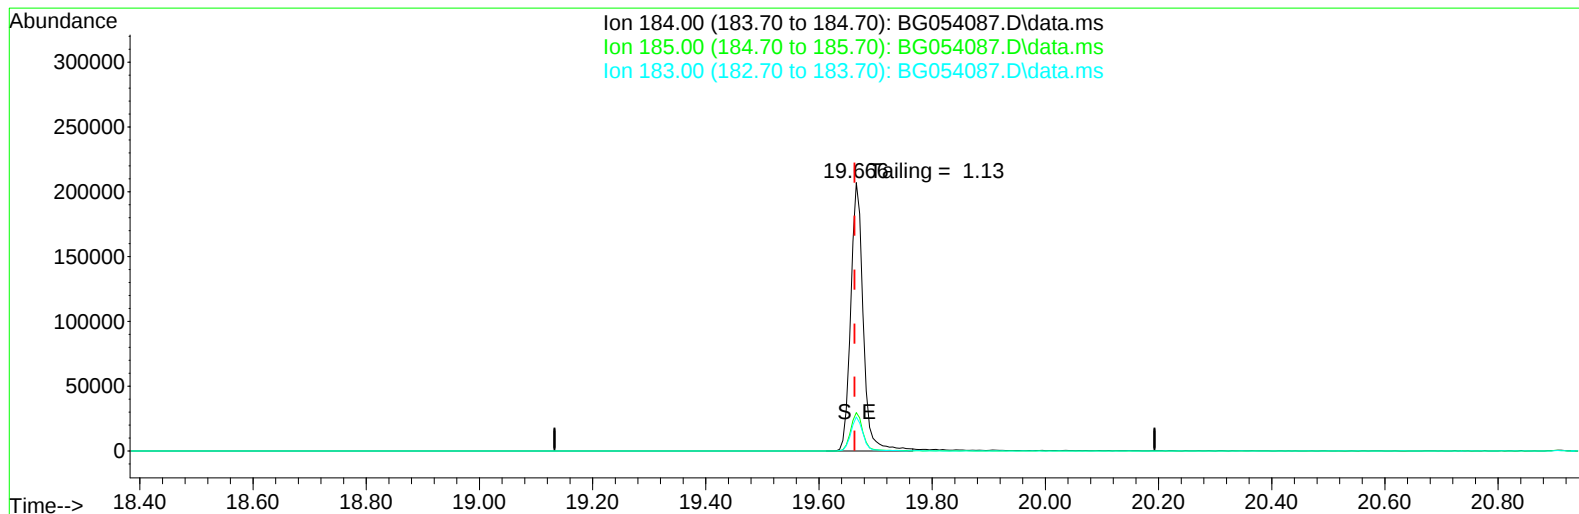

TIC: BG054087.D\data.ms

(77) Benzidine

19.666min (+ 0.003) 0.00 ng

response 319049

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.34
183.00	11.10	12.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/27/2022	BNA_G	BG054087.D
Compound Name	Response	Retention Time
DDT	185595	20.9
DDD	4547	20.45
DDE	605	19.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5152	190747	2.70

Instrument :
BNA_G
ClientSampleId :
DFTPP