
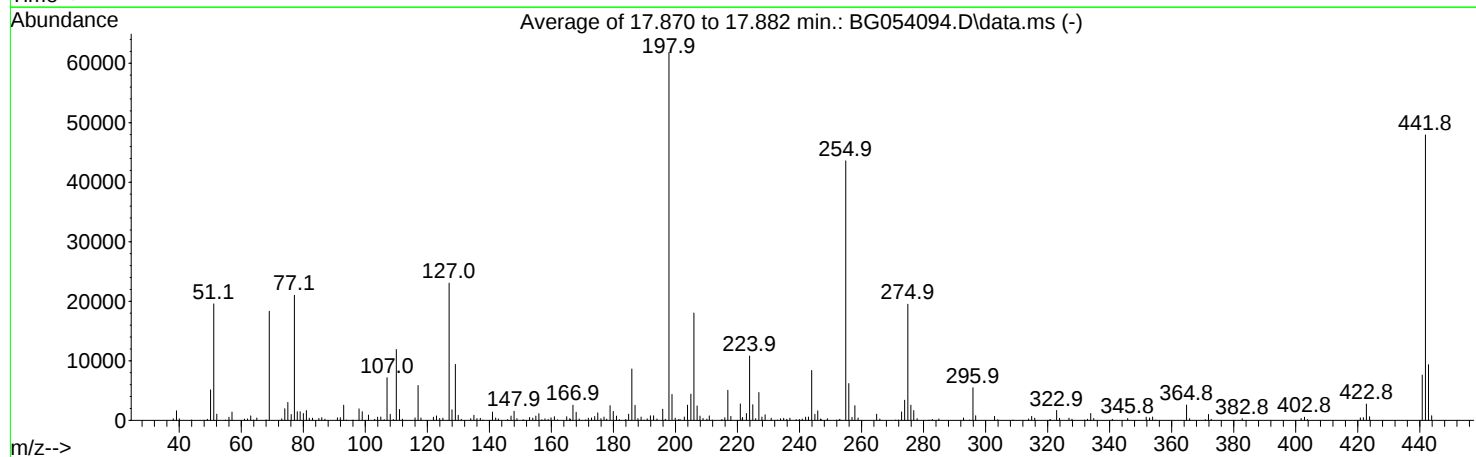


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\
Data File : BG054094.D
Acq On : 27 Jun 2022 16:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 27 00:27:54 2022

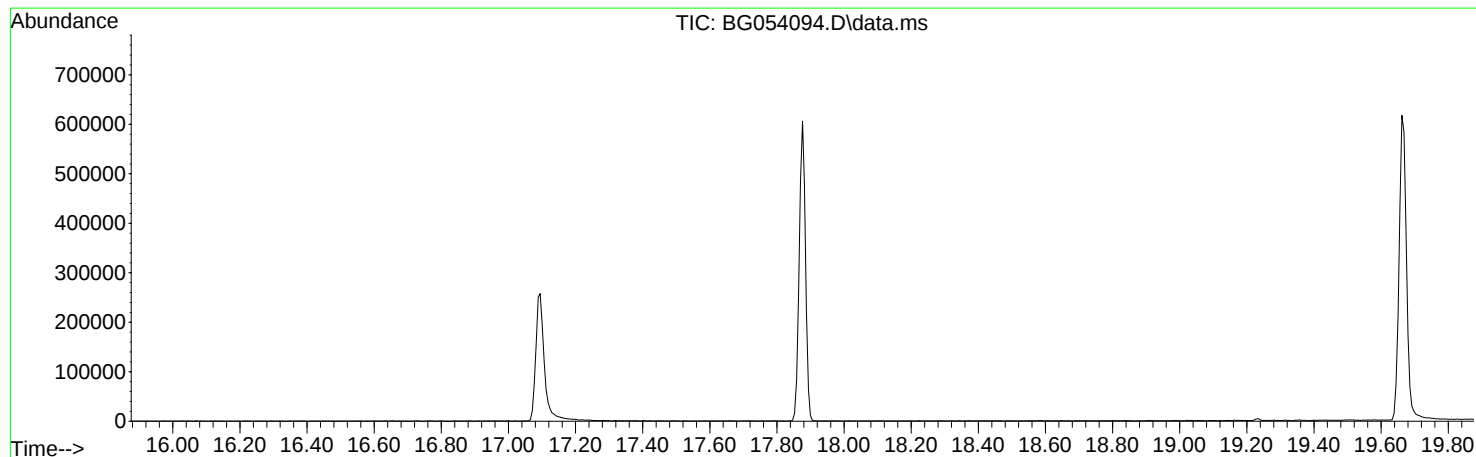




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	19565	PASS
68	69	0.00	2	0.5	92	PASS
69	198	0.00	100	29.7	18335	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.3	23067	PASS
197	198	0.00	2	0.3	188	PASS
198	198	100	100	100.0	61805	PASS
199	198	5	9	7.1	4360	PASS
275	198	10	60	31.6	19515	PASS
365	198	1	100	4.2	2595	PASS
441	198	0.01	100	12.3	7605	PASS
442	442	50	100	100.0	47955	PASS
443	442	15	24	19.5	9367	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\
Data File : BG054094.D
Acq On : 27 Jun 2022 16:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 05:14:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

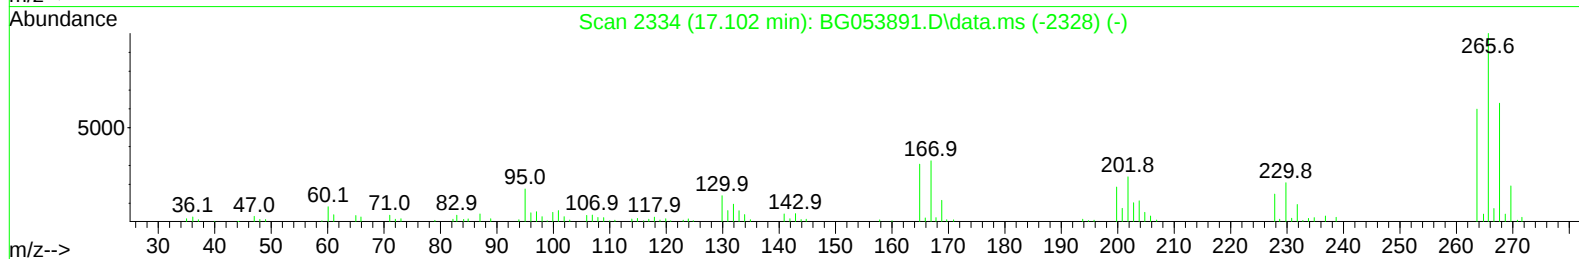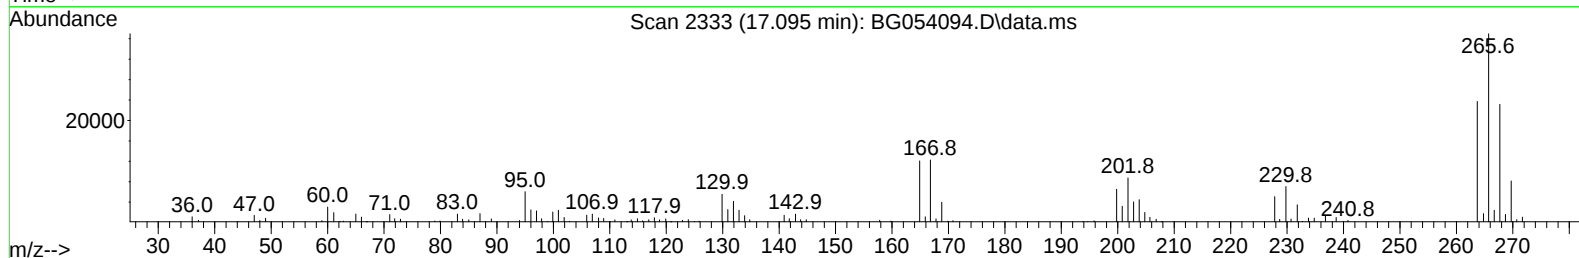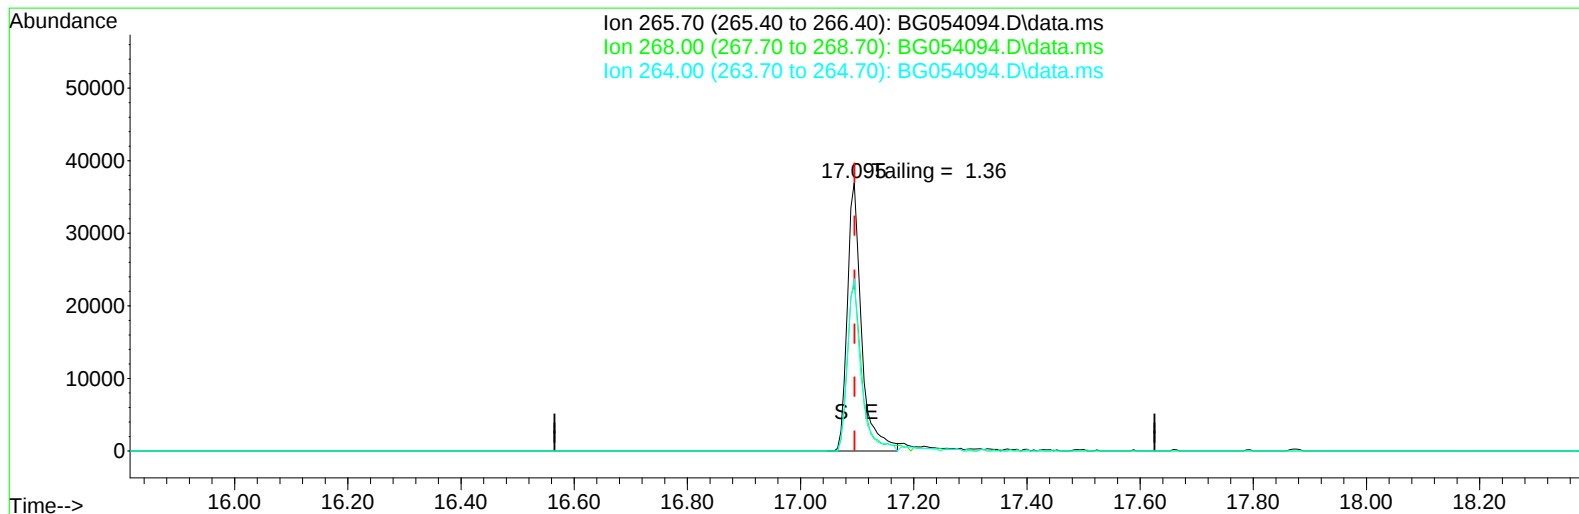

TIC: BG054094.D\data.ms

(70) Pentachlorophenol (C)

17.095min (-0.000) 31468.30 ng




response 66410

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.03
264.00	66.20	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062722\
Data File : BG054094.D
Acq On : 27 Jun 2022 16:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 05:14:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

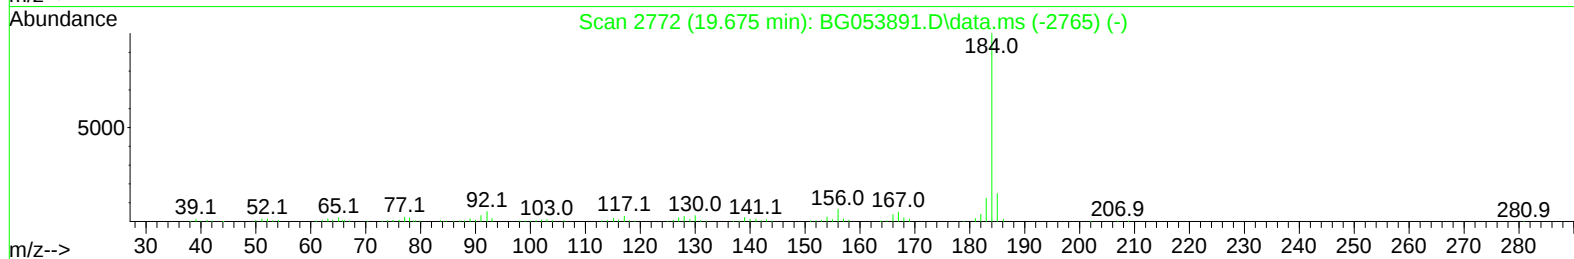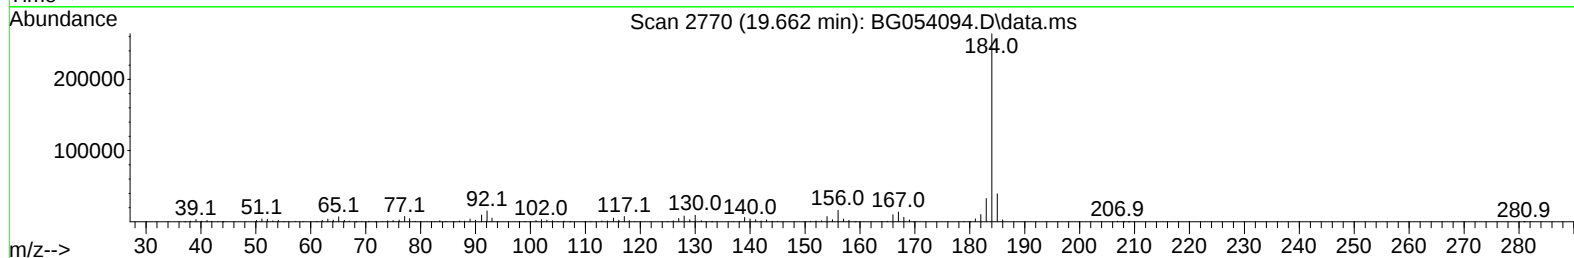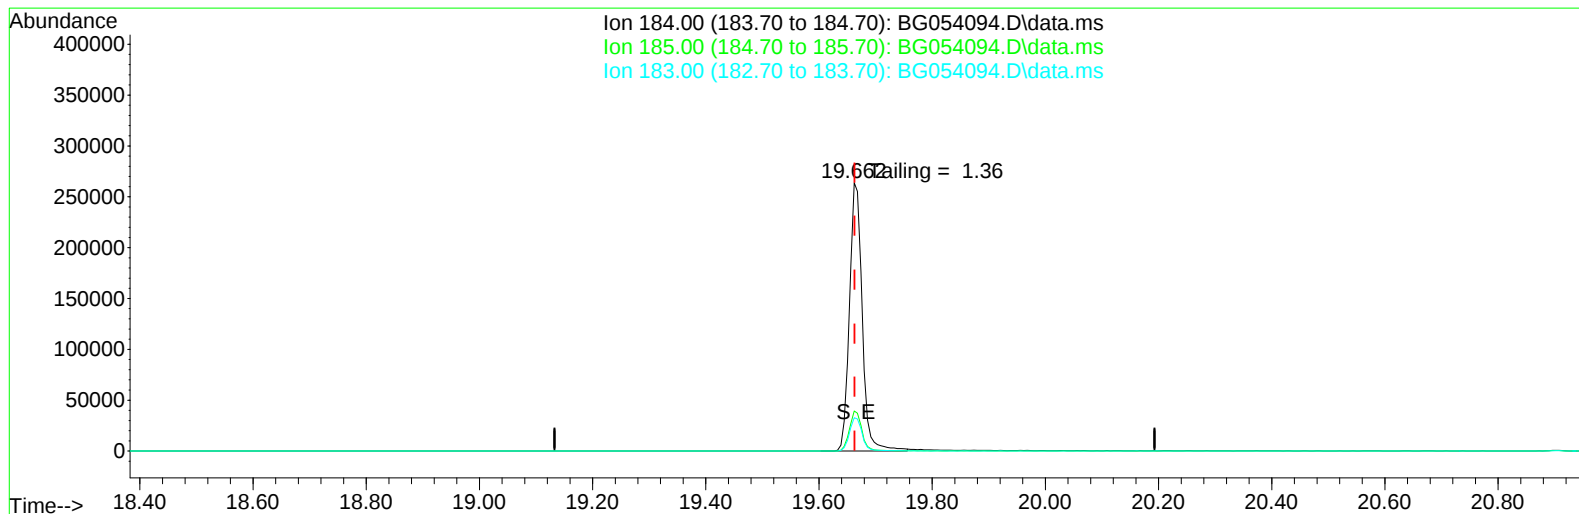

TIC: BG054094.D\data.ms

(77) Benzidine

19.662min (-0.000) 0.00 ng

response 416967

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.93
183.00	11.10	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/27/2022	BNA_G	BG054094.D
Compound Name	Response	Retention Time
DDT	225653	20.9
DDD	6076	20.46
DDE	998	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7074	232727	3.04

Instrument :
BNA_G
ClientSampleId :
DFTPP