
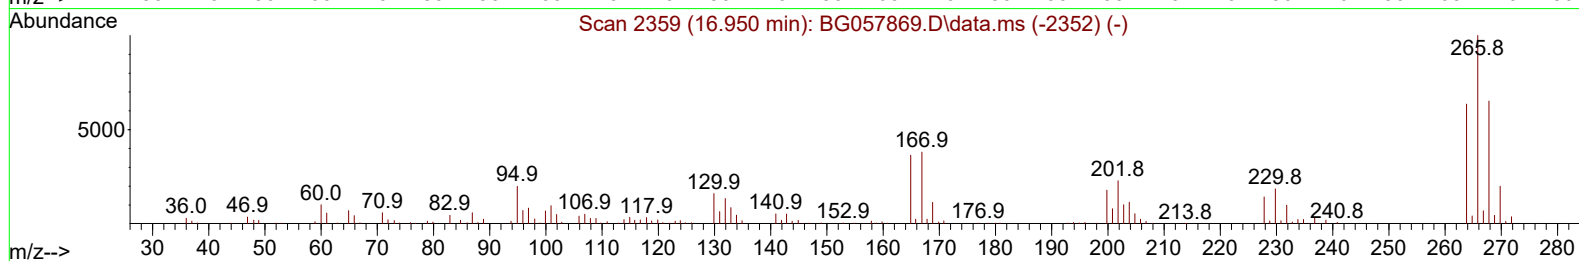
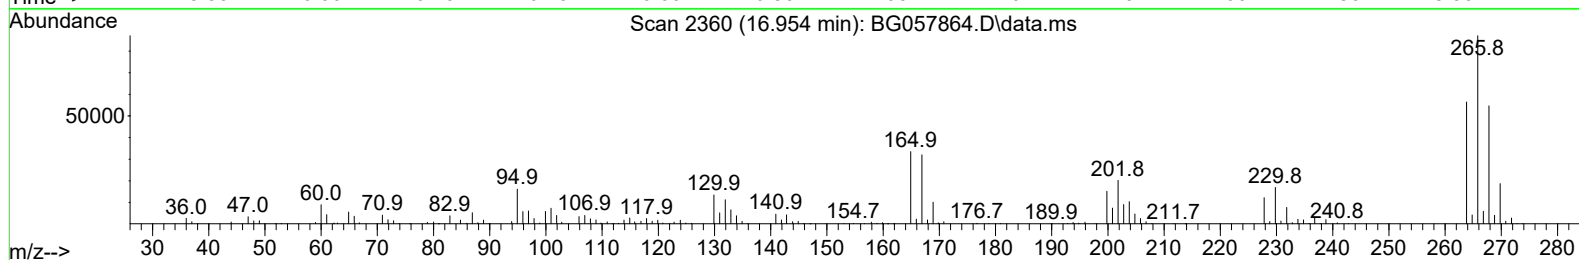


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062723\
Data File : BG057864.D
Acq On : 27 Jun 2023 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:12:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

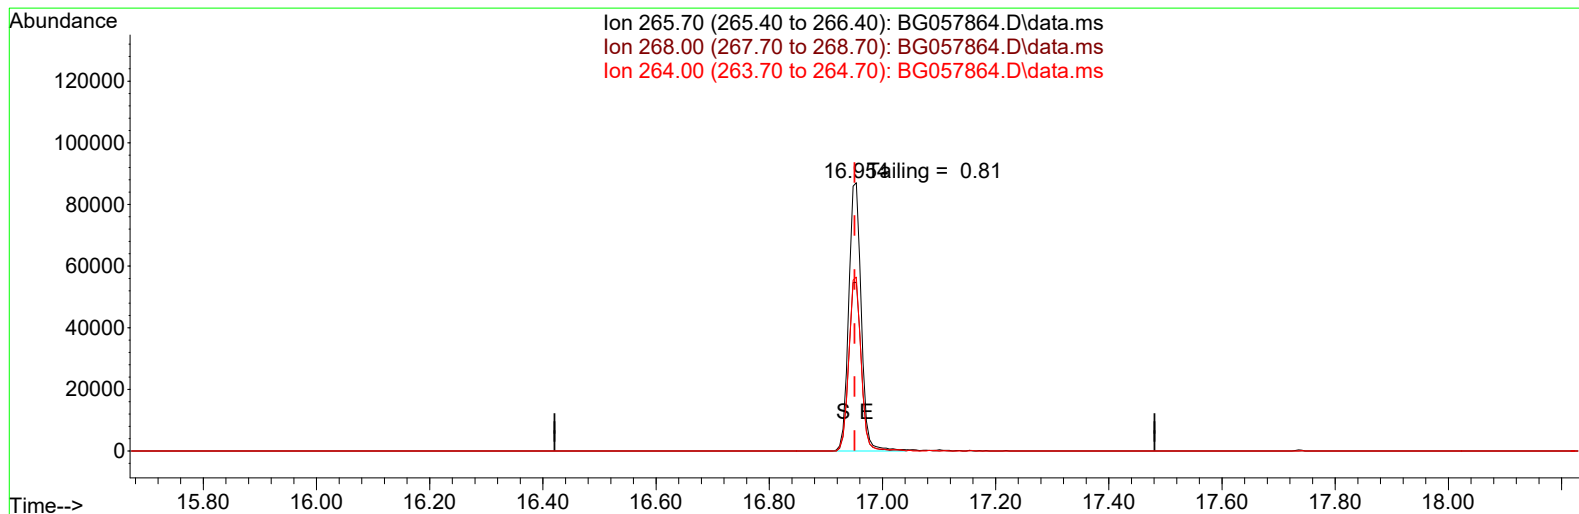

TIC: BG057864.D\data.ms

(70) Pentachlorophenol (C)




16.954min (+ 0.003) 22792.44 ng

response 134065

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.82
264.00	63.60	64.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062723\
Data File : BG057864.D
Acq On : 27 Jun 2023 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:12:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

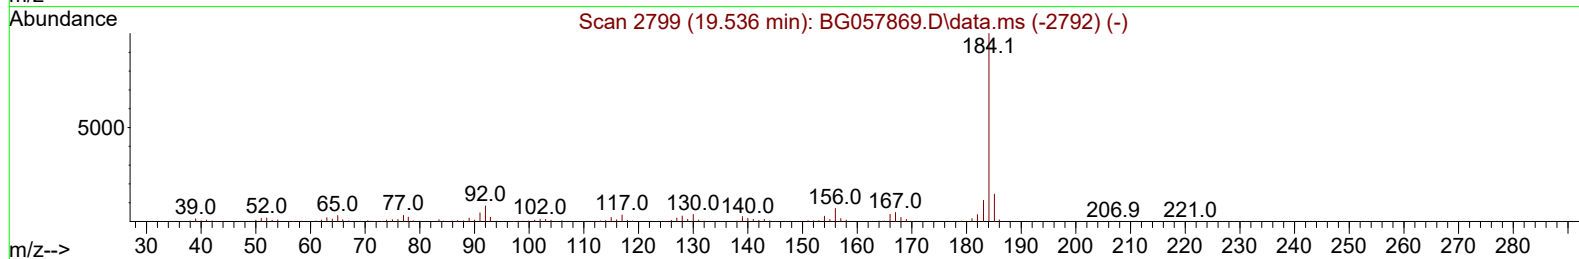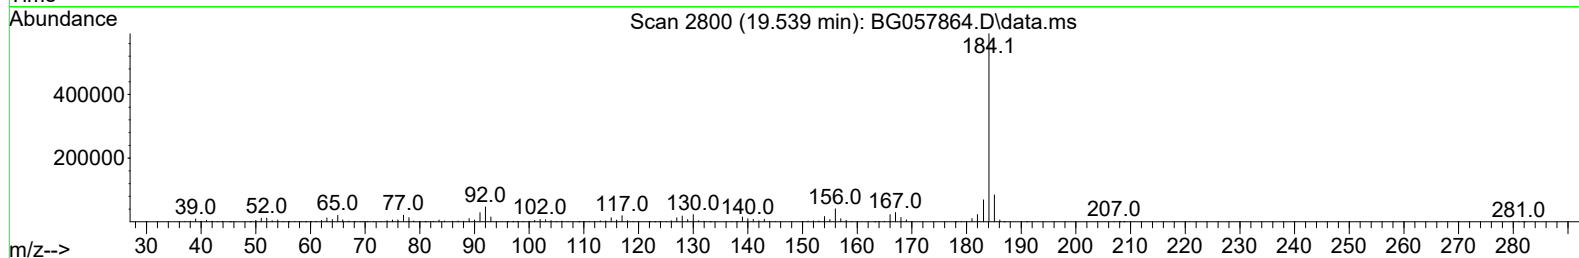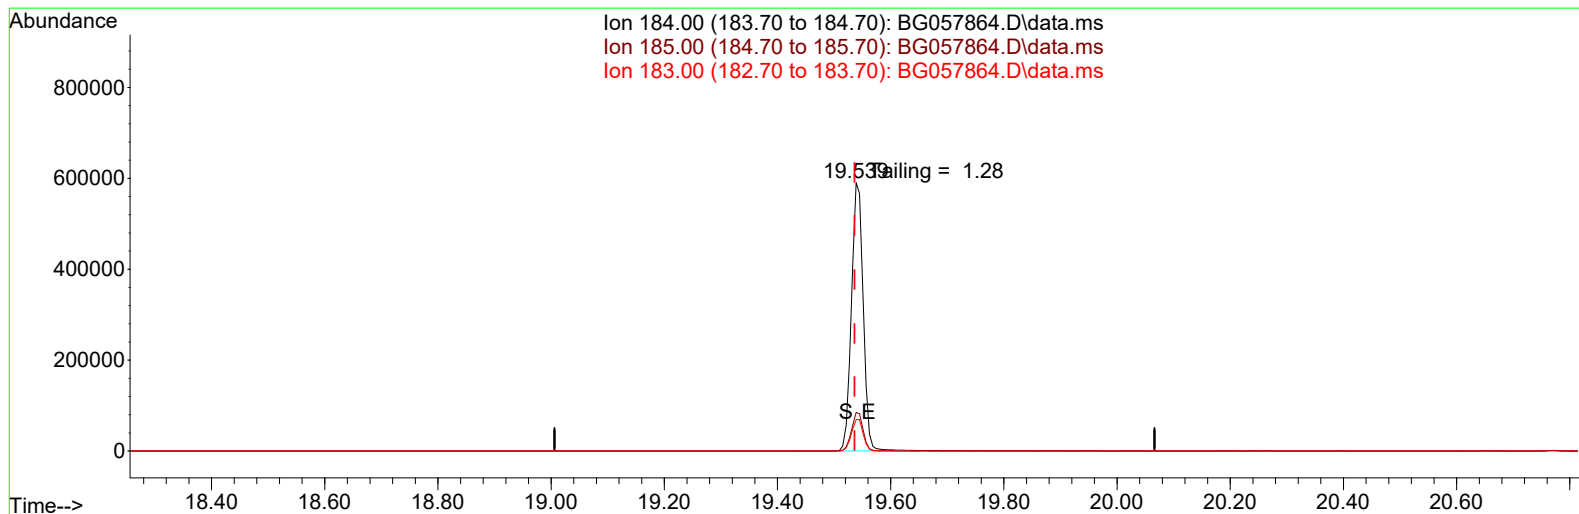

TIC: BG057864.D\data.ms

(77) Benzidine

19.539min (+ 0.003) 0.00 ng

response 854295

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	11.20	11.73
0.00	0.00	0.00