


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062723\
 Data File : BG057864.D
 Acq On : 27 Jun 2023 12:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 01:12:33 2023

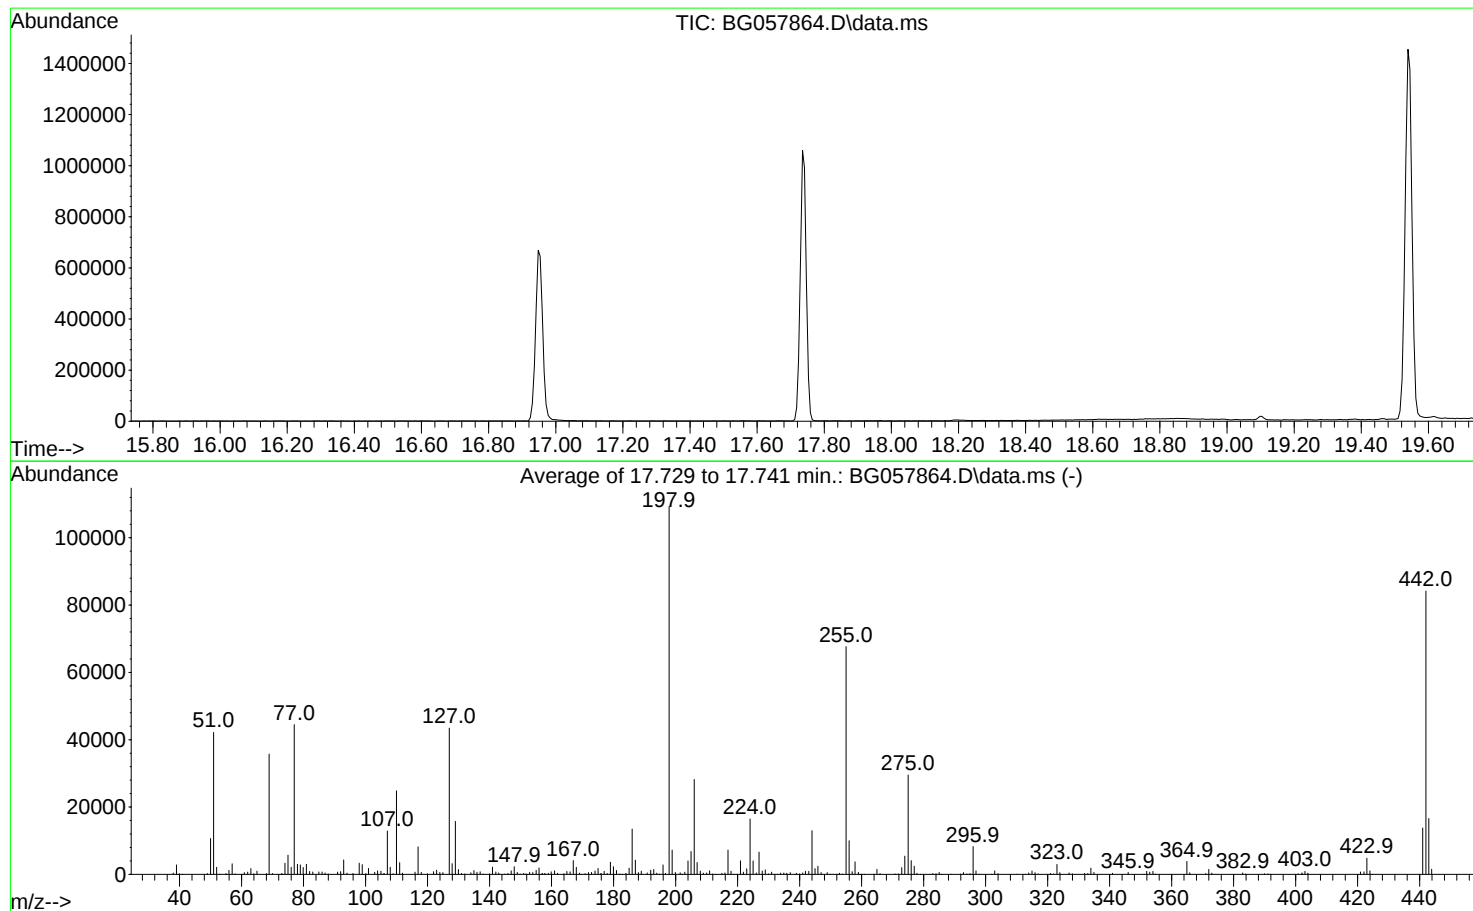

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	42187	PASS
68	69	0.00	2	0.6	224	PASS
69	198	0.00	100	32.7	35749	PASS
70	69	0.00	2	0.6	216	PASS
127	198	10	80	39.7	43424	PASS
197	198	0.00	2	0.2	269	PASS
198	198	100	100	100.0	109280	PASS
199	198	5	9	6.6	7207	PASS
275	198	10	60	27.0	29523	PASS
365	198	1	100	3.5	3838	PASS
441	198	0.01	100	12.6	13804	PASS
442	442	50	100	100.0	84205	PASS
443	442	15	24	19.7	16597	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/27/2023	BNA_G	<u>BG057864.D</u>
Compound Name	Response	Retention Time
DDT	378247	20.773
DDD	4860	20.385
DDE	0	19.823
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4860	383107	1.27

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062723\
Data File : BG057864.D
Acq On : 27 Jun 2023 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 07:12:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

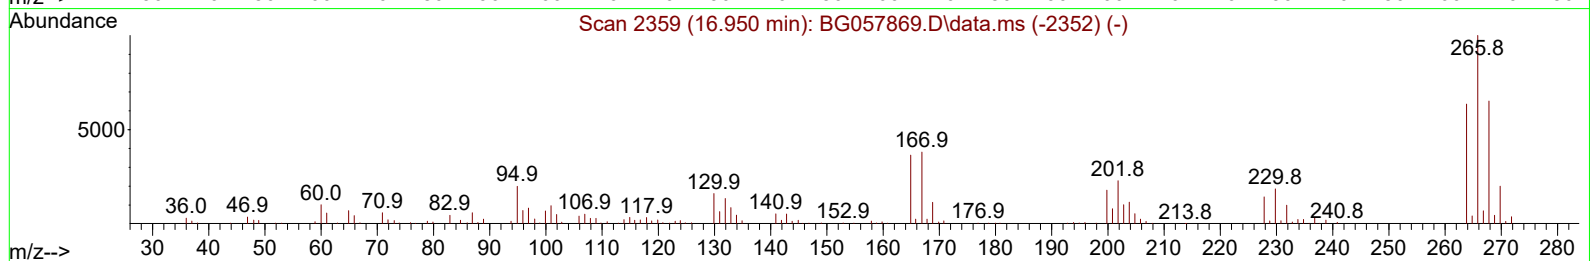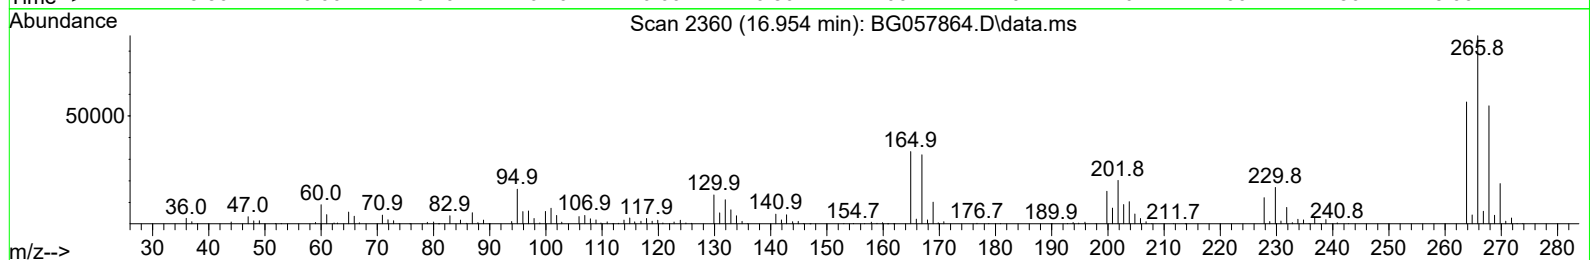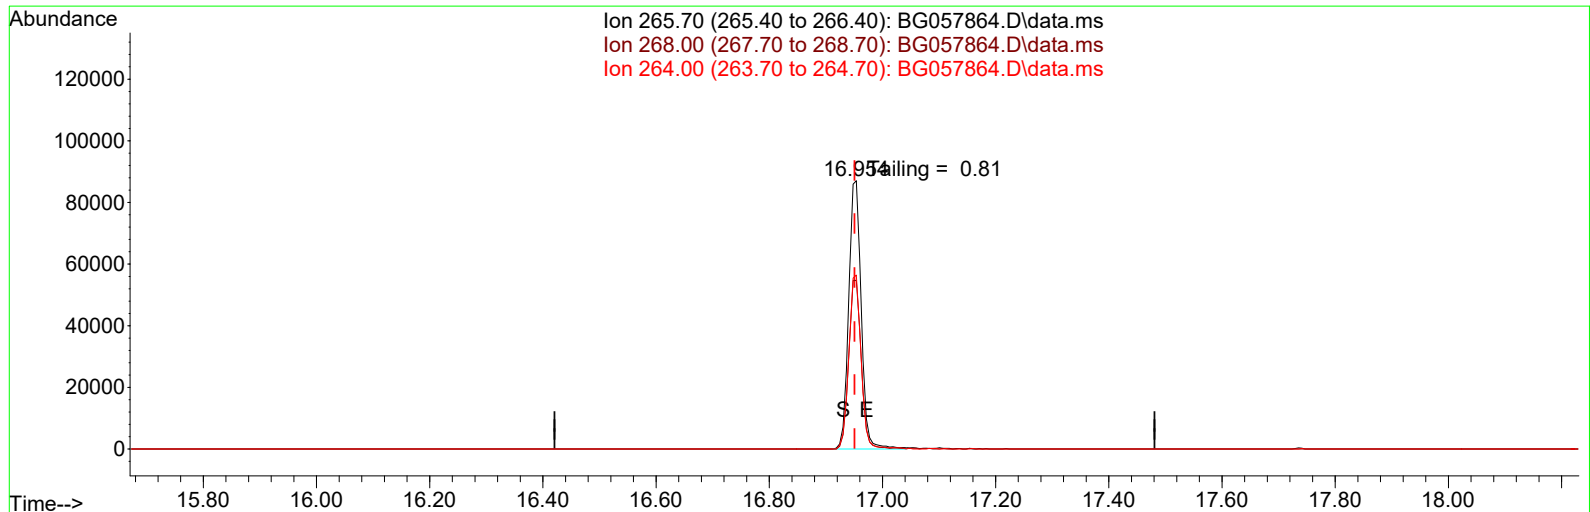

TIC: BG057864.D\data.ms

(70) Pentachlorophenol (C)

16.954min (+ 0.003) 22792.44 ng




response 134065

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.82
264.00	63.60	64.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062723\
Data File : BG057864.D
Acq On : 27 Jun 2023 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 07:12:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

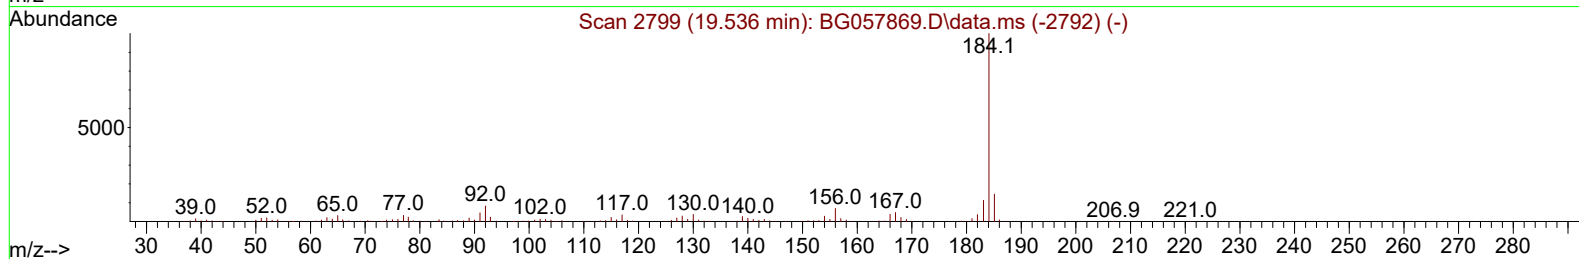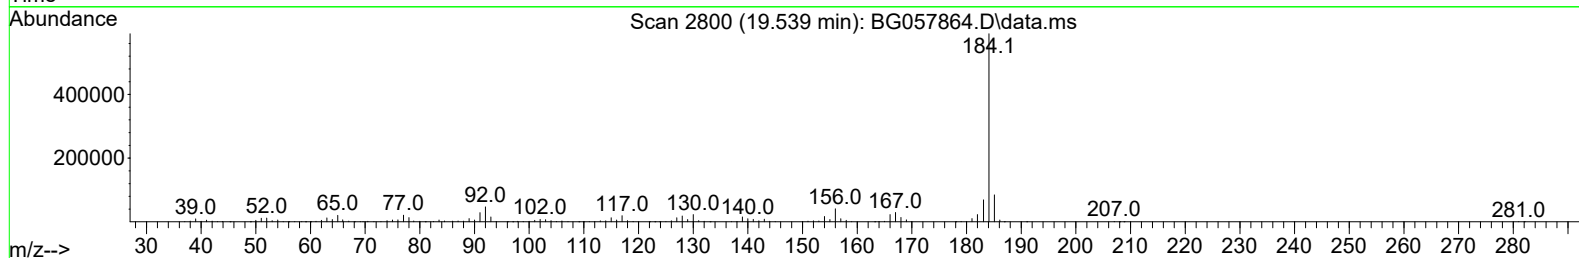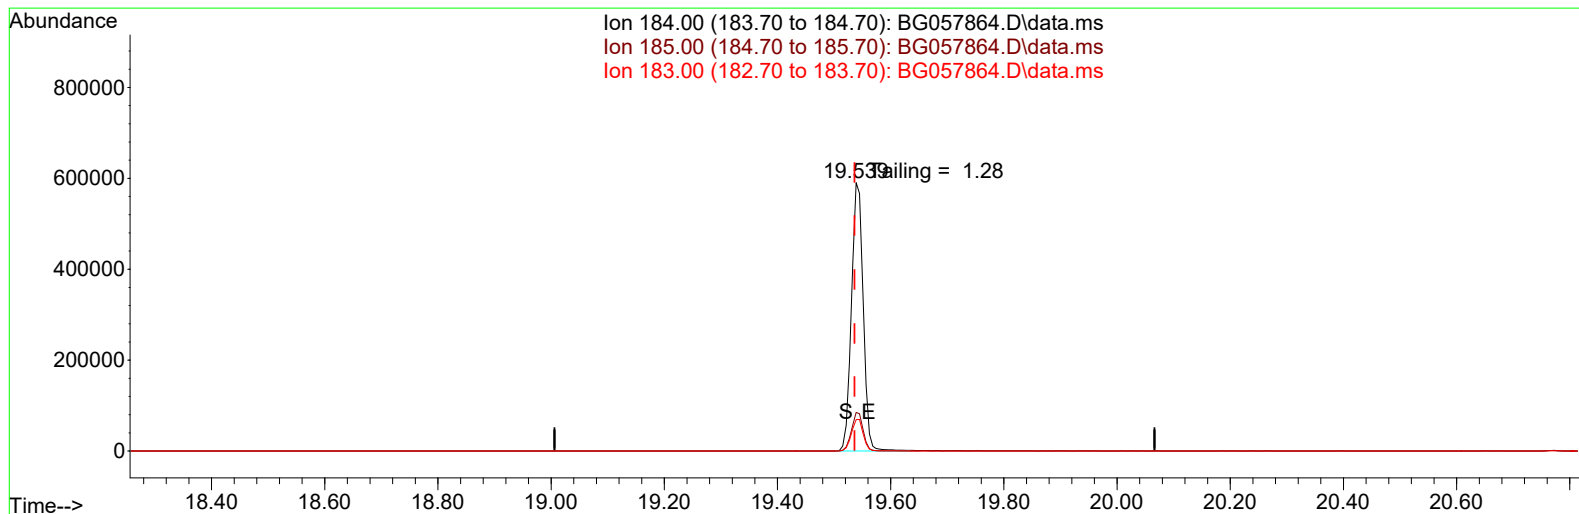

TIC: BG057864.D\data.ms

(77) Benzidine

19.539min (+ 0.003) 0.00 ng

response 854295

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	11.20	11.73
0.00	0.00	0.00