

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062818\
 Data File : BG035497.D
 Acq On : 29 Jun 2018 3:23
 Operator : JU/SJ
 Sample : J3719-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 062518-TIPC-F-D-S

Quant Time: Jun 29 04:54:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	34166	20.00	ng	-0.02
21) Naphthalene-d8	10.85	136	124605	20.00	ng	-0.03
38) Acenaphthene-d10	14.67	164	87699	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	238786	20.00	ng	-0.02
75) Chrysene-d12	21.68	240	263528	20.00	ng	-0.04
86) Perylene-d12	24.89	264	244212	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	96856	47.84	ng	-0.02
7) Phenol-d6	7.21	99	87316	29.22	ng	-0.01
23) Nitrobenzene-d5	9.22	82	320115	122.12	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	124810	111.17	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	757484	112.28	ng	-0.03
78) Terphenyl-d14	20.02	244	1336626	106.24	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062818\
Data File : BG035497.D
Acq On : 29 Jun 2018 3:23
Operator : JU/SJ
Sample : J3719-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
062518-TIPC-F-D-S

Quant Time: Jun 29 04:54:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

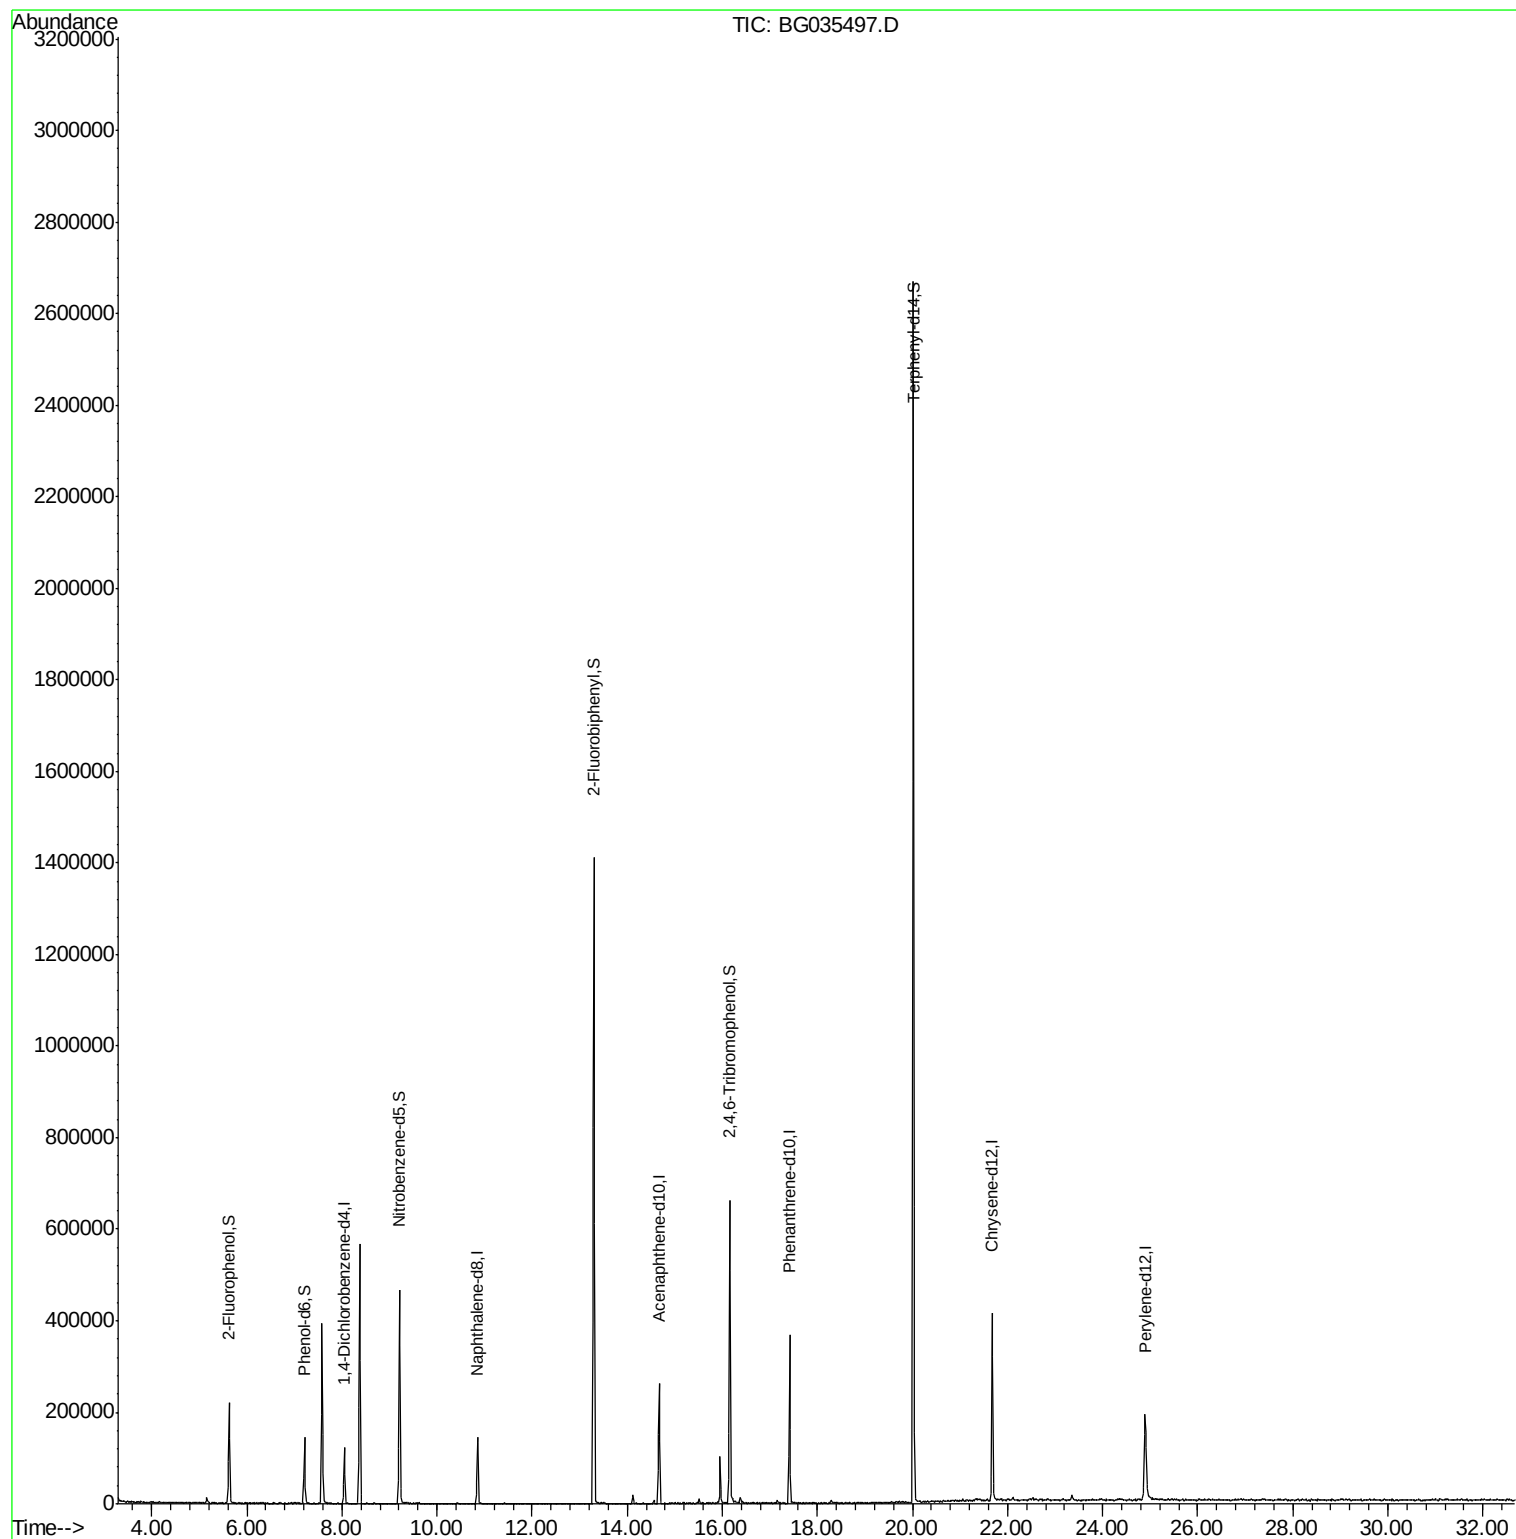

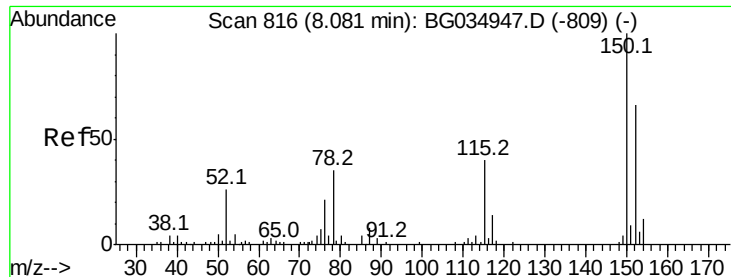


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 811
Delta R.T. -0.02 min
Lab File: BG035497.D
Acq: 29 Jun 2018 3:23

Instrument :
BNA_G
ClientSampleId :
062518-TIPC-F-D-S

Tot Ion:152 Resp: 34166
Ion Ratio Lower Upper
152 100
150 150.2 126.6 189.8
115 63.5 53.0 79.4

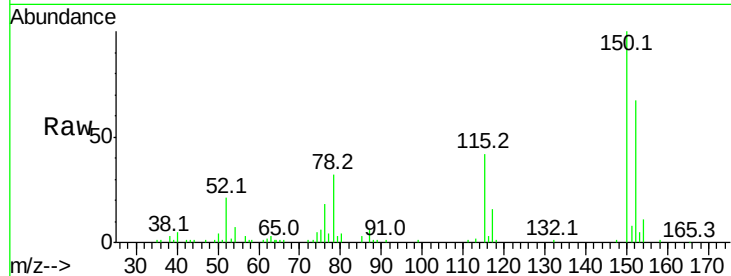


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

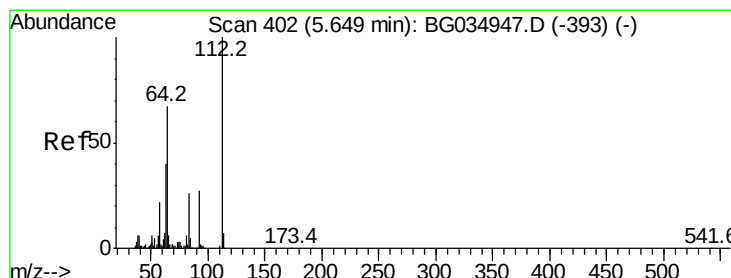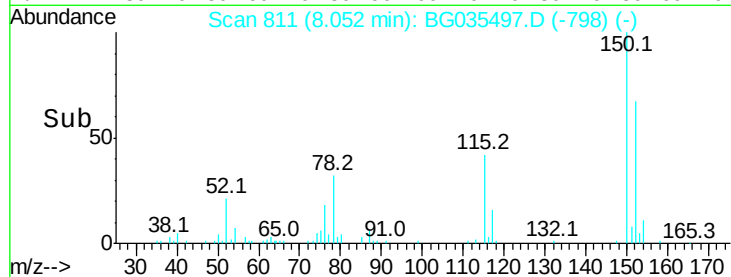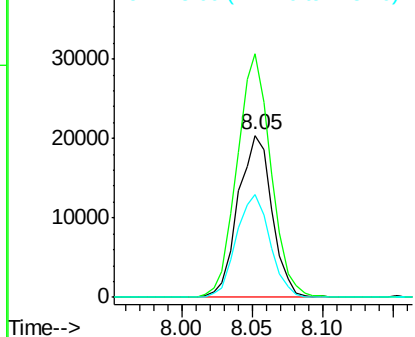



#5


2-Fluorophenol
Concen: 47.841 ng
RT: 5.63 min Scan# 398
Delta R.T. -0.02 min
Lab File: BG035497.D
Acq: 29 Jun 2018 3:23

Tgt Ion:112 Resp: 96856
Ion Ratio Lower Upper
112 100
64 63.4 56.3 84.5
63 37.2 30.1 45.1

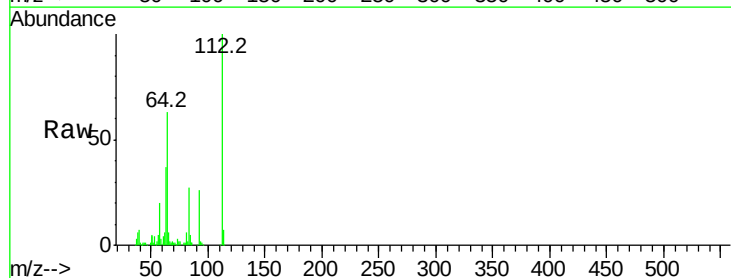

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

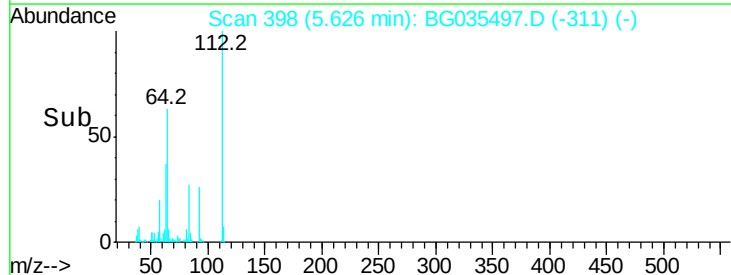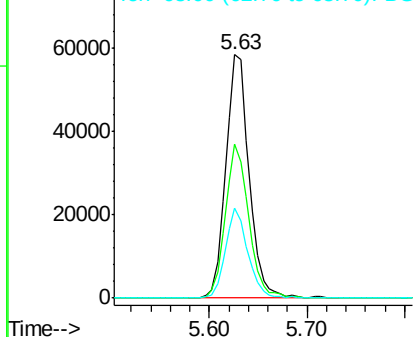

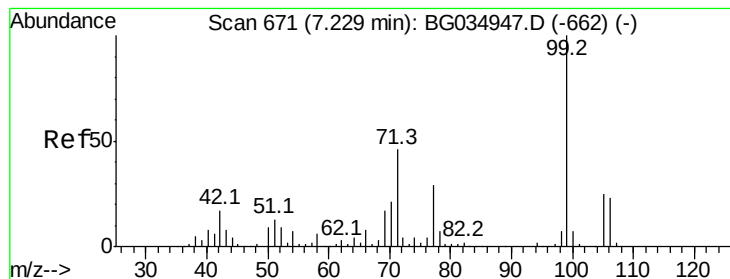

#7

Phenol-d6

Concen: 29.221 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23

Instrument :

BNA_G

ClientSampleId :

062518-TIPC-F-D-S


Tot Ion: 99 Resp: 87316

Ion Ratio Lower Upper




99 100

42 14.2 14.1 21.1

71 41.1 26.1 39.1#

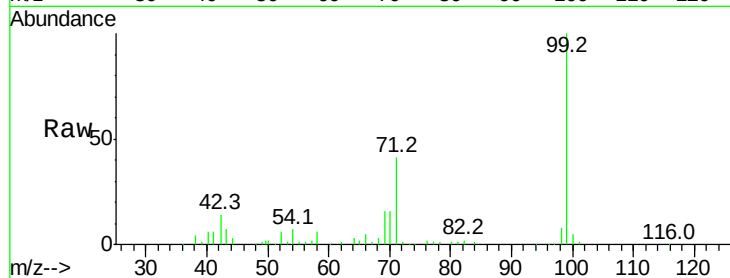

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

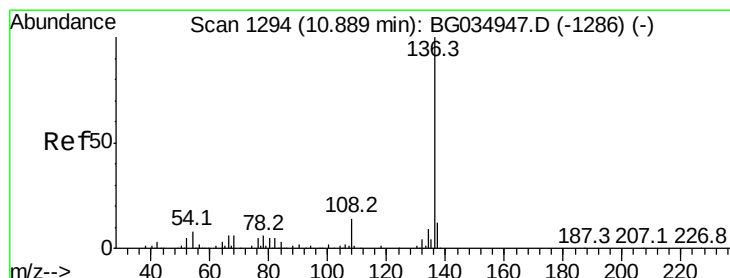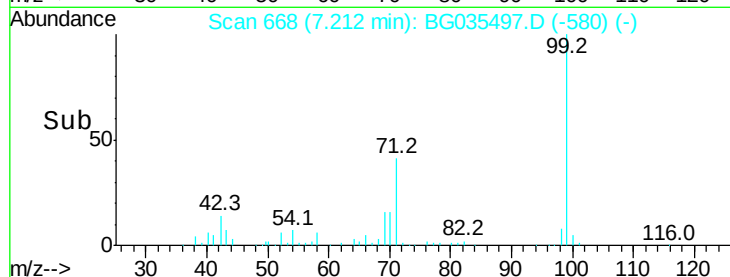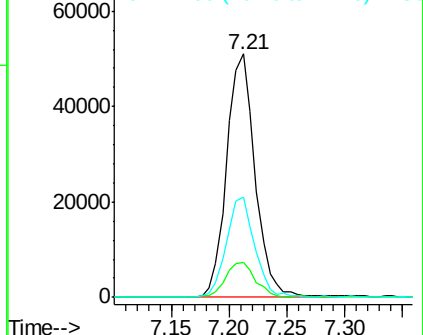

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1288

Delta R.T. -0.03 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23

Tgt Ion: 136 Resp: 124605


Ion Ratio Lower Upper

136 100



137 11.5 9.2 13.8


54 6.3 10.3 15.5#

68 3.9 4.5 6.7#

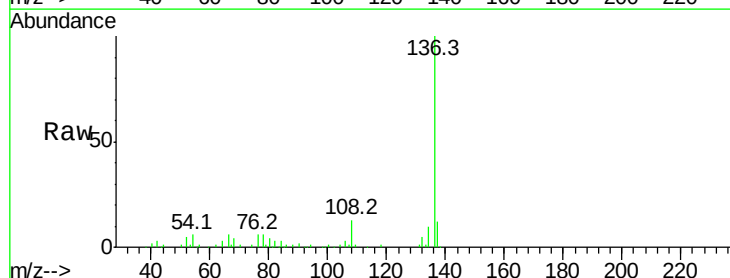

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

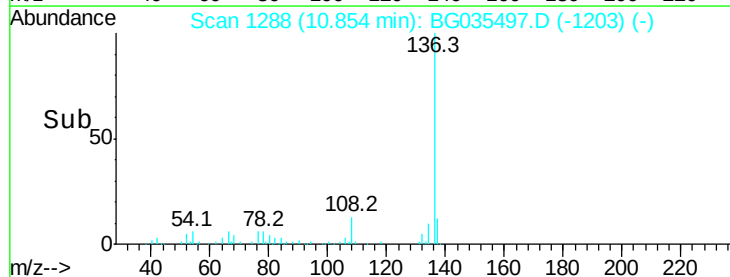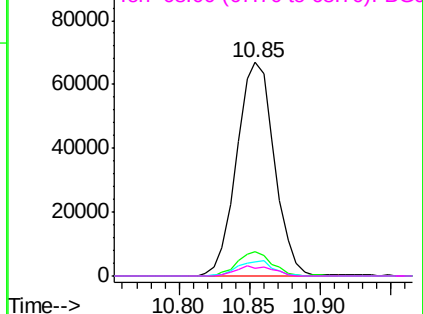

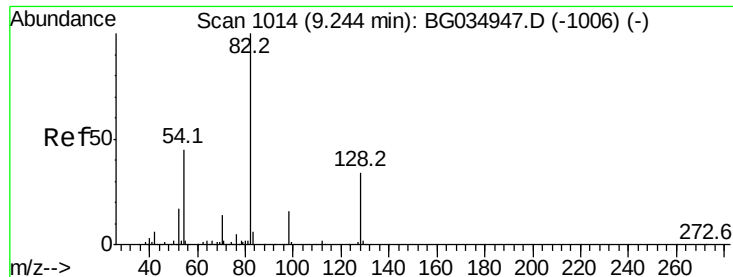

#23

Nitrobenzene-d5

Concen: 122.118 ng

RT: 9.22 min Scan# 1009

Delta R.T. -0.02 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23

Instrument :

BNA_G

ClientSampleId :

062518-TIPC-F-D-S


Tot Ion: 82 Resp: 320115

Ion Ratio Lower Upper

82 100

128 34.6 29.7 44.5




54 42.1 43.1 64.7#

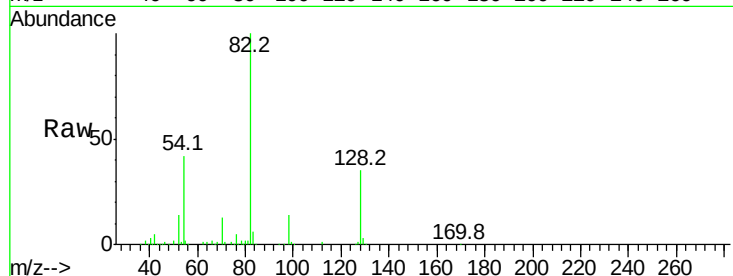

Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

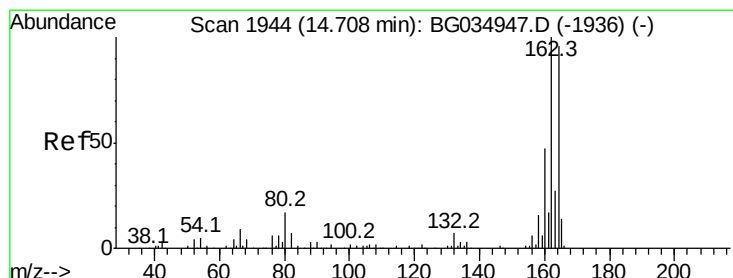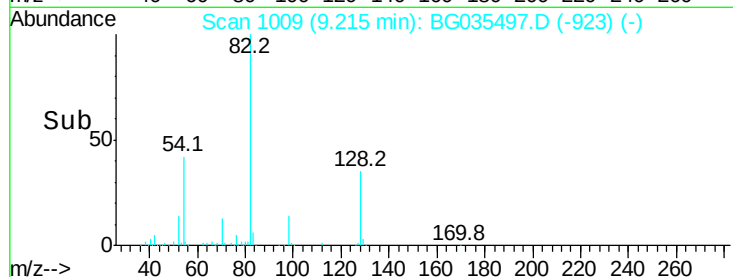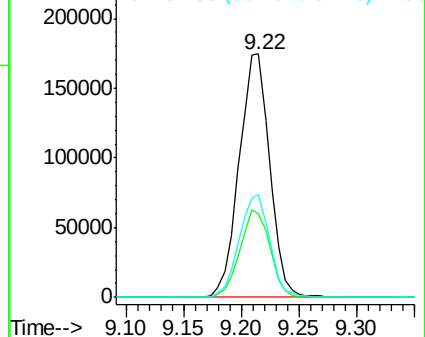

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1938

Delta R.T. -0.02 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23


Tgt Ion:164 Resp: 87699

Ion Ratio Lower Upper

164 100

162 108.0 78.8 118.2



160 46.9 35.4 53.0

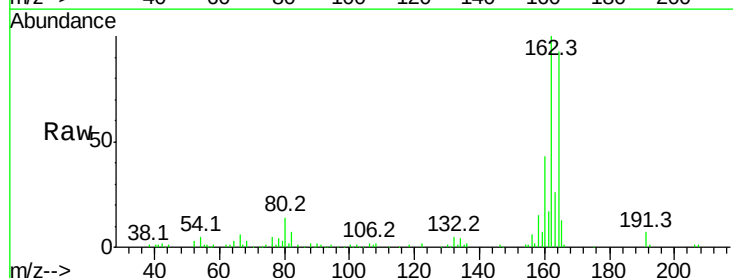


Abundance Ion 164.00 (163.70 to 164.70): BGC

Ion 162.00 (161.70 to 162.70): BGC

Ion 160.00 (159.70 to 160.70): BGC

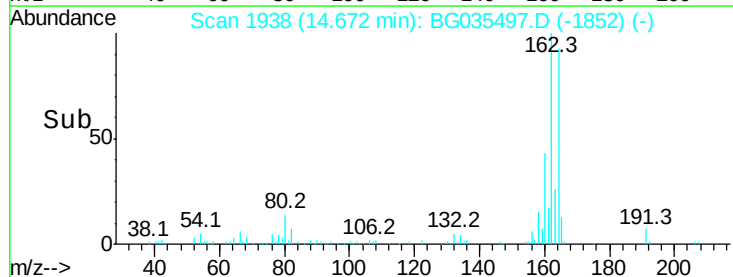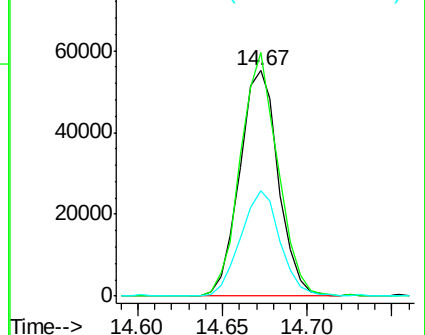


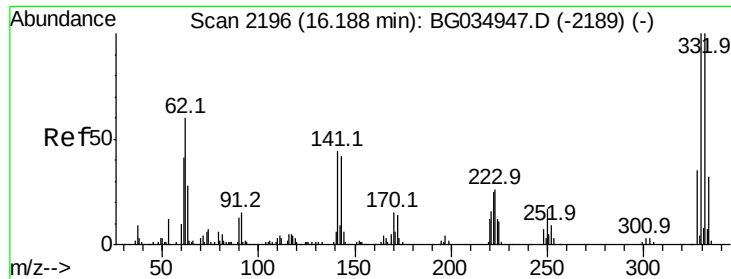




#41
 2,4,6-Tribromophenol
 Concen: 111.174 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.02 min
 Lab File: BG035497.D
 Acq: 29 Jun 2018 3:23

Instrument :
 BNA_G
 ClientSampleId :
 062518-TIPC-F-D-S

Tot Ion:330 Resp: 124810
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.0 115.6
 141 38.1 25.2 37.8#

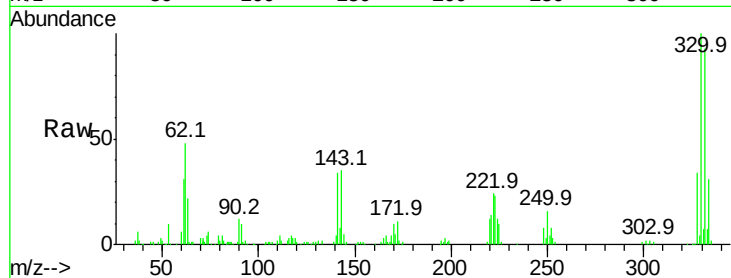


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

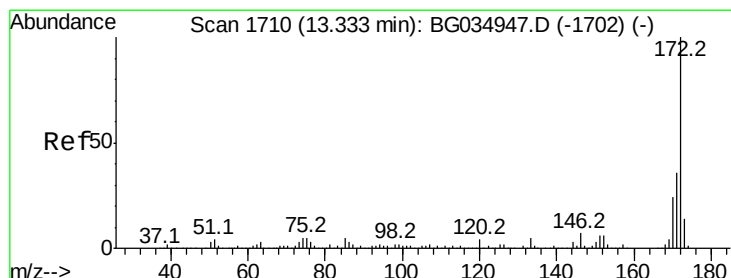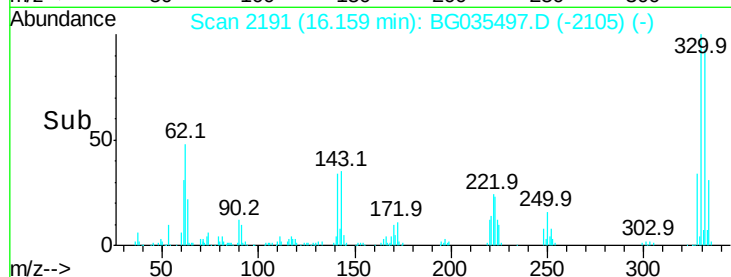
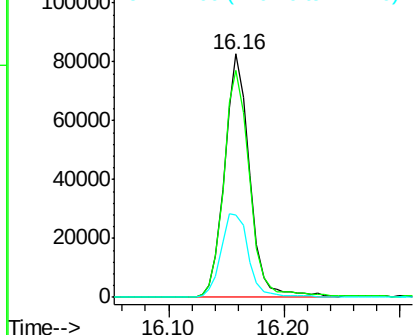



#44
 2-Fluorobiphenyl
 Concen: 112.285 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.03 min
 Lab File: BG035497.D
 Acq: 29 Jun 2018 3:23

Tgt Ion:172 Resp: 757484
 Ion Ratio Lower Upper
 172 100
 171 34.1 30.0 45.0
 170 23.4 19.5 29.3

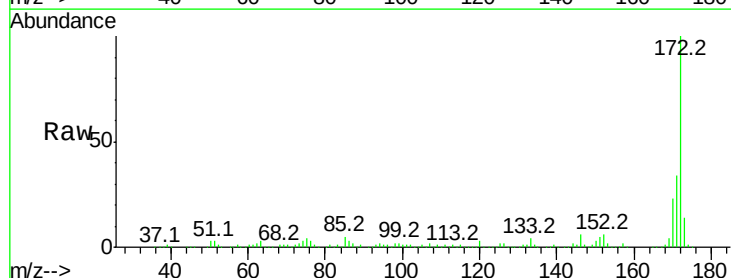

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

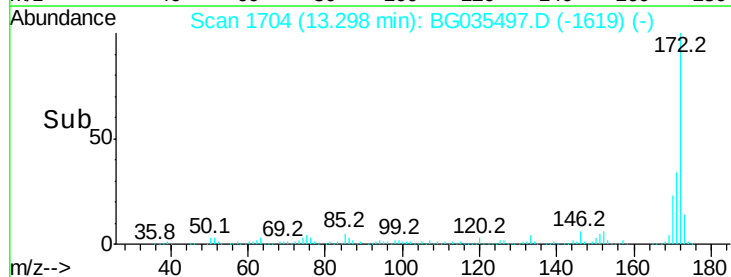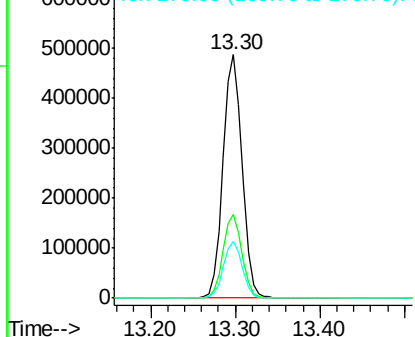

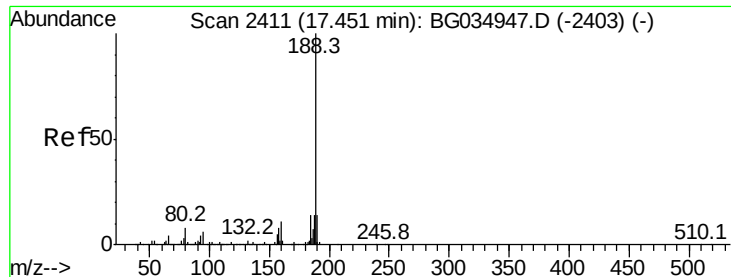

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2405

Delta R.T. -0.02 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23

Instrument :

BNA_G

ClientSampleId :

062518-TIPC-F-D-S


Tot Ion:188 Resp: 238786

Ion Ratio Lower Upper

188 100

94 5.0 6.9 10.3#




80 6.7 7.7 11.5#

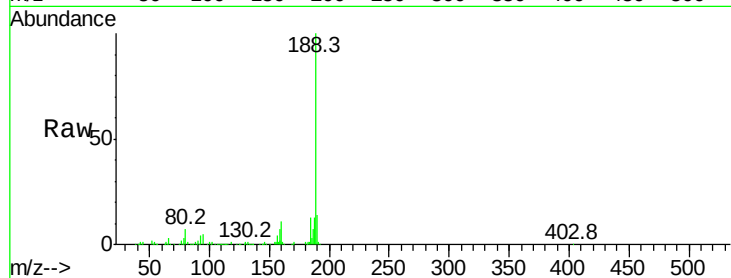

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

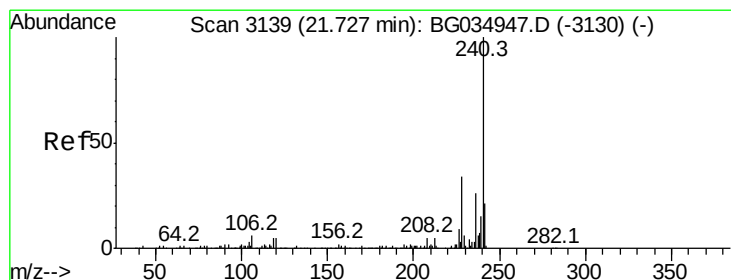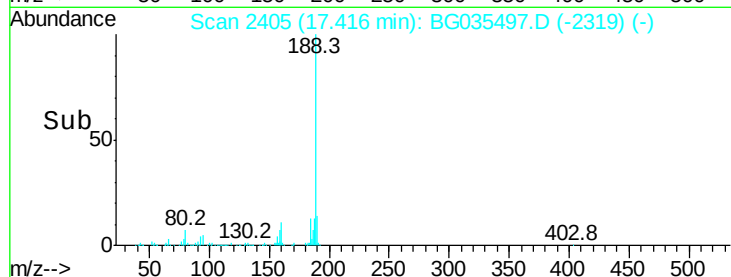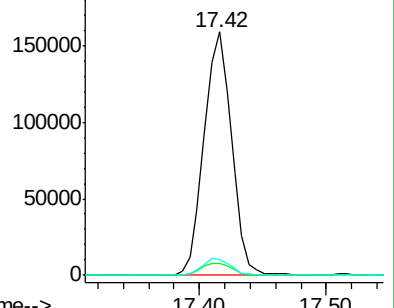

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3131

Delta R.T. -0.04 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23


Tgt Ion:240 Resp: 263528

Ion Ratio Lower Upper

240 100

120 5.0 6.8 10.2#



236 25.0 20.9 31.3

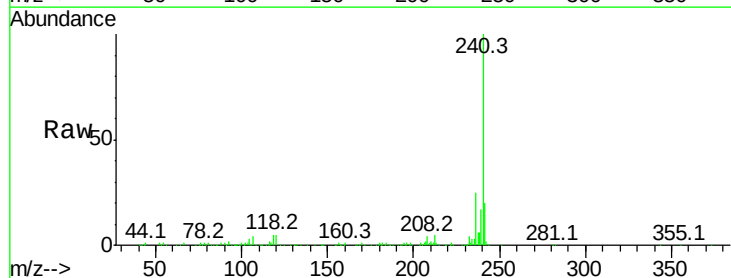


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

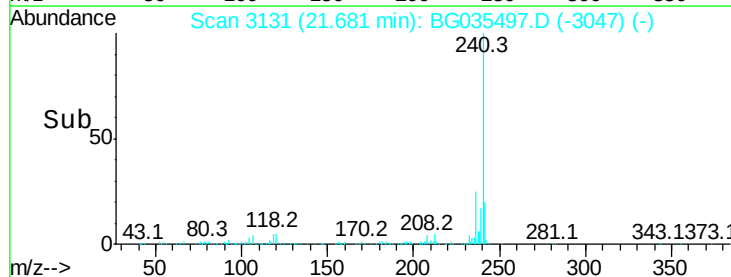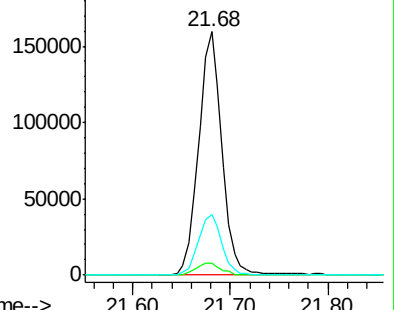

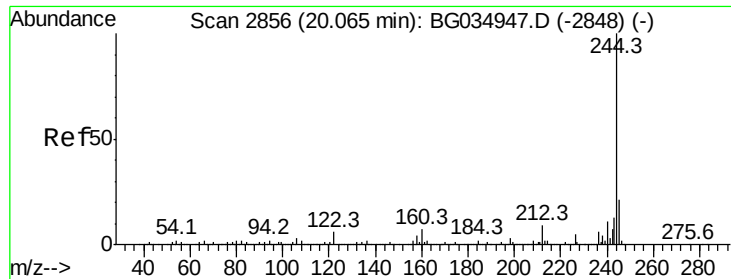

#78

Terphenyl-d14

Concen: 106.243 ng

RT: 20.02 min Scan# 2849

Delta R.T. -0.02 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23

Instrument :

BNA_G

ClientSampleId :

062518-TIPC-F-D-S


Tot Ion:244 Resp: 1336626

Ion Ratio Lower Upper

244 100

212 9.0 5.8 8.8#




122 6.2 7.0 10.4#

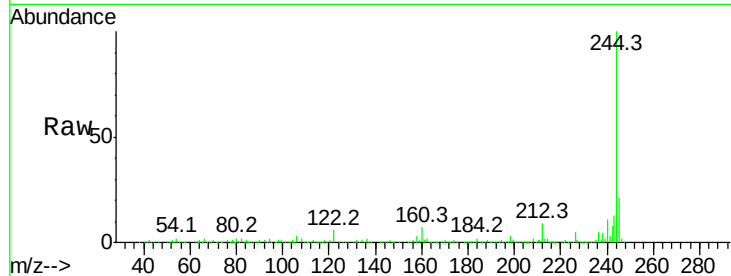

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

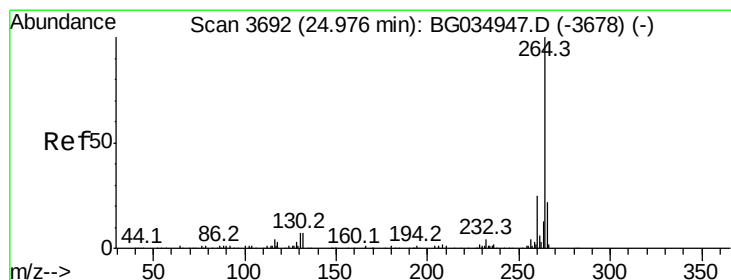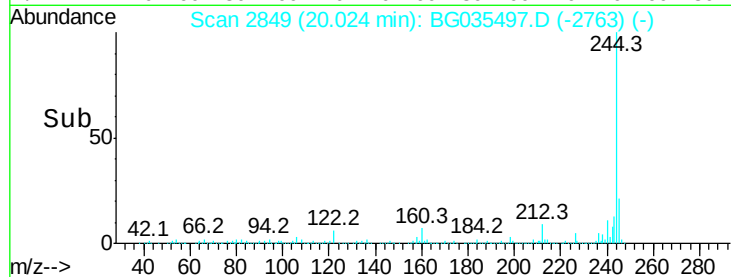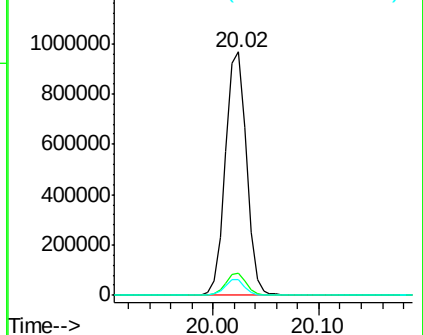

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.89 min Scan# 3678

Delta R.T. -0.06 min

Lab File: BG035497.D

Acq: 29 Jun 2018 3:23


Tgt Ion:264 Resp: 244212

Ion Ratio Lower Upper

264 100

260 21.0 17.4 26.0

265 19.2 17.7 26.5

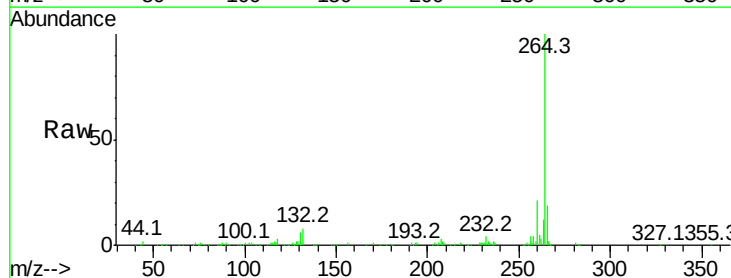

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

